

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002857.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 14:56
Operator : AJ\SJ
Sample : J5770-13 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A

Integration File: autoint1.e
Quant Time: Dec 01 01:27:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	975159	12.483 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002857.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 14:56
Operator : AJ\SJ
Sample : J5770-13 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A

Integration File: autoint1.e
Quant Time: Dec 01 01:27:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

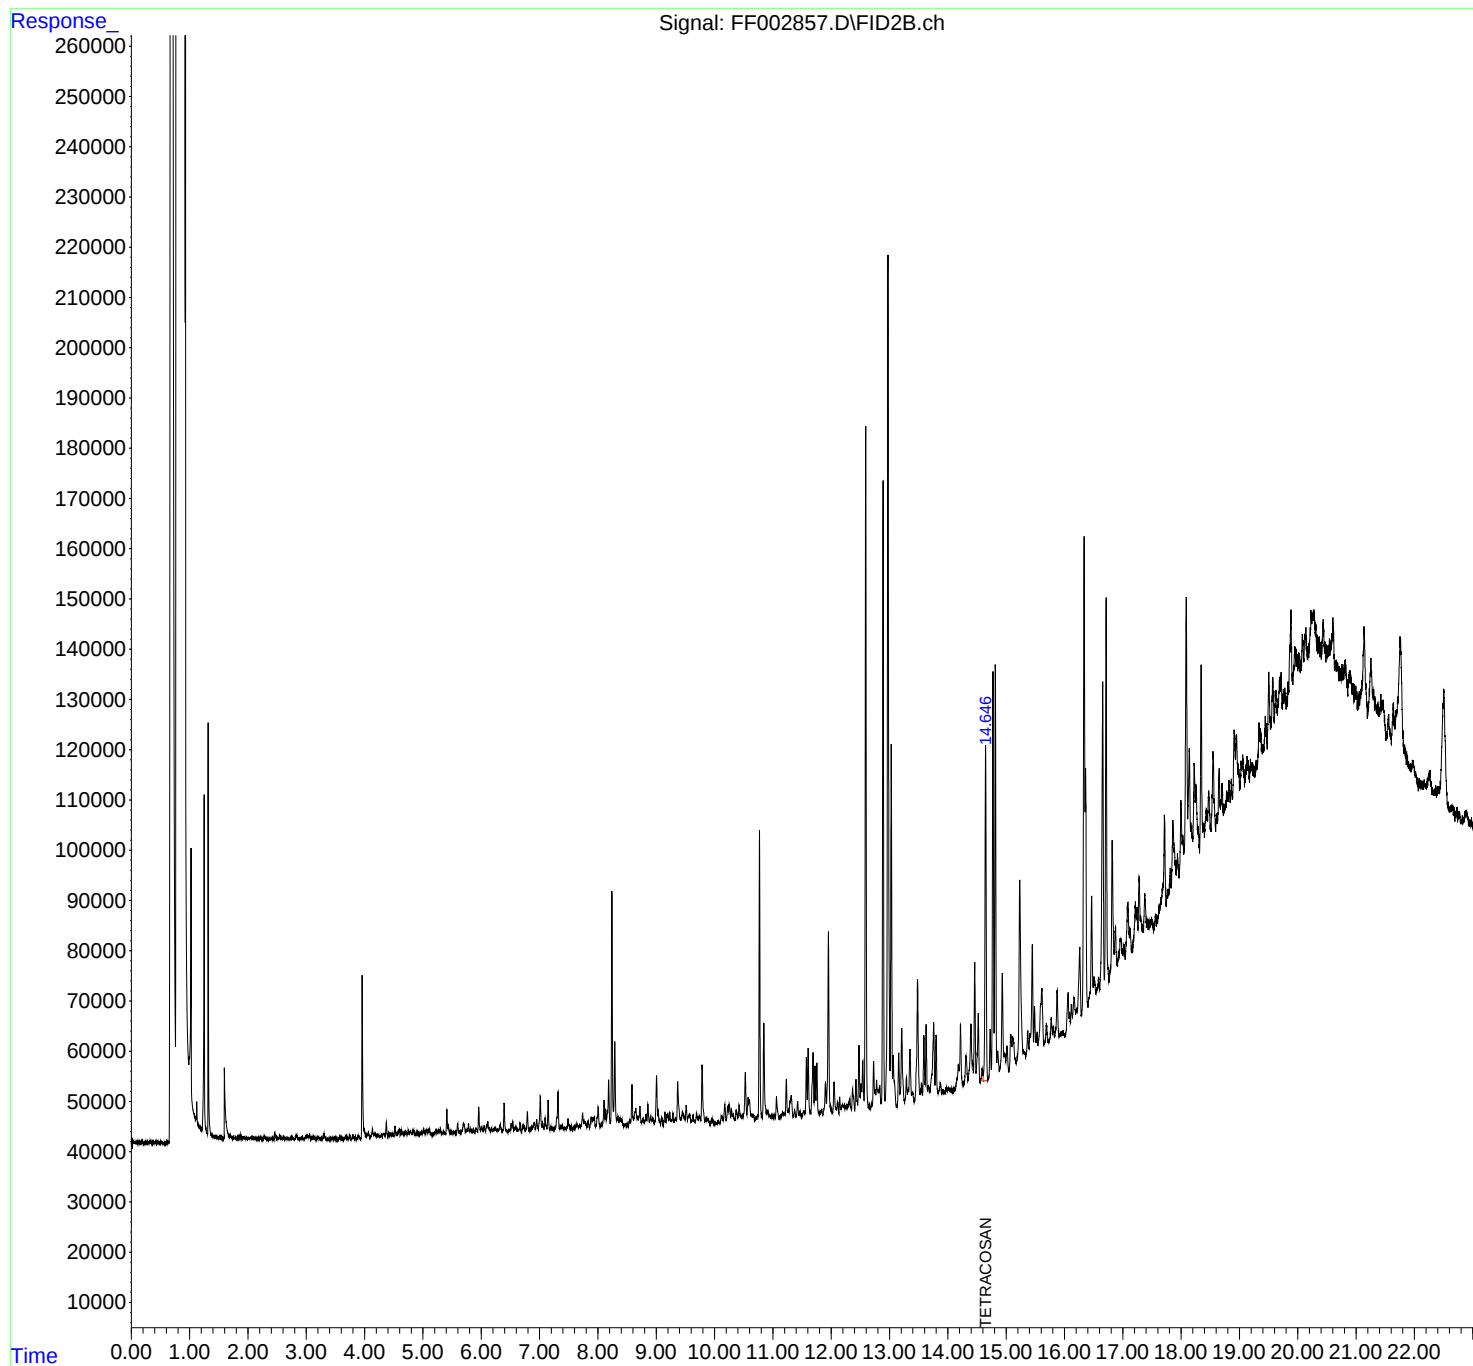

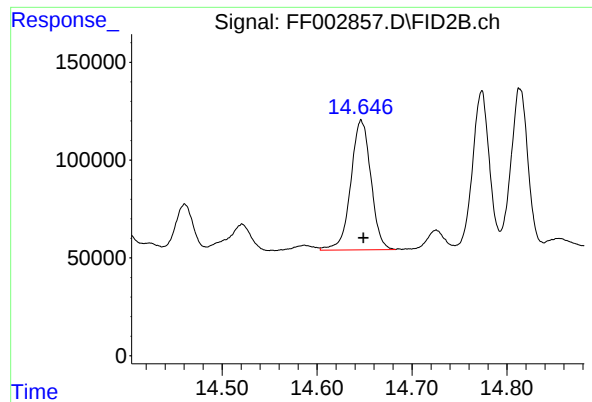

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 975159
Conc: 12.48 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A