

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120220\
 Data File : FF007923.D
 Signal(s) : FID2B.ch
 Acq On : 02 Dec 2020 19:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 03 00:34:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
 Quant Title :
 QLast Update : Thu Dec 03 00:32:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.710	2593885	20.517 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.623	247977	2.237 ug/ml
16) N-HEXATRIACONTANE	20.177	719045	11.445 ug/ml
18) N-TETRACONTANE	21.865	1114893	19.878 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120220\
Data File : FF007923.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2020 19:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 03 00:34:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120220.M
Quant Title :
QLast Update : Thu Dec 03 00:32:34 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

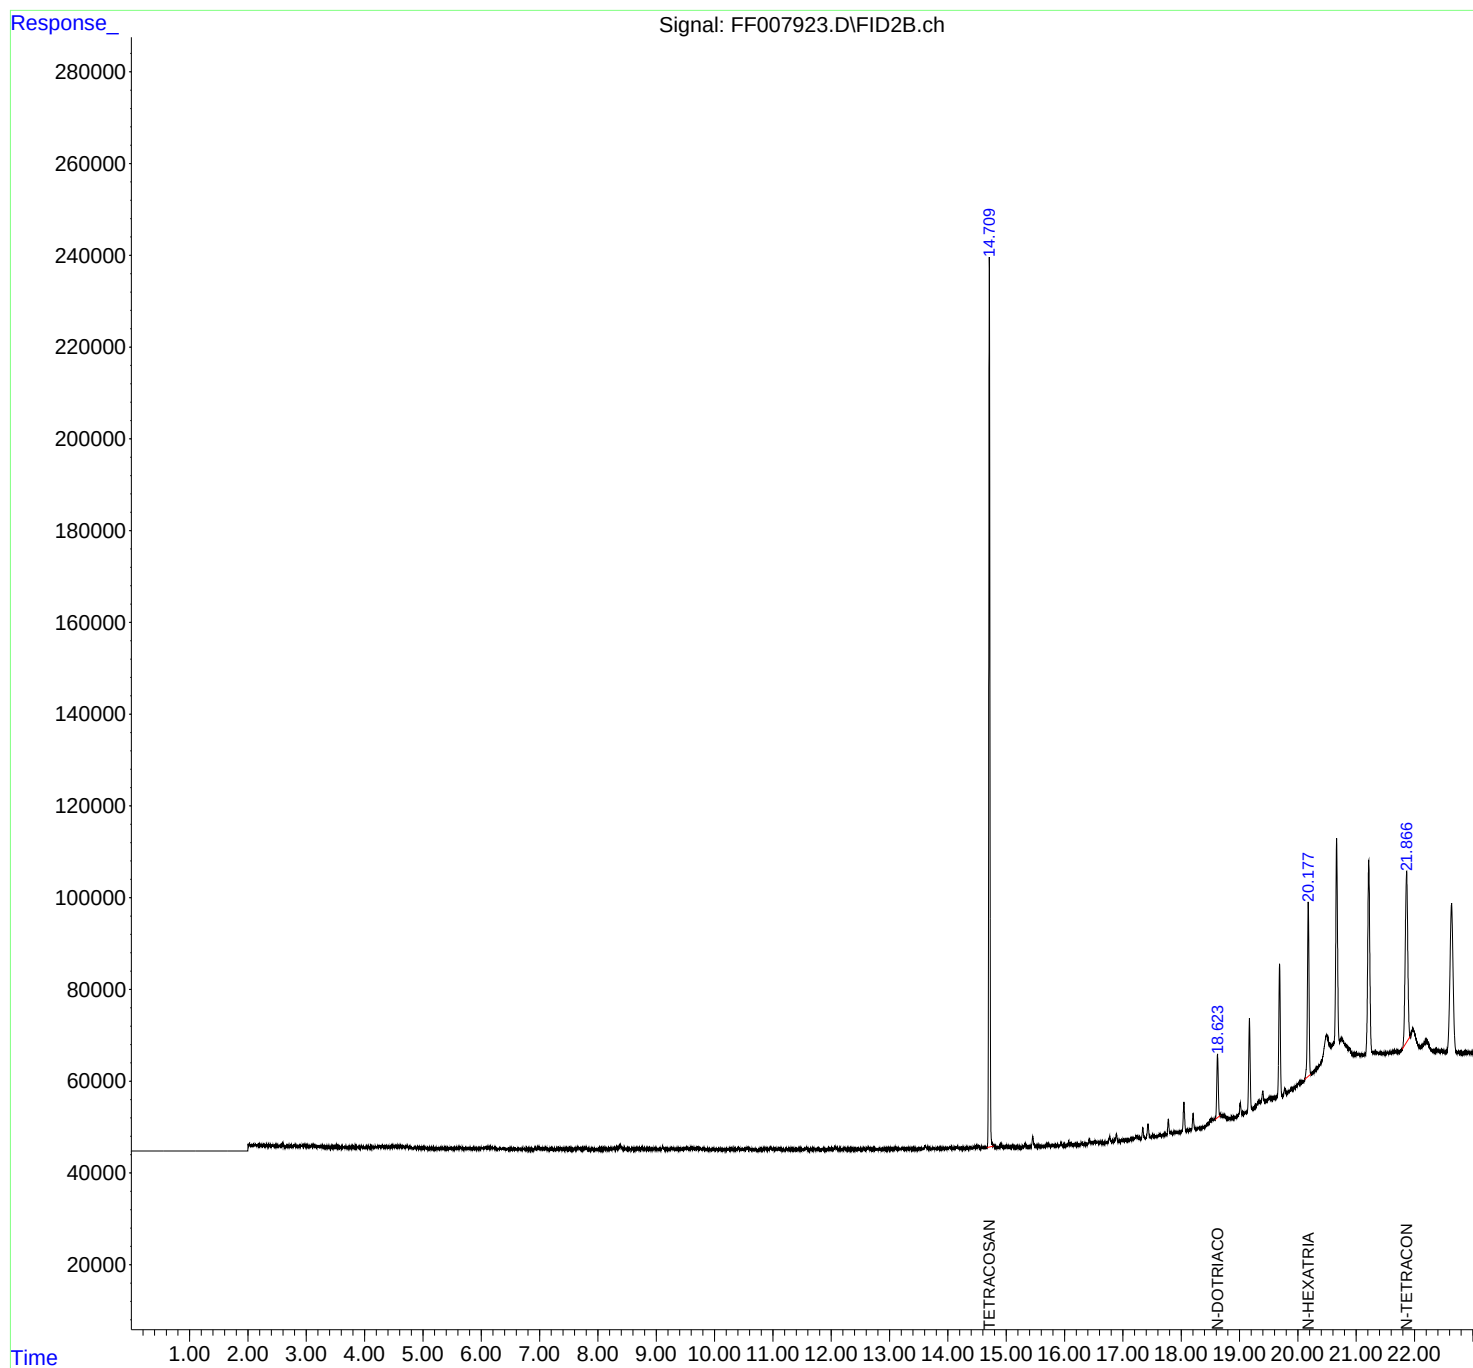


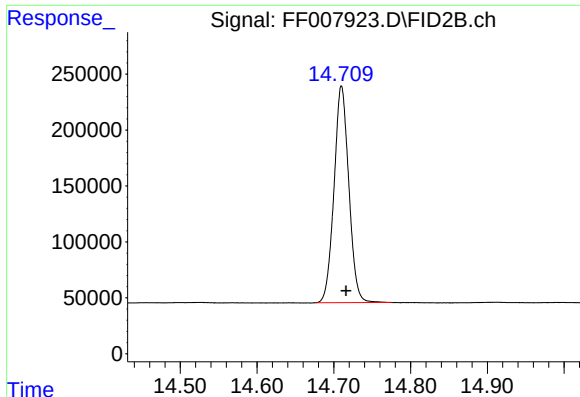

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.710 min
Delta R.T.: -0.006 min
Response: 2593885
Conc: 20.52 ug/ml

Instrument :
FID_F
ClientSampleId :

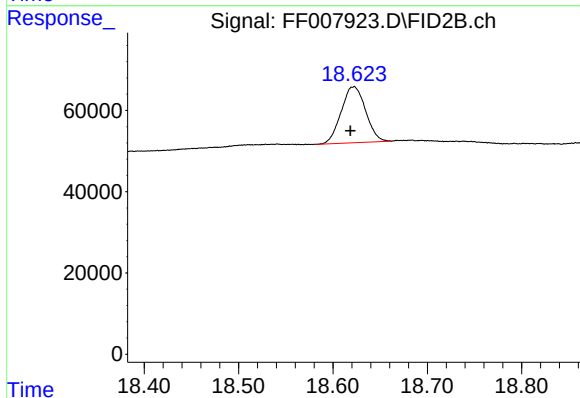


#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: 0.004 min
Response: 247977
Conc: 2.24 ug/ml

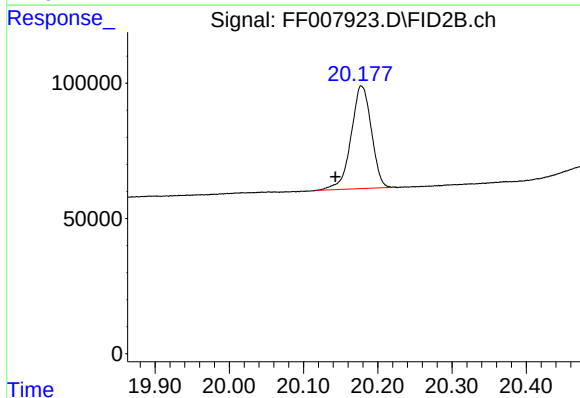

#16 N-HEXATRIACONTANE

R.T.: 20.177 min
Delta R.T.: 0.035 min
Response: 719045
Conc: 11.45 ug/ml

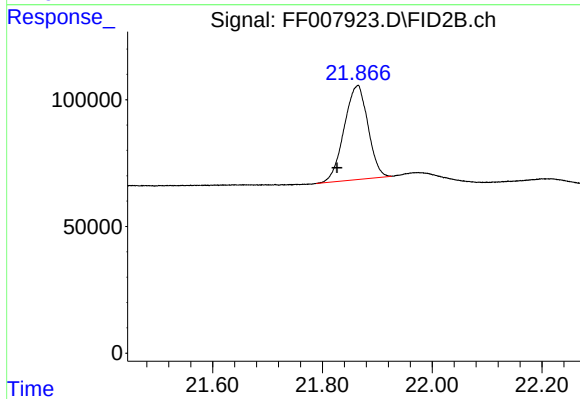

#18 N-TETRACONTANE

R.T.: 21.865 min
Delta R.T.: 0.039 min
Response: 1114893
Conc: 19.88 ug/ml