

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
 Data File : FF011747.D
 Signal(s) : FID2B.ch
 Acq On : 02 Dec 2022 10:54
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 04 10:52:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.887f	58077	0.420 ug/ml
8)	N-DOCOSANE	14.141	187163	1.387 ug/ml
10)	N-TETRACOSANE	15.231	1489991	10.987 ug/ml
11)	N-HEXACOSANE	16.273	113615	0.850 ug/ml
12)	N-OCTACOSANE	17.222	114330	0.863 ug/ml
13)	N-TRIACONTANE	18.111	118932	0.902 ug/ml
14)	N-DOTRIACONTANE	18.946	217416	1.615 ug/ml
15)	N-TETRATRIACONTANE	19.727	112585	0.855 ug/ml
16)	N-HEXATRIACONTANE	20.466	76598	0.622 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011747.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 10:54
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 10:52:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

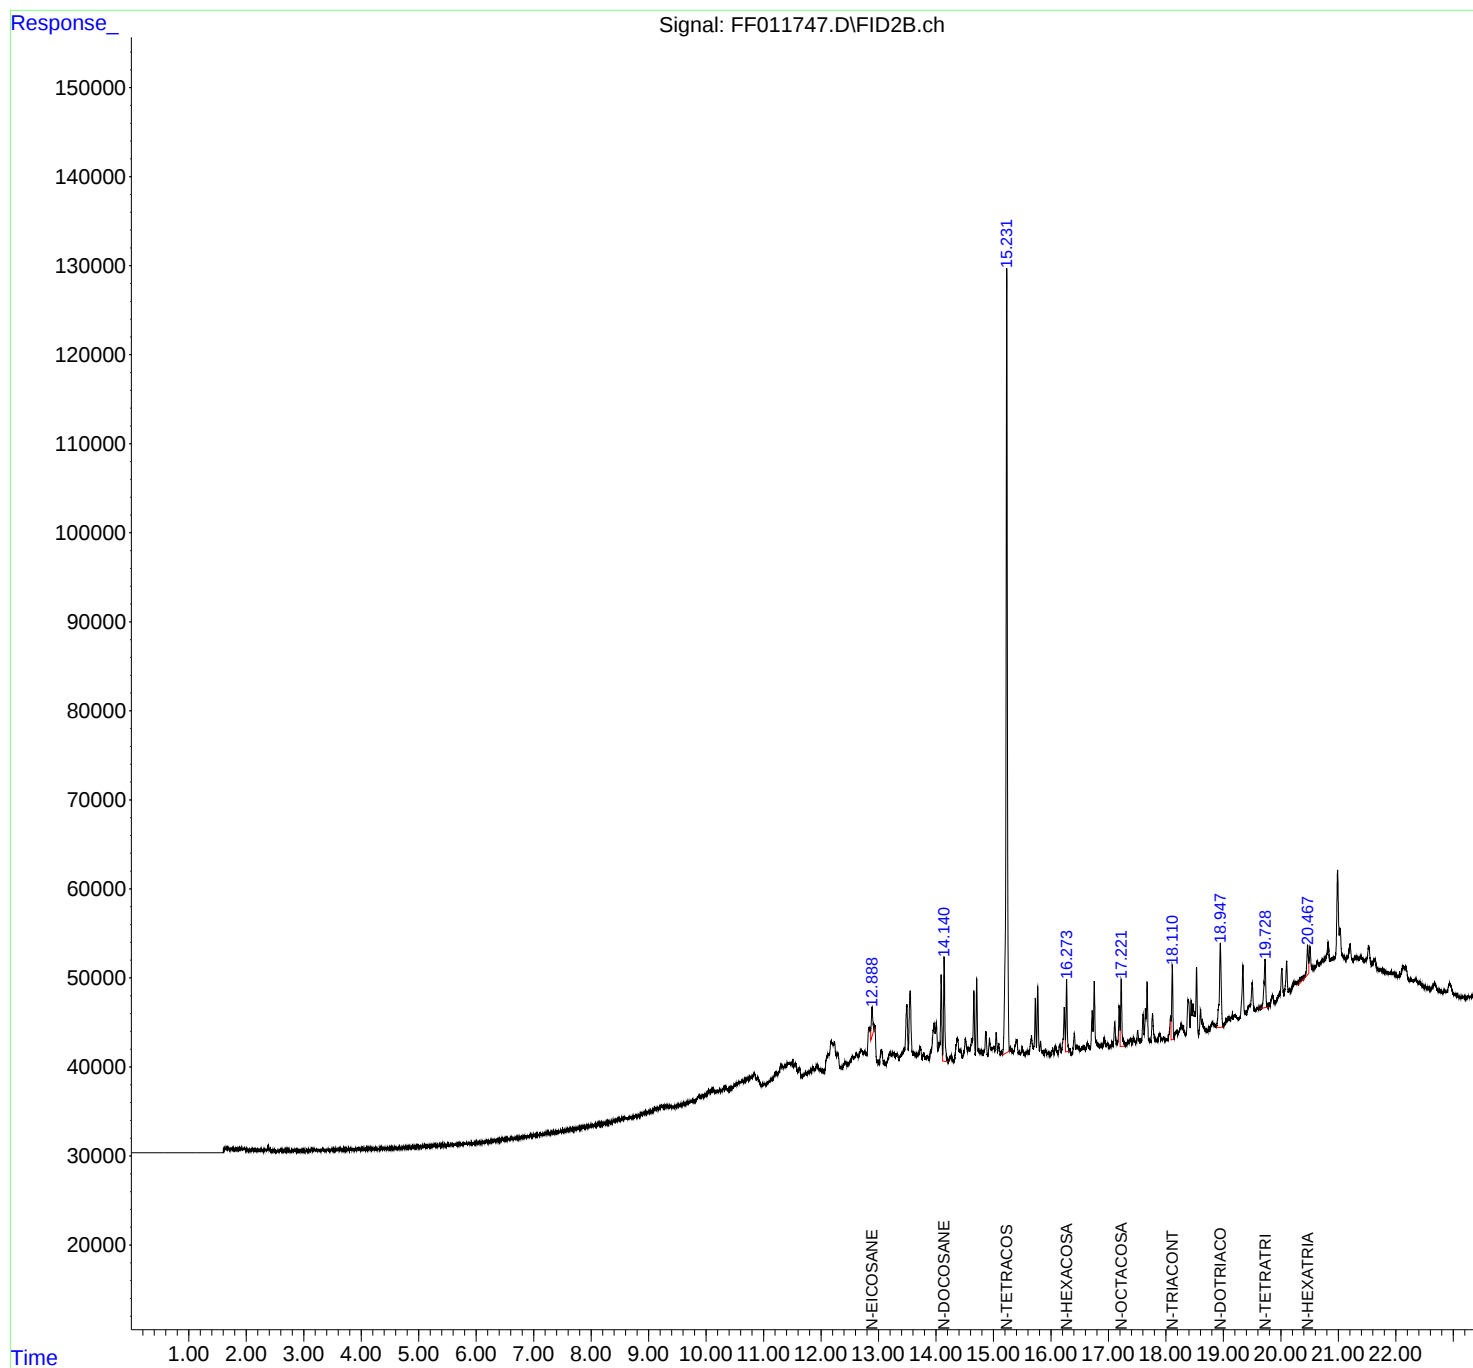


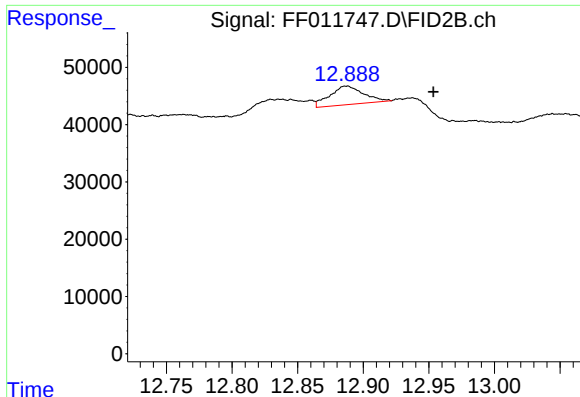

#7 N-EICOSANE


R.T.: 12.887 min
Delta R.T.: -0.066 min
Response: 58077
Conc: 0.42 ug/ml

Instrument :
FID_F
ClientSampleId :

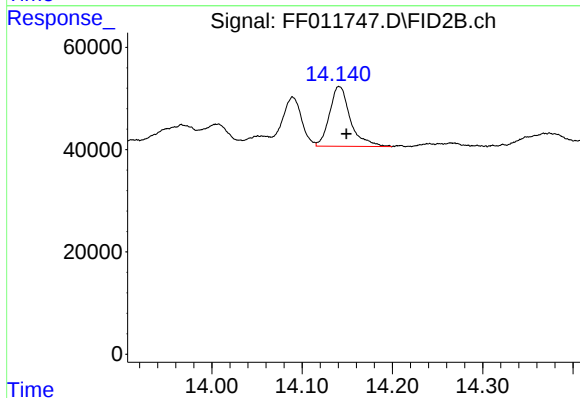


#8 N-DOCOSANE

R.T.: 14.141 min
Delta R.T.: -0.008 min
Response: 187163
Conc: 1.39 ug/ml

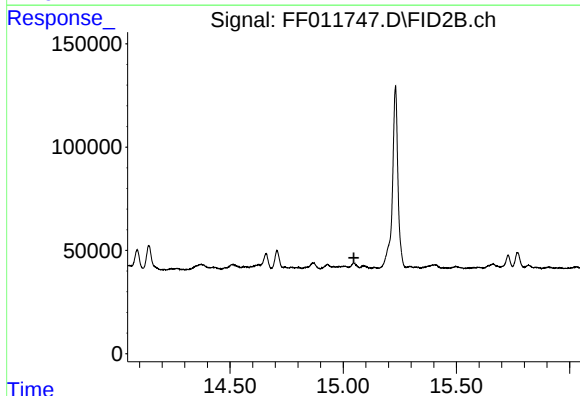


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

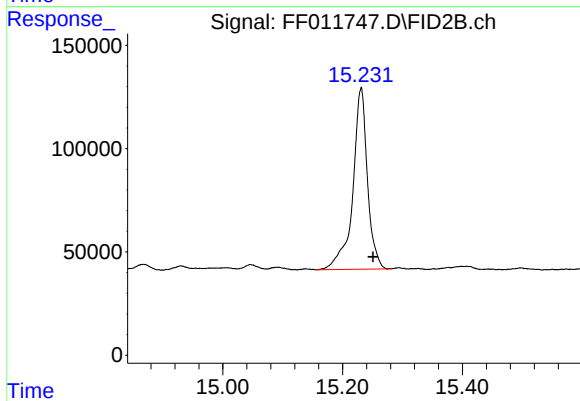

#10 N-TETRACOSANE


R.T.: 15.231 min
Delta R.T.: -0.020 min
Response: 1489991
Conc: 10.99 ug/ml

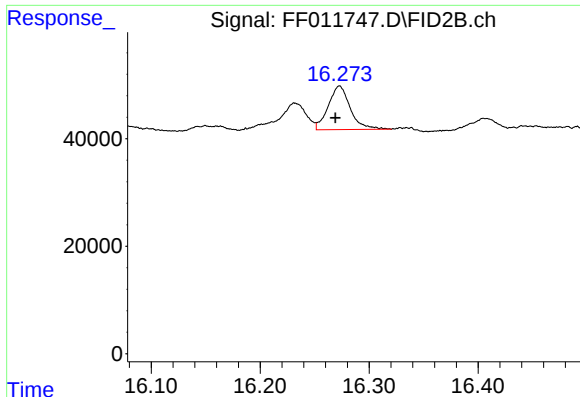

#11 N-HEXACOSANE


R.T.: 16.273 min
Delta R.T.: 0.004 min
Response: 113615
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

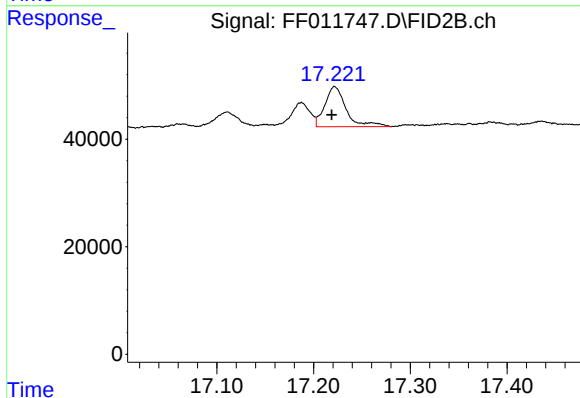


#12 N-OCTACOSANE

R.T.: 17.222 min
Delta R.T.: 0.003 min
Response: 114330
Conc: 0.86 ug/ml

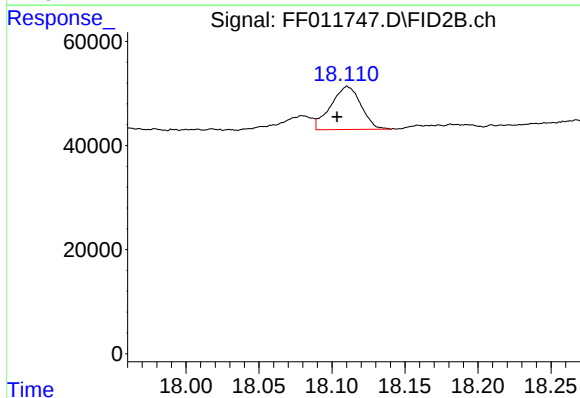


#13 N-TRIACONTANE

R.T.: 18.111 min
Delta R.T.: 0.007 min
Response: 118932
Conc: 0.90 ug/ml

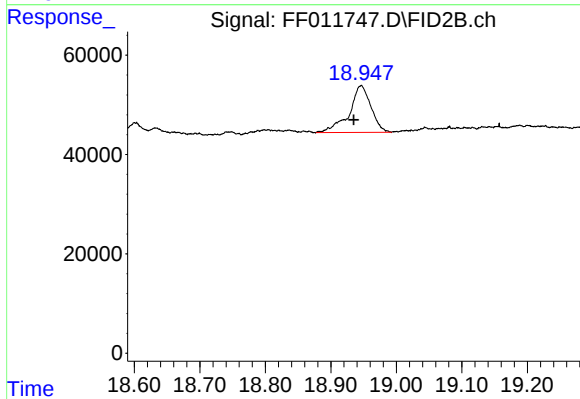

#14 N-DOTRIACONTANE


R.T.: 18.946 min
Delta R.T.: 0.011 min
Response: 217416
Conc: 1.62 ug/ml

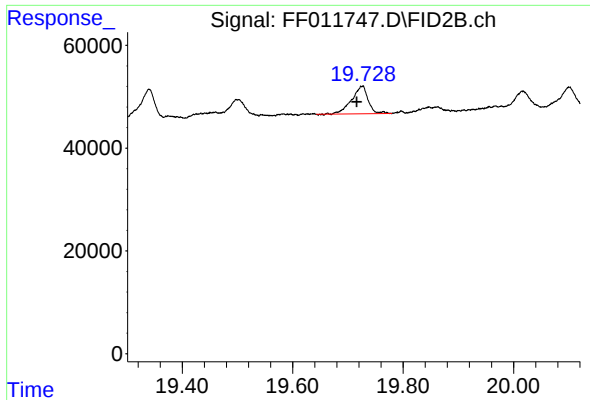

#15 N-TETRATRIACONTANE

R.T.: 19.727 min
Delta R.T.: 0.011 min
Response: 112585
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

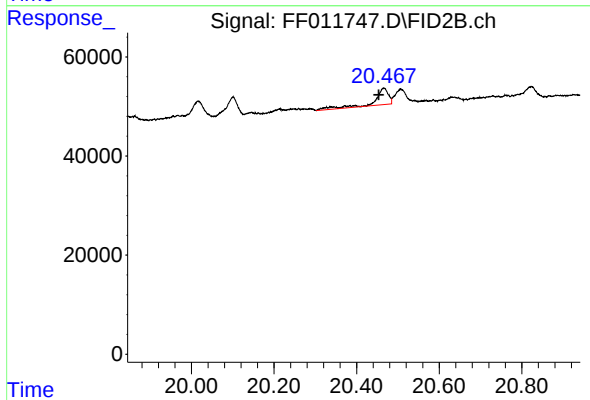

#16 N-HEXATRIACONTANE

R.T.: 20.466 min
Delta R.T.: 0.012 min
Response: 76598
Conc: 0.62 ug/ml