

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
 Data File : FF011748.D
 Signal(s) : FID2B.ch
 Acq On : 02 Dec 2022 11:24
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 04 10:52:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.052	2578483	21.733 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.110	87066	0.660 ug/ml
14) N-DOTRIACONTANE	18.943	112006	0.832 ug/ml
15) N-TETRATRIACONTANE	19.727	89266	0.678 ug/ml
16) N-HEXATRIACONTANE	20.467	50914	0.413 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011748.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 11:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 10:52:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

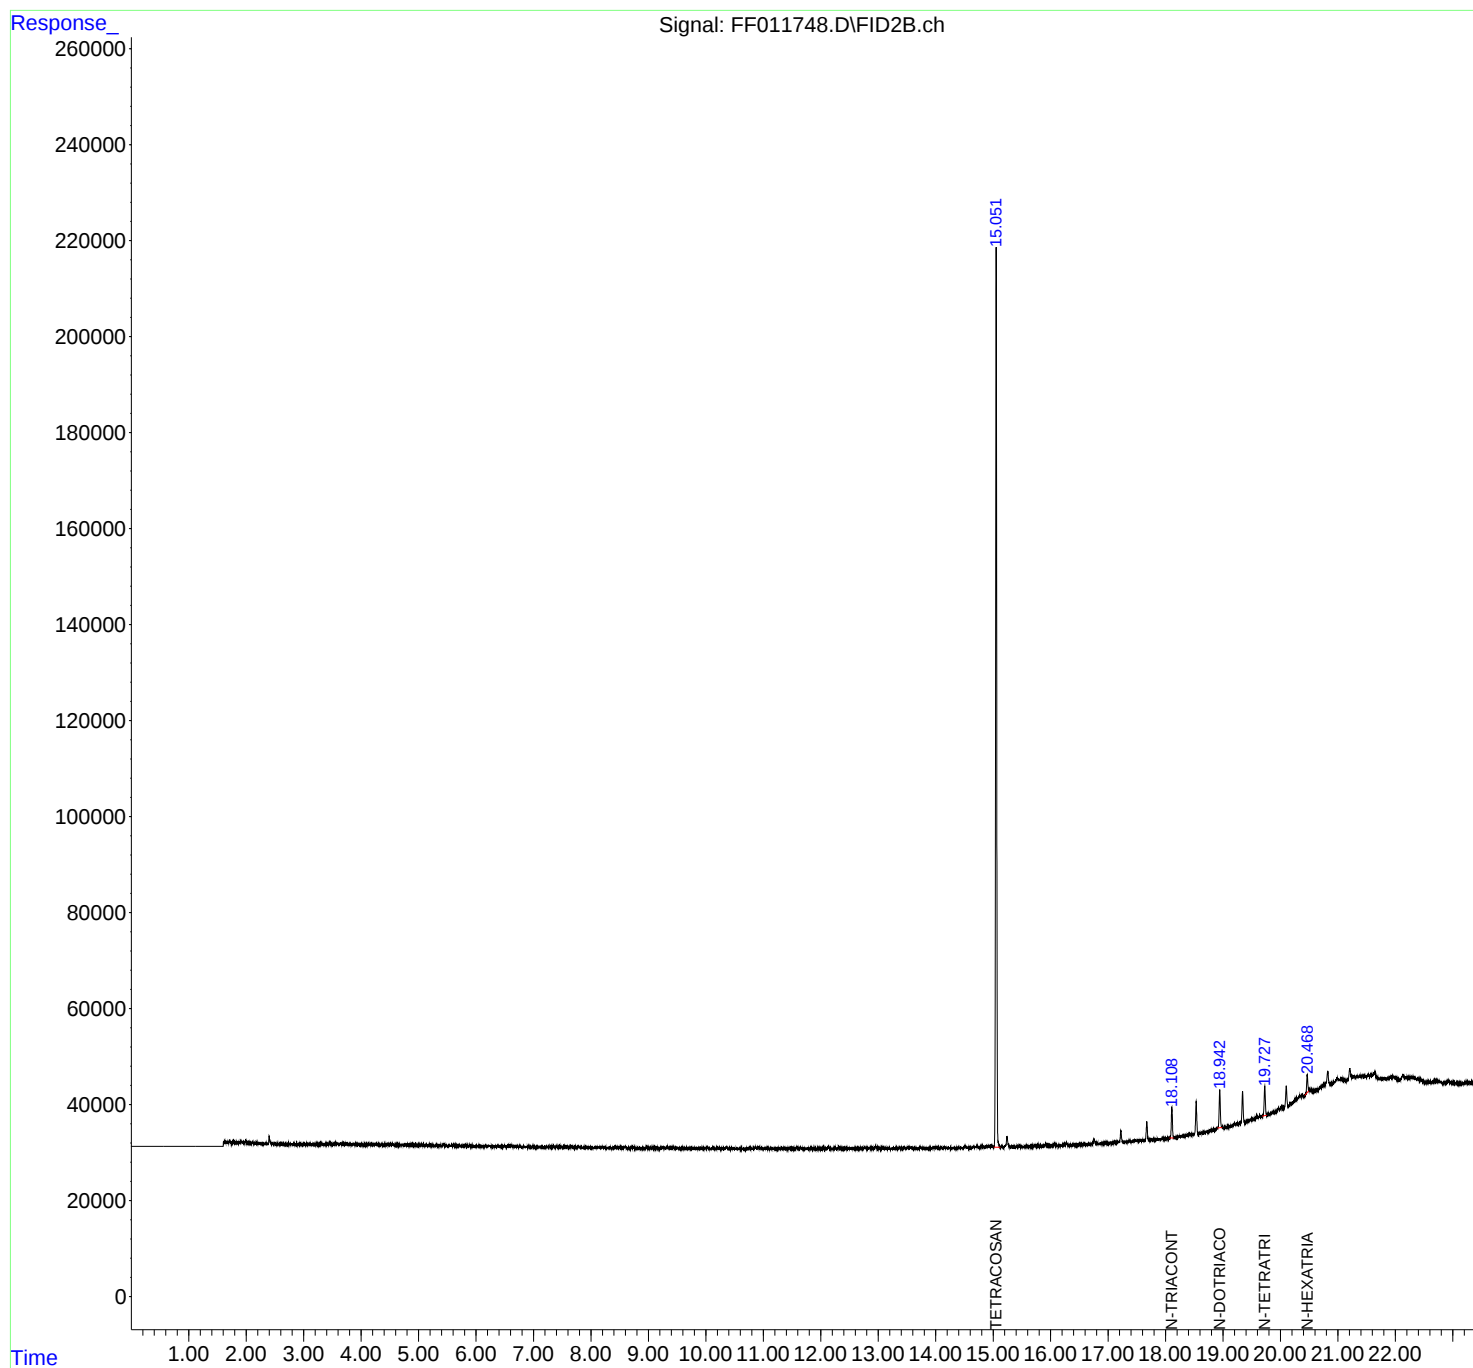


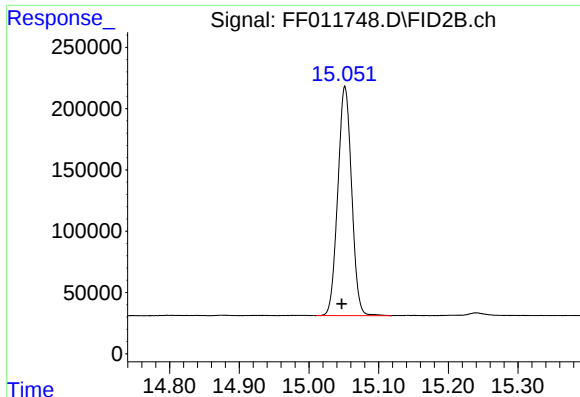

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.052 min
Delta R.T.: 0.005 min
Response: 2578483
Conc: 21.73 ug/ml

Instrument :
FID_F
ClientSampleId :

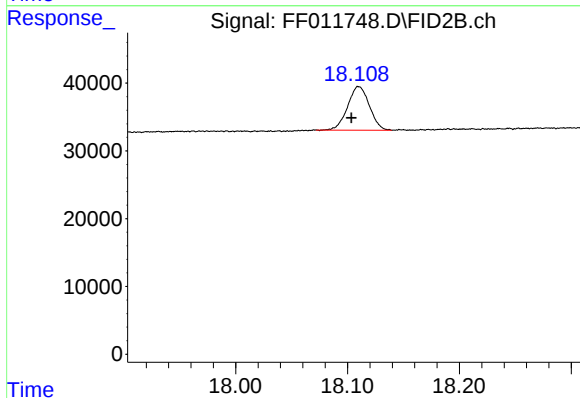


#13 N-TRIACONTANE

R.T.: 18.110 min
Delta R.T.: 0.007 min
Response: 87066
Conc: 0.66 ug/ml

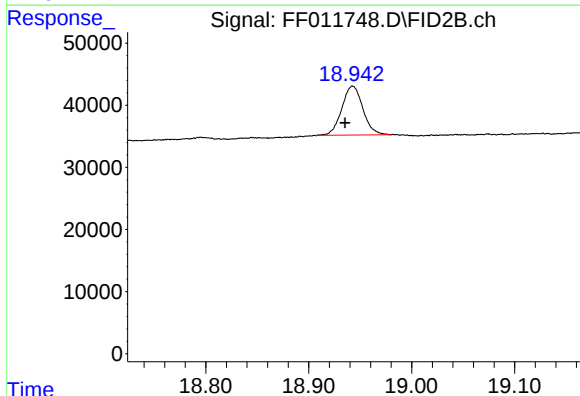


#14 N-DOTRIACONTANE

R.T.: 18.943 min
Delta R.T.: 0.008 min
Response: 112006
Conc: 0.83 ug/ml

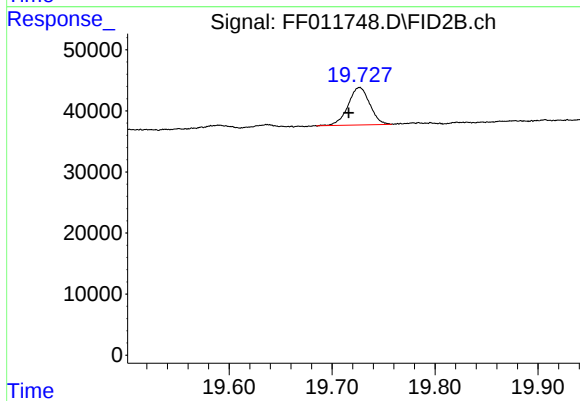

#15 N-TETRATRIACONTANE

R.T.: 19.727 min
Delta R.T.: 0.011 min
Response: 89266
Conc: 0.68 ug/ml

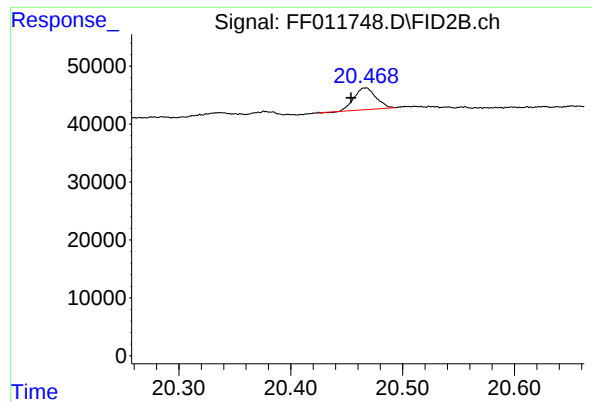

#16 N-HEXATRIACONTANE

R.T.: 20.467 min
Delta R.T.: 0.013 min
Response: 50914
Conc: 0.41 ug/ml

Instrument :

FID_F

ClientSampleId :