

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
 Data File : FF011750.D
 Signal(s) : FID2B.ch
 Acq On : 02 Dec 2022 12:28
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 04 10:53:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.770	2355223	17.523 ug/ml
12) N-OCTACOSANE	17.226	2203644	16.634 ug/ml
13) N-TRIACONTANE	18.113	192215	1.457 ug/ml
14) N-DOTRIACONTANE	18.944	245021	1.820 ug/ml
15) N-TETRATRIACONTANE	19.728	200855	1.525 ug/ml
16) N-HEXATRIACONTANE	20.467	129310	1.050 ug/ml
17) N-OCTATRIACONTANE	21.208	90936	0.781 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011750.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 12:28
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 10:53:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

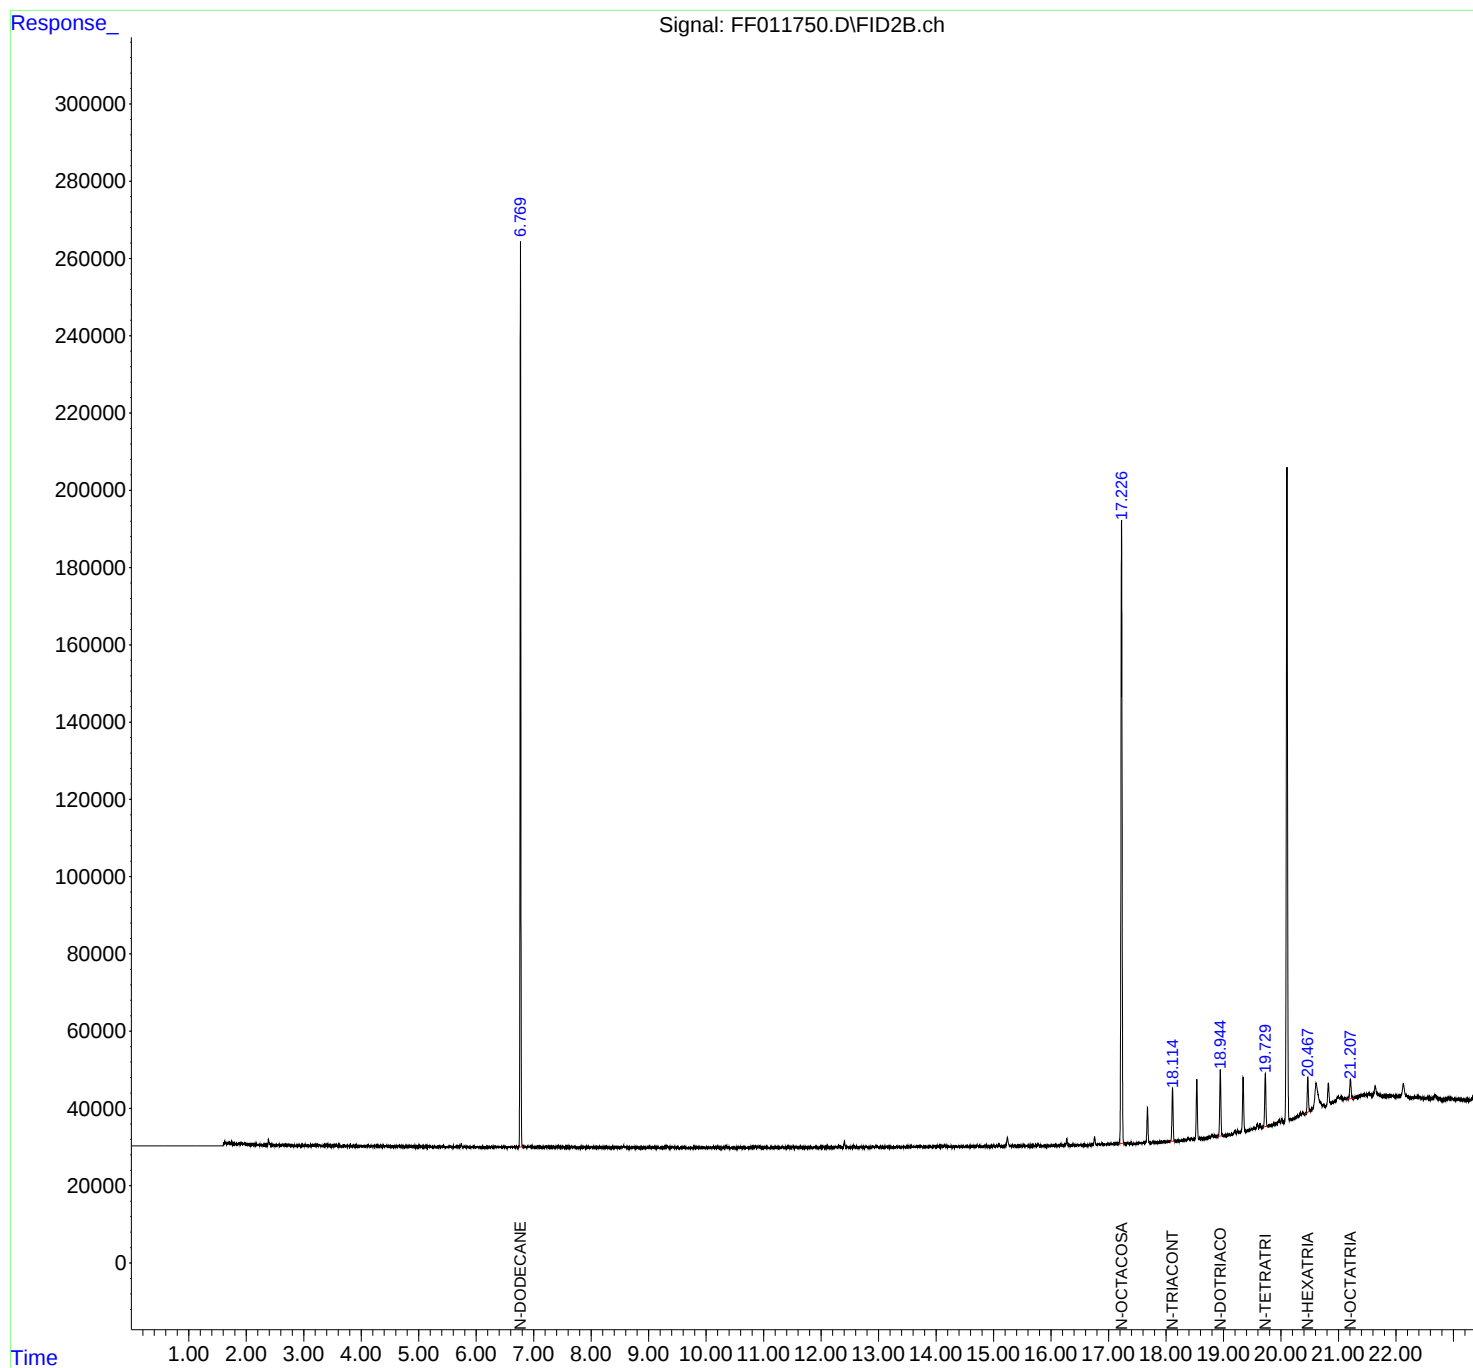


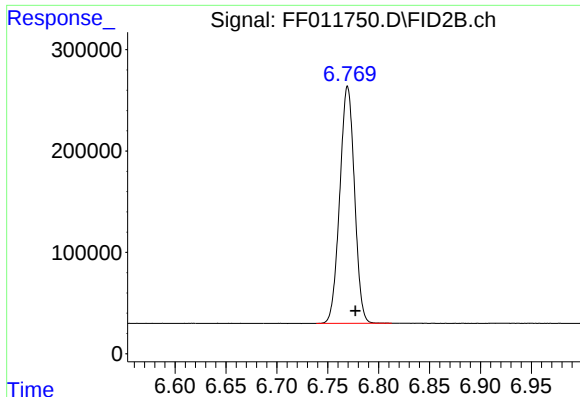

#3 N-DODECANE


R.T.: 6.770 min
Delta R.T.: -0.008 min
Response: 2355223
Conc: 17.52 ug/ml

Instrument :
FID_F
ClientSampleId :

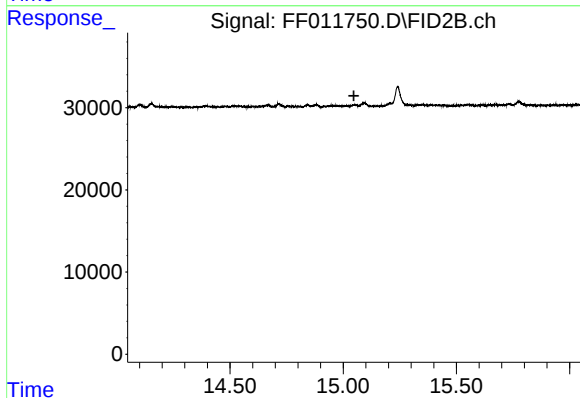


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

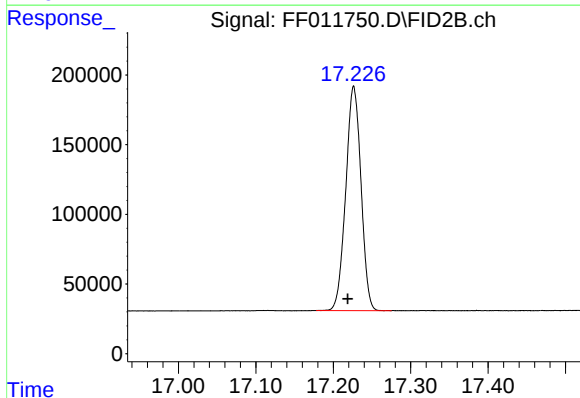


#12 N-OCTACOSANE

R.T.: 17.226 min
Delta R.T.: 0.008 min
Response: 2203644
Conc: 16.63 ug/ml

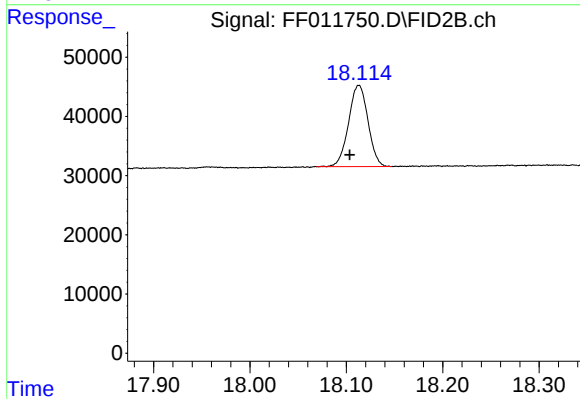

#13 N-TRIACONTANE


R.T.: 18.113 min
Delta R.T.: 0.009 min
Response: 192215
Conc: 1.46 ug/ml

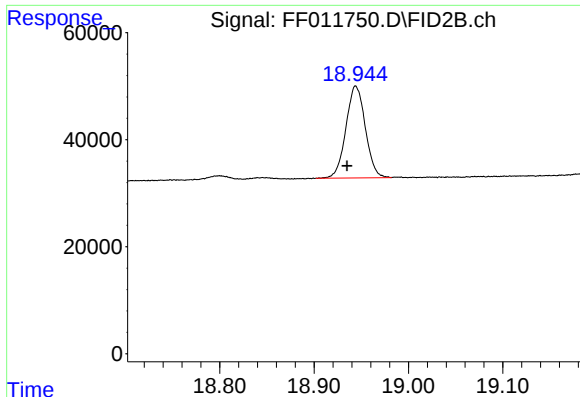

#14 N-DOTRIACONTANE


R.T.: 18.944 min
Delta R.T.: 0.009 min
Response: 245021
Conc: 1.82 ug/ml

Instrument :
FID_F
ClientSampleId :

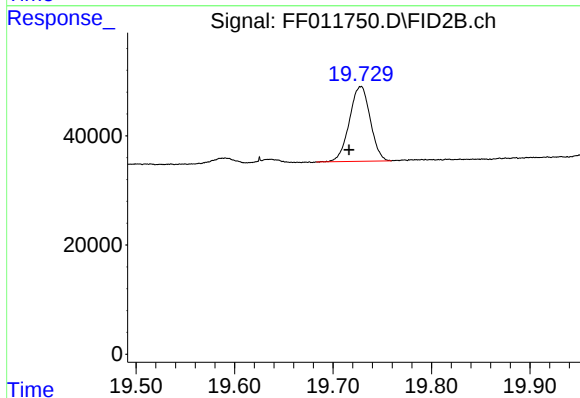


#15 N-TETRATRIACONTANE

R.T.: 19.728 min
Delta R.T.: 0.012 min
Response: 200855
Conc: 1.53 ug/ml

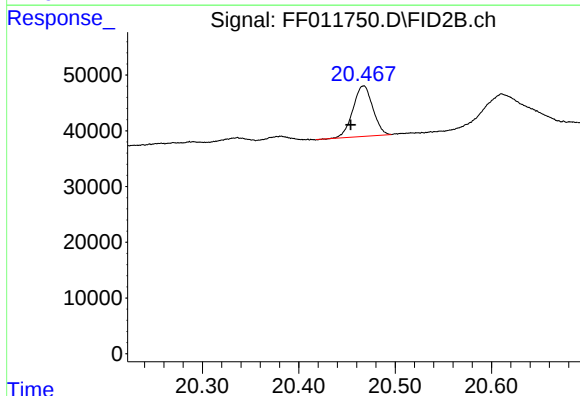

#16 N-HEXATRIACONTANE

R.T.: 20.467 min
Delta R.T.: 0.013 min
Response: 129310
Conc: 1.05 ug/ml

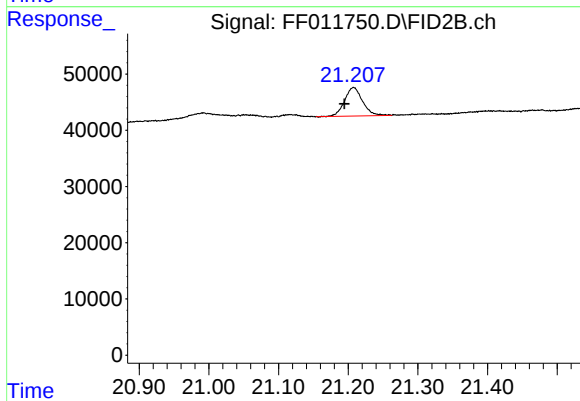

#17 N-OCTATRIACONTANE

R.T.: 21.208 min
Delta R.T.: 0.014 min
Response: 90936
Conc: 0.78 ug/ml