

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
 Data File : FF011751.D
 Signal(s) : FID2B.ch
 Acq On : 02 Dec 2022 14:02
 Operator : YP\AJ
 Sample : N5846-07
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 04 10:53:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	2023651	17.056 ug/ml
Target Compounds			
4) N-TETRADECANE	8.587	57738	0.427 ug/ml
5) N-HEXADECANE	10.209	134020	0.975 ug/ml
6) N-OCTADECANE	11.653	187260	1.354 ug/ml
7) N-EICOSANE	12.943	358325	2.591 ug/ml
8) N-DOCOSANE	14.151	295304	2.188 ug/ml
10) N-TETRACOSANE	15.238	2028851	14.961 ug/ml
11) N-HEXACOSANE	16.282	326528	2.444 ug/ml
12) N-OCTACOSANE	17.235	822477	6.208 ug/ml
13) N-TRIACONTANE	18.115	613536	4.652 ug/ml
14) N-DOTRIACONTANE	18.946	188313	1.399 ug/ml
15) N-TETRATRIACONTANE	19.728	94034	0.714 ug/ml
16) N-HEXATRIACONTANE	20.433	138249	1.122 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011751.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 14:02
Operator : YP\AJ
Sample : N5846-07
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 10:53:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

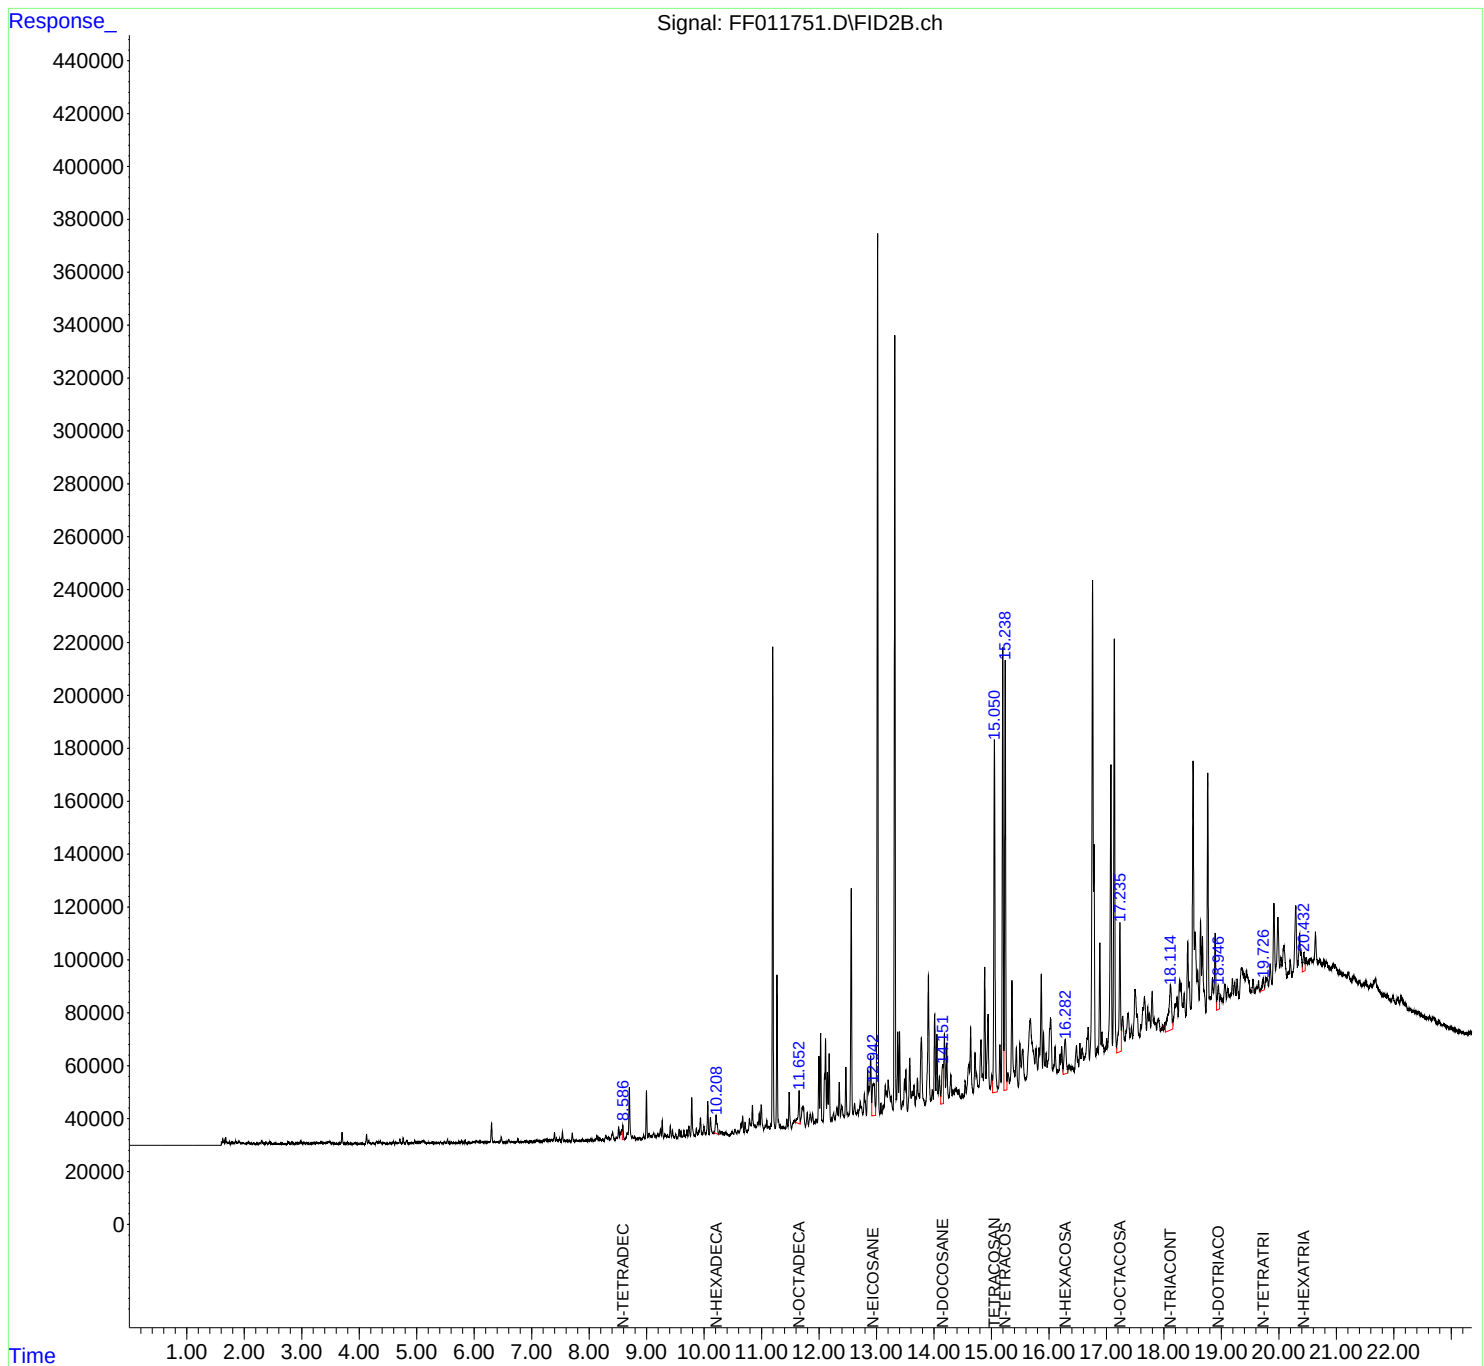


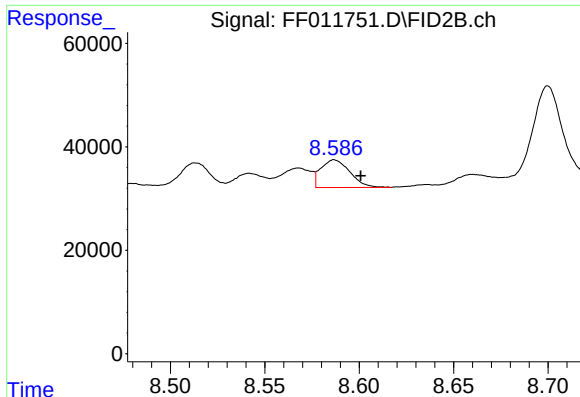

#4 N-TETRADECANE


R.T.: 8.587 min
Delta R.T.: -0.014 min
Response: 57738
Conc: 0.43 ug/ml

Instrument :
FID_F
ClientSampleId :

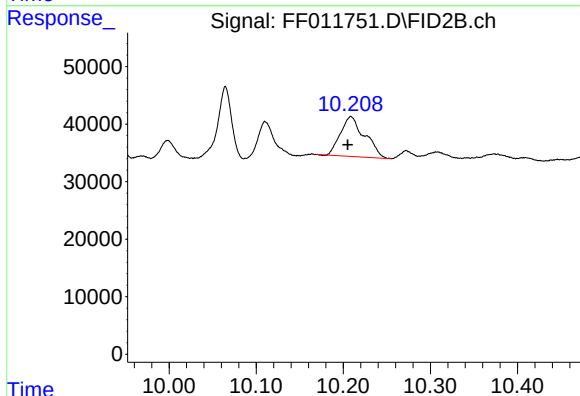


#5 N-HEXADECANE

R.T.: 10.209 min
Delta R.T.: 0.004 min
Response: 134020
Conc: 0.97 ug/ml

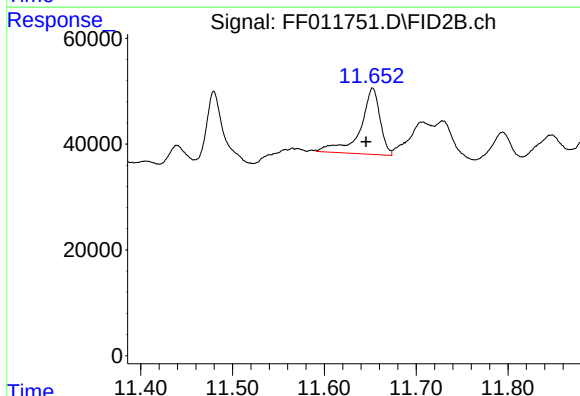


#6 N-OCTADECANE

R.T.: 11.653 min
Delta R.T.: 0.007 min
Response: 187260
Conc: 1.35 ug/ml

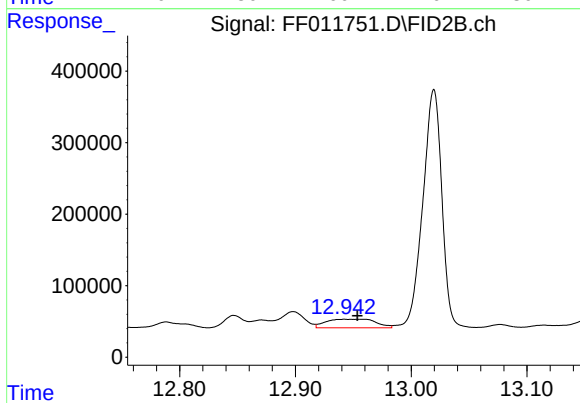

#7 N-EICOSANE


R.T.: 12.943 min
Delta R.T.: -0.011 min
Response: 358325
Conc: 2.59 ug/ml

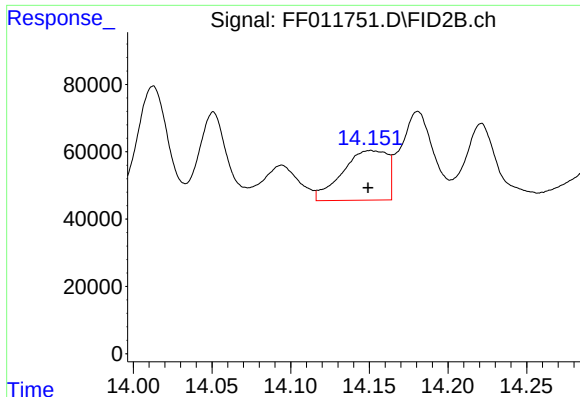

#8 N-DOCOSANE


R.T.: 14.151 min
Delta R.T.: 0.001 min
Response: 295304
Conc: 2.19 ug/ml

Instrument :
FID_F
ClientSampleId :

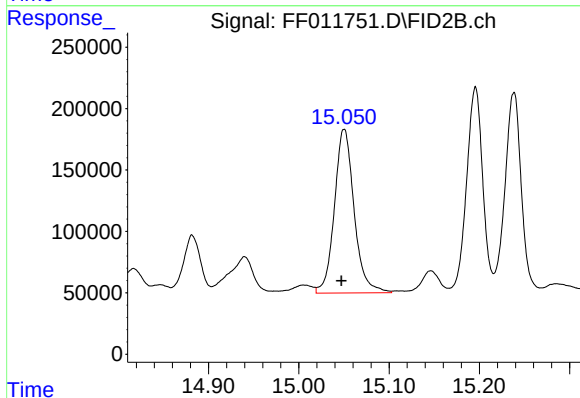


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.050 min
Delta R.T.: 0.003 min
Response: 2023651
Conc: 17.06 ug/ml

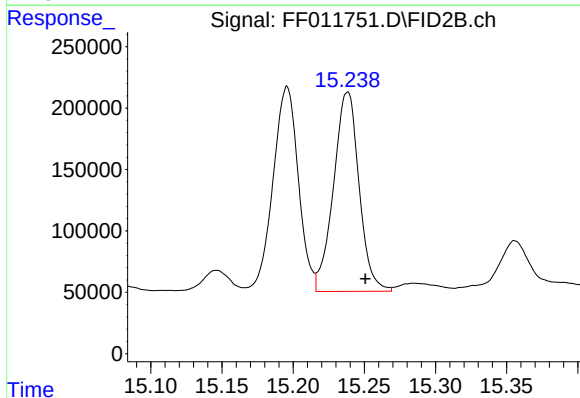


#10 N-TETRACOSANE

R.T.: 15.238 min
Delta R.T.: -0.013 min
Response: 2028851
Conc: 14.96 ug/ml

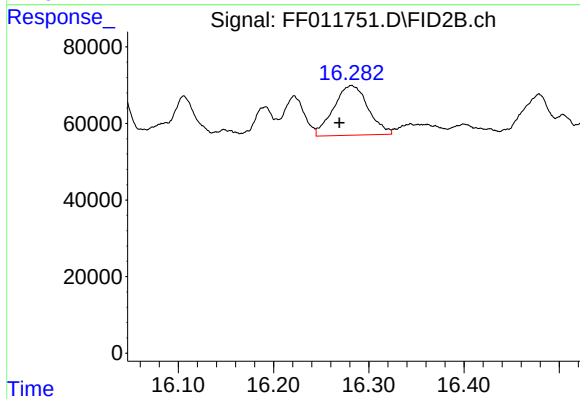

#11 N-HEXACOSANE


R.T.: 16.282 min
Delta R.T.: 0.013 min
Response: 326528
Conc: 2.44 ug/ml

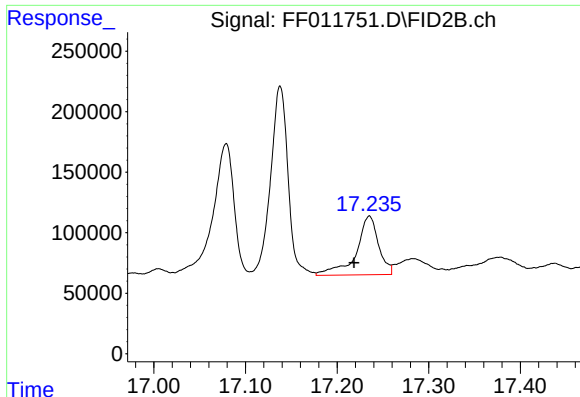

#12 N-OCTACOSANE


R.T.: 17.235 min
Delta R.T.: 0.017 min
Response: 822477
Conc: 6.21 ug/ml

Instrument :
FID_F
ClientSampleId :

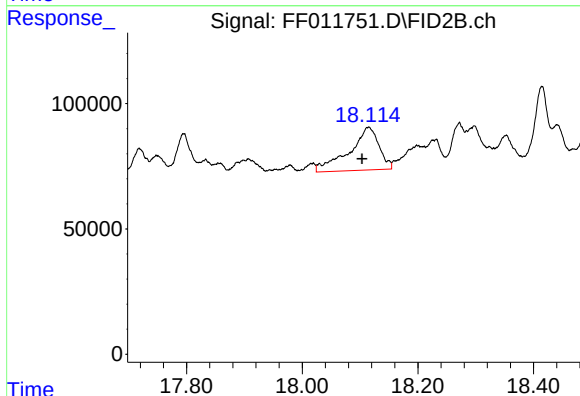


#13 N-TRIACONTANE

R.T.: 18.115 min
Delta R.T.: 0.012 min
Response: 613536
Conc: 4.65 ug/ml

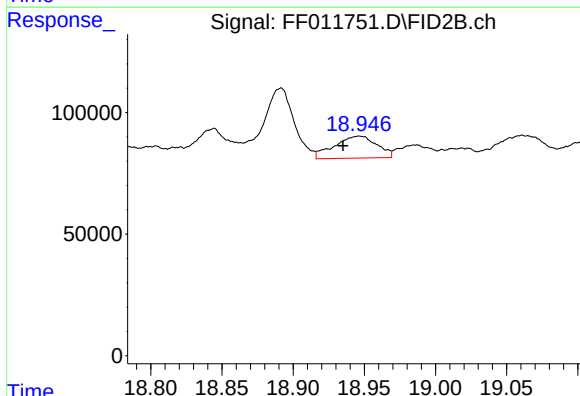


#14 N-DOTRIACONTANE

R.T.: 18.946 min
Delta R.T.: 0.011 min
Response: 188313
Conc: 1.40 ug/ml

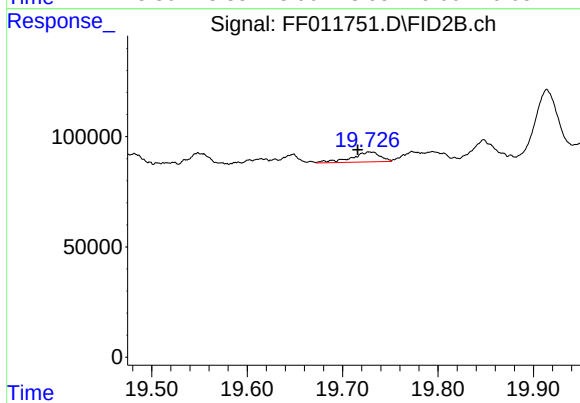

#15 N-TETRATRIACONTANE

R.T.: 19.728 min
Delta R.T.: 0.012 min
Response: 94034
Conc: 0.71 ug/ml

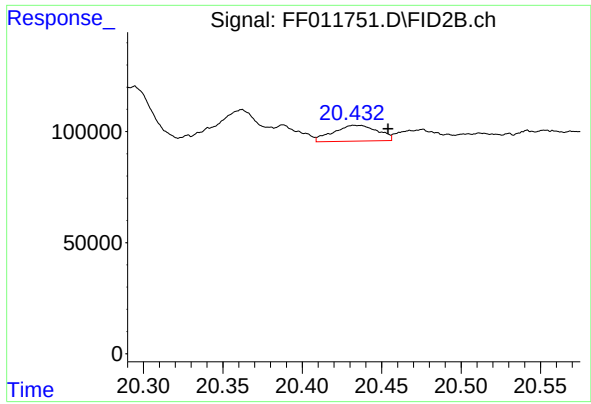

#16 N-HEXATRIACONTANE

R.T.: 20.433 min
Delta R.T.: -0.021 min
Response: 138249
Conc: 1.12 ug/ml

Instrument :

FID_F

ClientSampleId :