

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011751.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 14:02
Operator : YP\AJ
Sample : N5846-07
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP25-10-20221201-6.5-7.0-A

Integration File: Sample.e
Quant Time: Dec 04 10:53:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	2023651	17.056 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011751.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 14:02
Operator : YP\AJ
Sample : N5846-07
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP25-10-20221201-6.5-7.0-A

Integration File: Sample.e
Quant Time: Dec 04 10:53:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

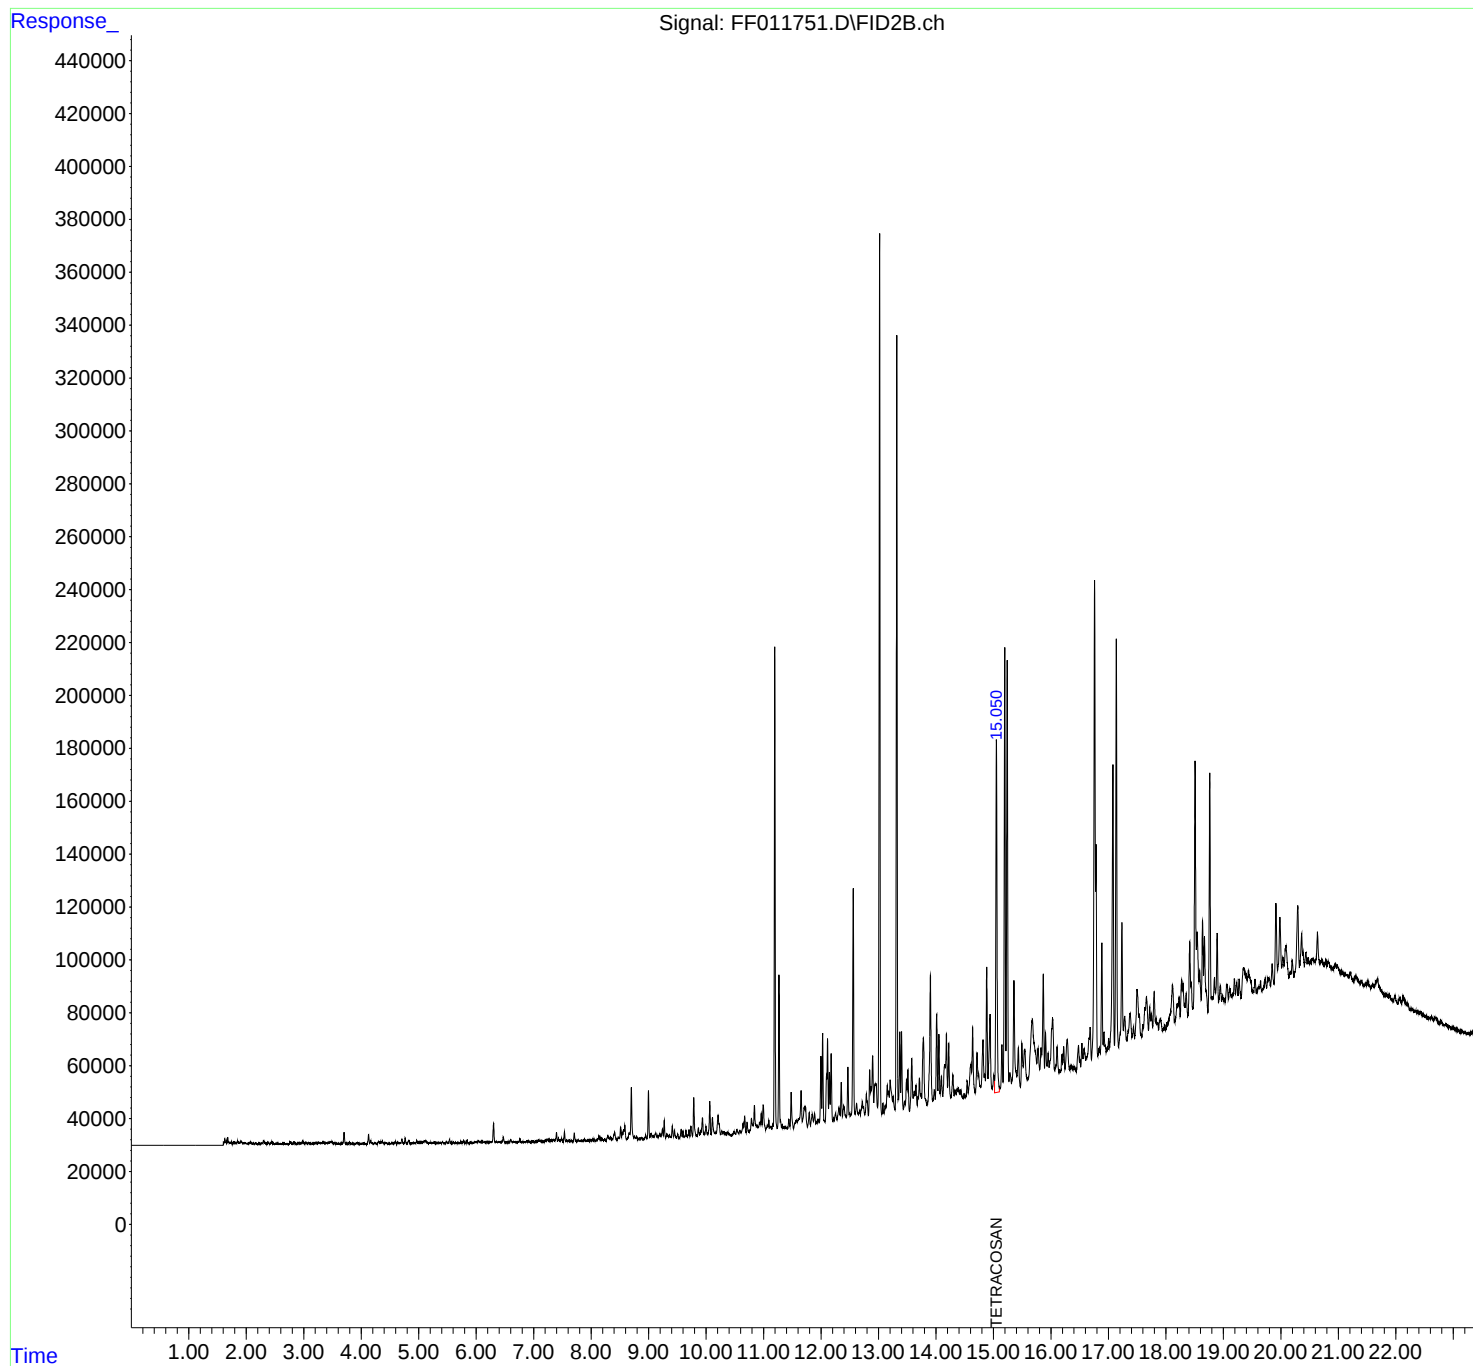

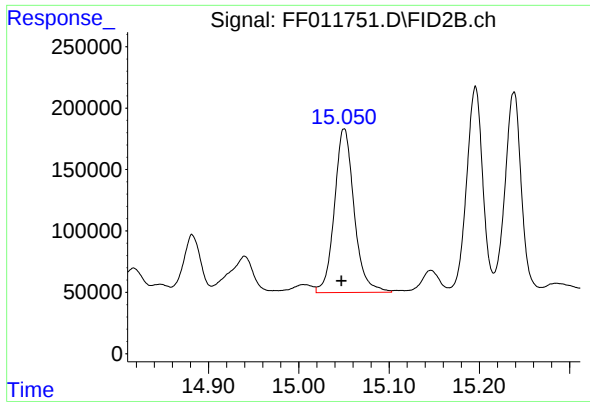

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.050 min
Delta R.T.: 0.003 min
Response: 2023651
Conc: 17.06 ug/ml

Instrument :
FID_F
ClientSampleId :
SP25-10-20221201-6.5-7.0-A