

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
 Data File : FF011754.D
 Signal(s) : FID2B.ch
 Acq On : 02 Dec 2022 15:30
 Operator : YP\AJ
 Sample : N5846-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SP25-09-20221201-16.5-17.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/05/2022
 Supervised By :Ankita Jodhani 12/05/2022

Integration File: Sample.e
 Quant Time: Dec 04 10:54:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.085	4950086	41.722 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011754.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 15:30
Operator : YP\AJ
Sample : N5846-10
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SP25-09-20221201-16.5-17.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/05/2022
Supervised By :Ankita Jodhani 12/05/2022

Integration File: Sample.e
Quant Time: Dec 04 10:54:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

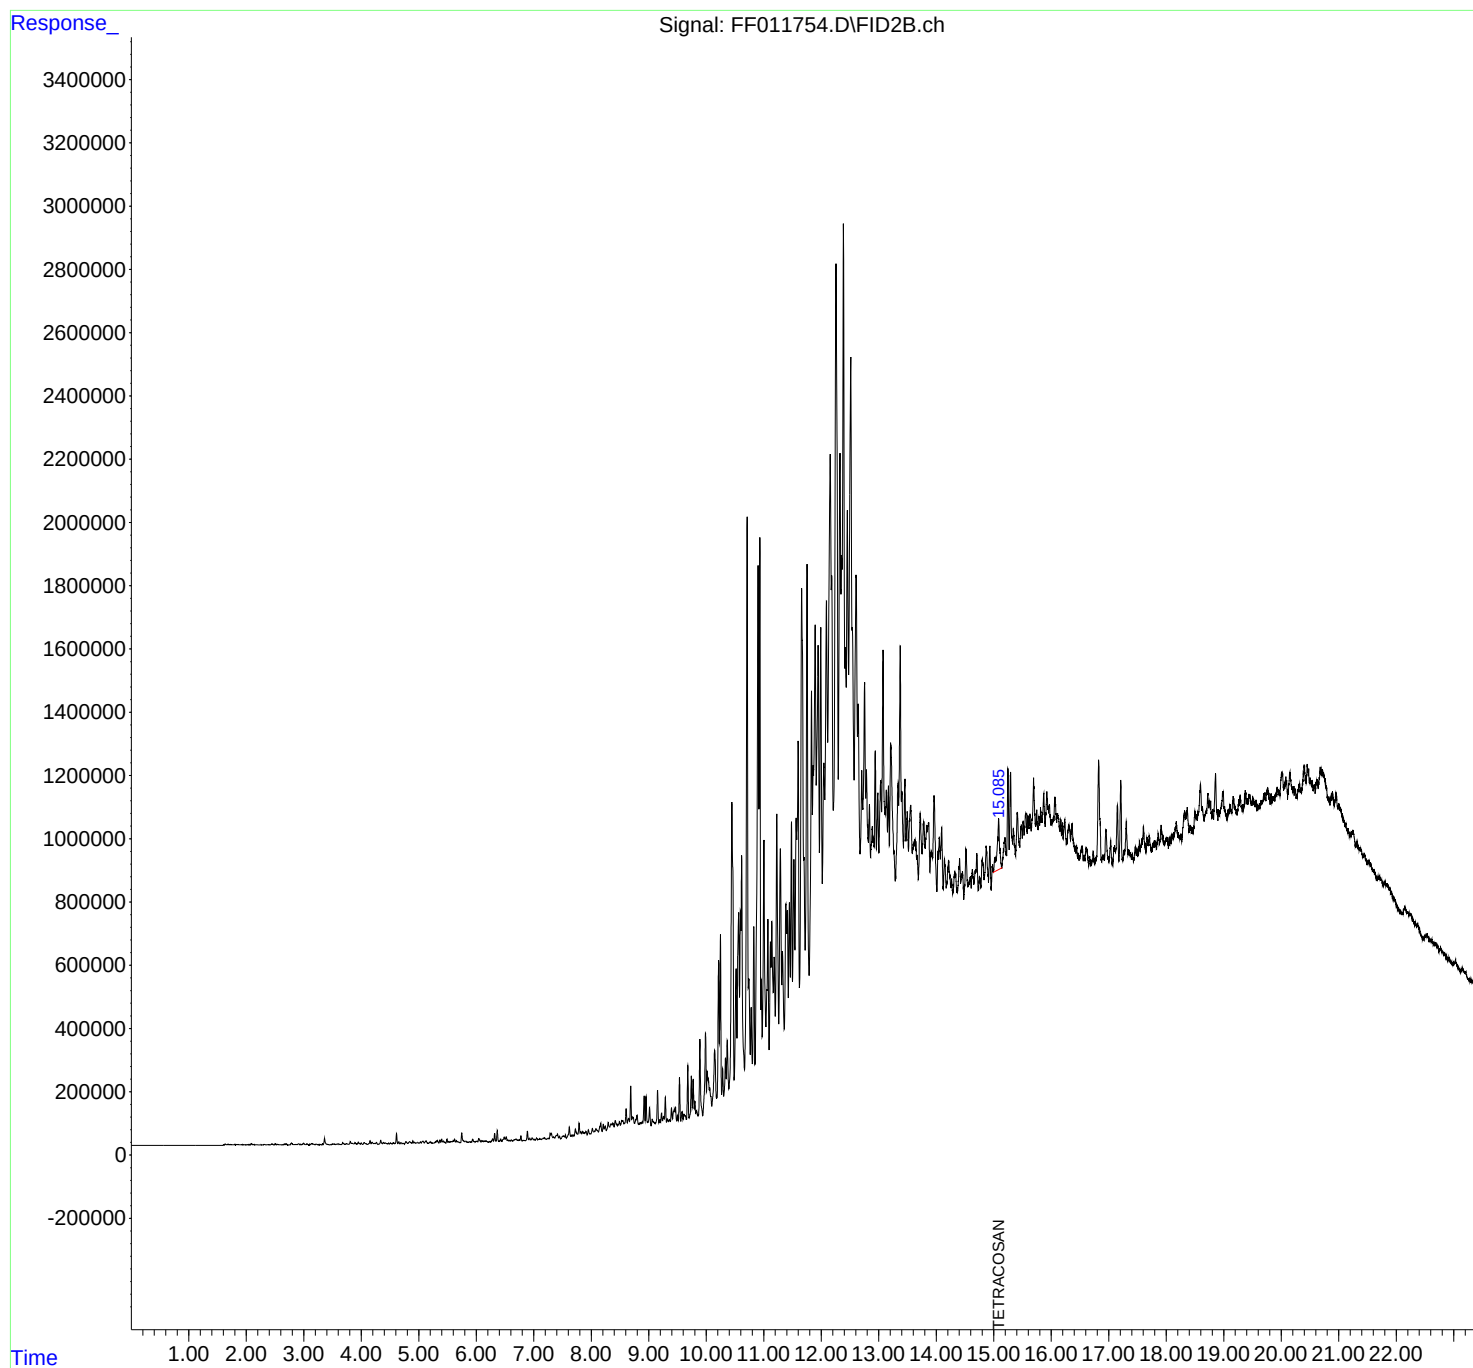

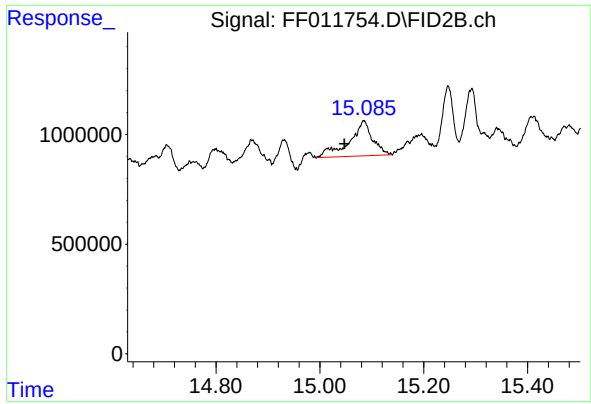

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.085 min
Delta R.T.: 0.038 min
Response: 4950086
Conc: 41.72 ug/ml

Instrument :
FID_F
ClientSampleId :
SP25-09-20221201-16.5-17.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/05/2022
Supervised By :Ankita Jodhani 12/05/2022