

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011755.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 16:00
Operator : YP\AJ
Sample : N5846-08 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP25-10-20221201-17.5-18.0

Integration File: Sample.e
Quant Time: Dec 04 10:54:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.060	388917	3.278 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120222\
Data File : FF011755.D
Signal(s) : FID2B.ch
Acq On : 02 Dec 2022 16:00
Operator : YP\AJ
Sample : N5846-08 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SP25-10-20221201-17.5-18.0

Integration File: Sample.e
Quant Time: Dec 04 10:54:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

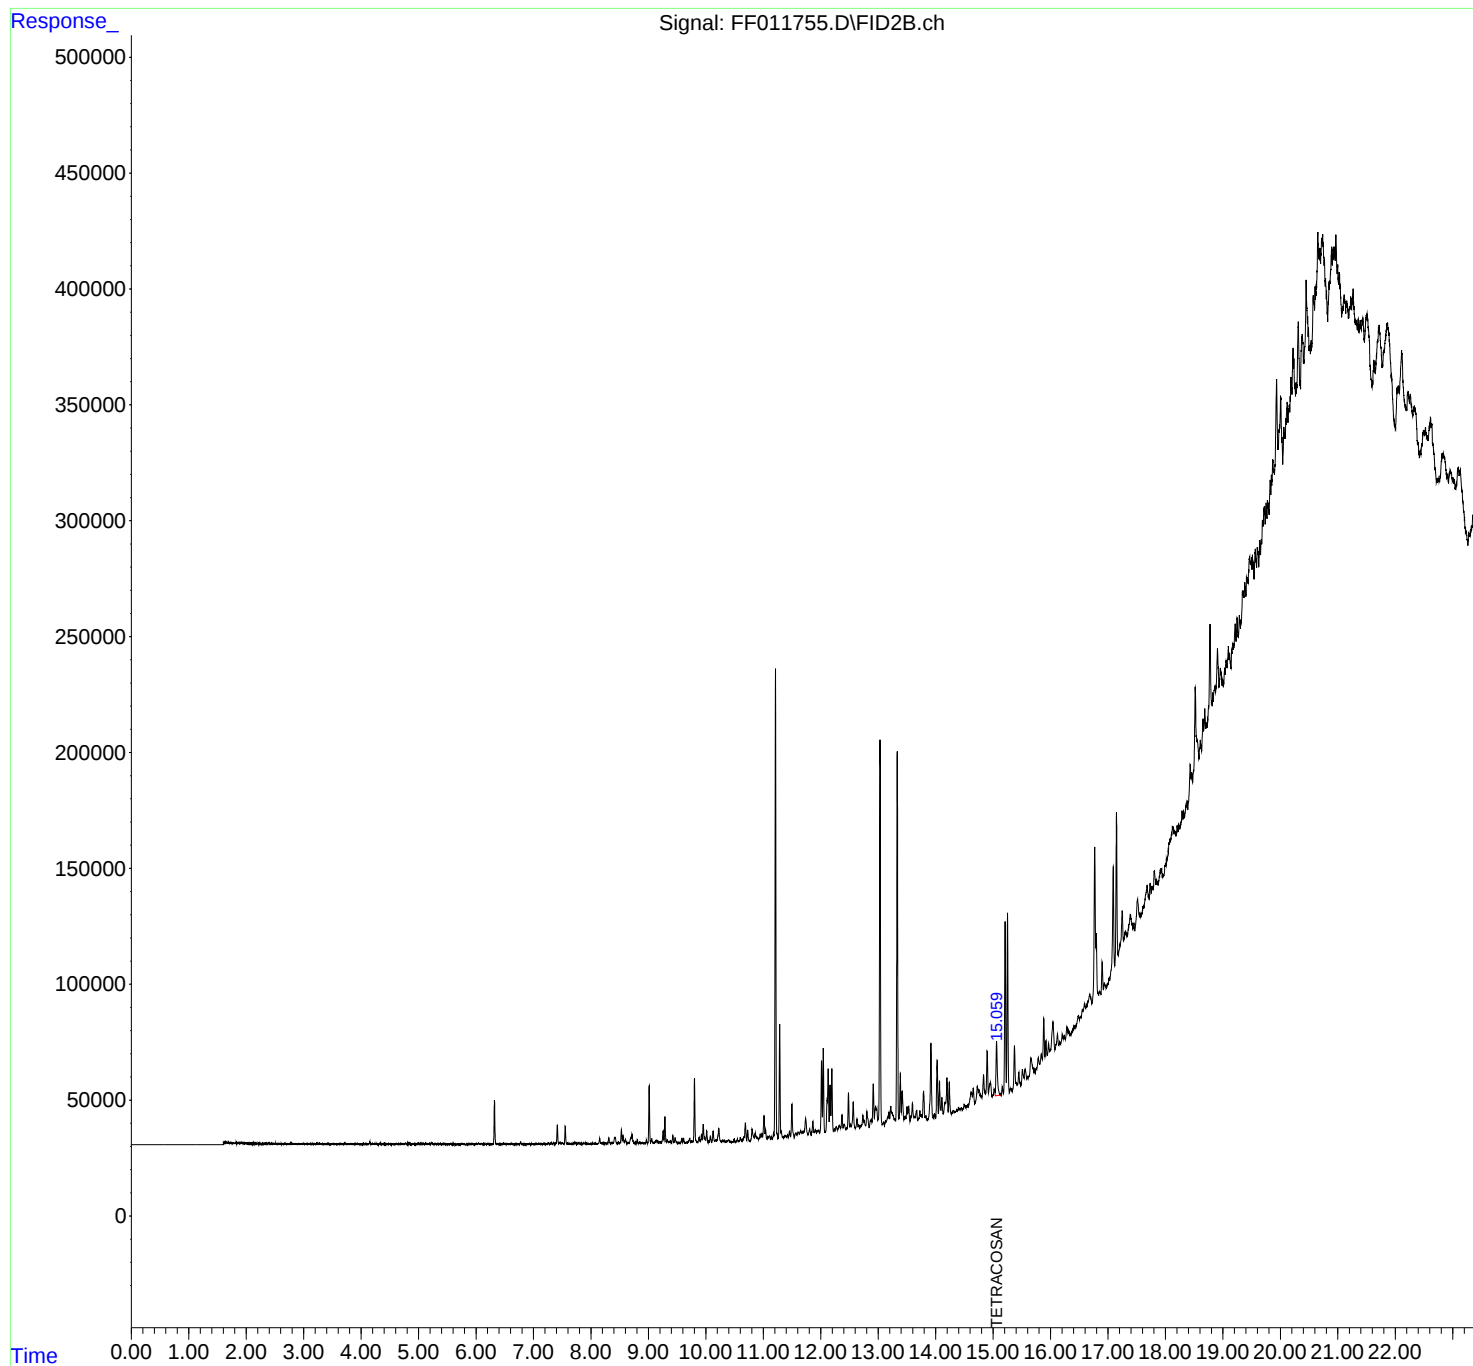

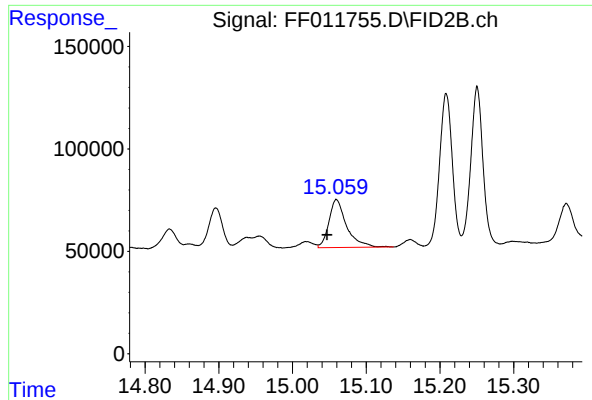

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.060 min
Delta R.T.: 0.013 min
Response: 388917
Conc: 3.28 ug/ml

Instrument :
FID_F
ClientSampleId :
SP25-10-20221201-17.5-18.0