

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002872.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 13:31
 Operator : AJ\SJ
 Sample : J5775-03 10X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:32:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	158390	2.028 ug/ml
Target Compounds			
6) N-OCTADECANE	11.281	118676	1.143 ug/ml
7) N-EICOSANE	12.593	770261	7.955 ug/ml
8) N-DOCOSANE	13.770	353635	3.862 ug/ml
10) N-TETRACOSANE	14.837	228338	2.563 ug/ml
11) N-HEXACOSANE	15.872	129727	1.429 ug/ml
12) N-OCTACOSANE	16.825	321854	3.374 ug/ml
13) N-TRIACONTANE	17.713	283385	2.859 ug/ml
14) N-DOTRIACONTANE	18.551	324664	3.280 ug/ml
15) N-TETRATRIACONTANE	19.338	134739	1.365 ug/ml
16) N-HEXATRIACONTANE	20.077	114355	1.200 ug/ml
17) N-OCTATRIACONTANE	20.822	339255	3.860 ug/ml
18) N-TETRACONTANE	21.723	618751	7.064 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002872.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 13:31
Operator : AJ\SJ
Sample : J5775-03 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:32:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

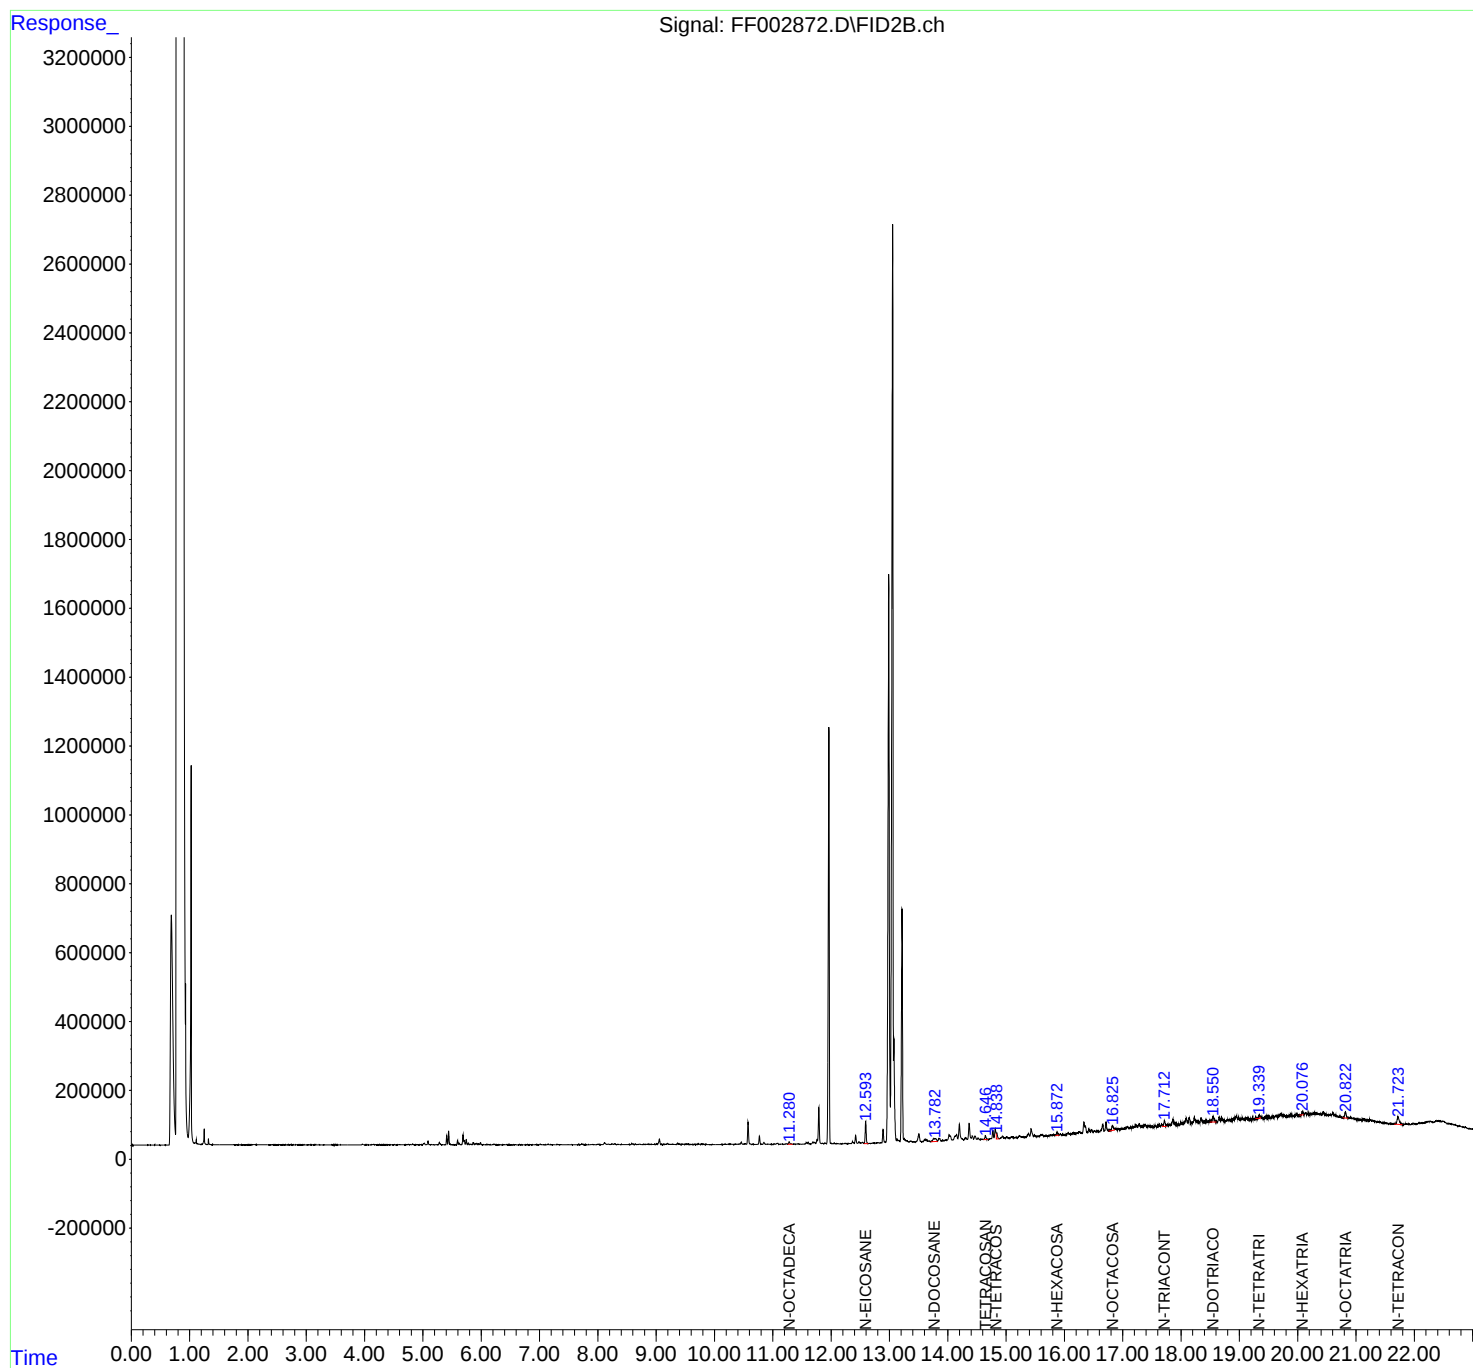

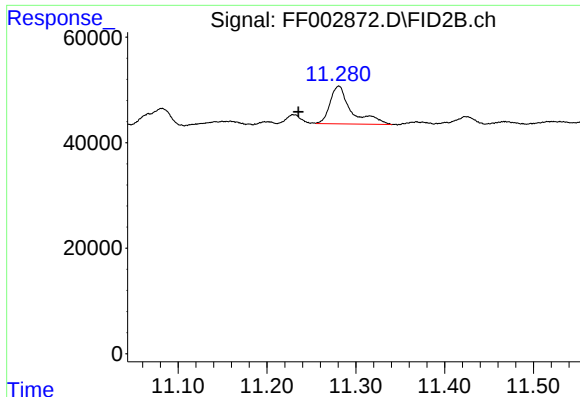


#6 N-OCTADECANE

R.T.: 11.281 min
Delta R.T.: 0.046 min
Response: 118676
Conc: 1.14 ug/ml

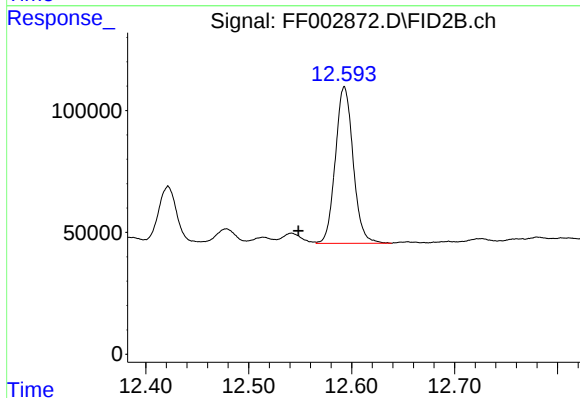


#7 N-EICOSANE

R.T.: 12.593 min
Delta R.T.: 0.045 min
Response: 770261
Conc: 7.96 ug/ml

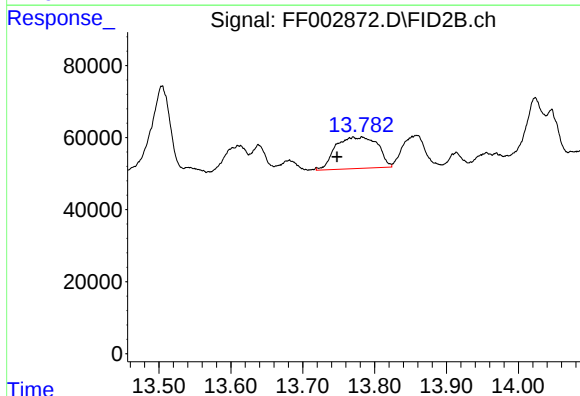


#8 N-DOCOSANE

R.T.: 13.770 min
Delta R.T.: 0.023 min
Response: 353635
Conc: 3.86 ug/ml

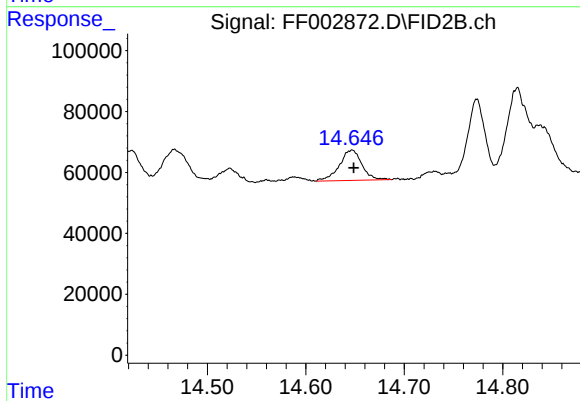


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 158390
Conc: 2.03 ug/ml

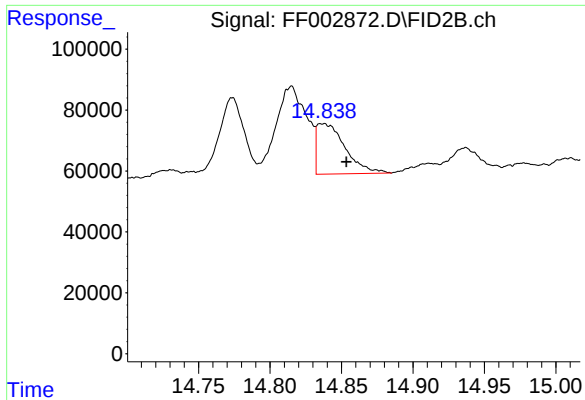


#10 N-TETRACOSANE

R.T.: 14.837 min
Delta R.T.: -0.017 min
Response: 228338
Conc: 2.56 ug/ml

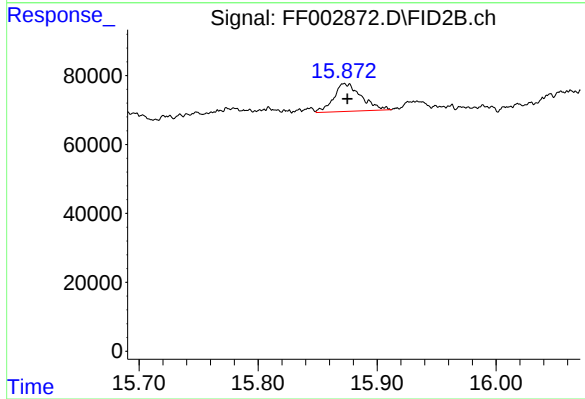


#11 N-HEXACOSANE

R.T.: 15.872 min
Delta R.T.: -0.003 min
Response: 129727
Conc: 1.43 ug/ml

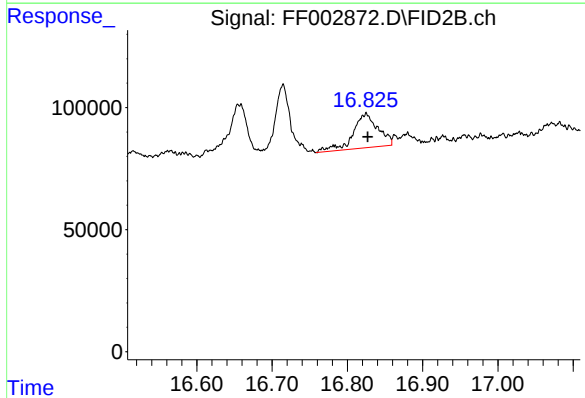


#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.002 min
Response: 321854
Conc: 3.37 ug/ml

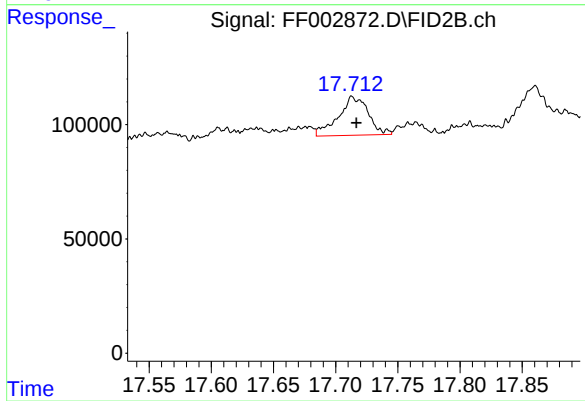


#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.003 min
Response: 283385
Conc: 2.86 ug/ml

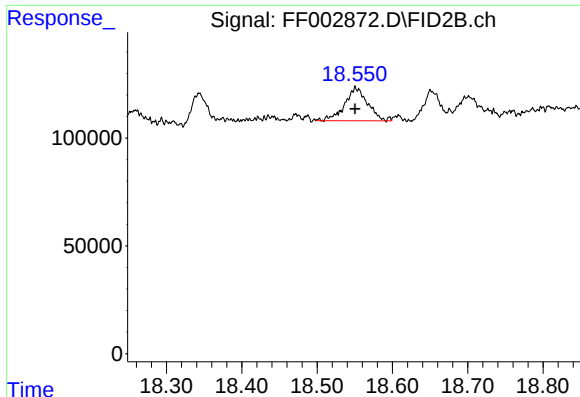


#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: 0.000 min
Response: 324664
Conc: 3.28 ug/ml

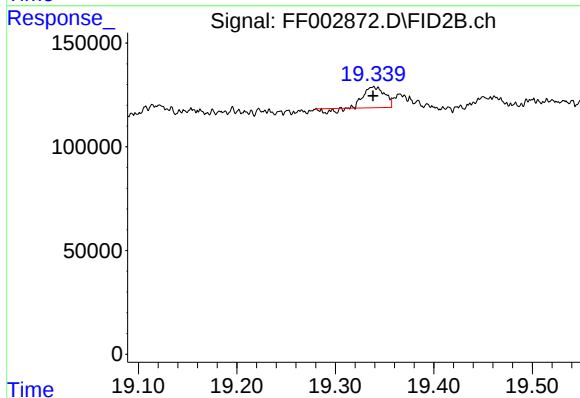


#15 N-TETRATRIACONTANE

R.T.: 19.338 min
Delta R.T.: 0.000 min
Response: 134739
Conc: 1.37 ug/ml

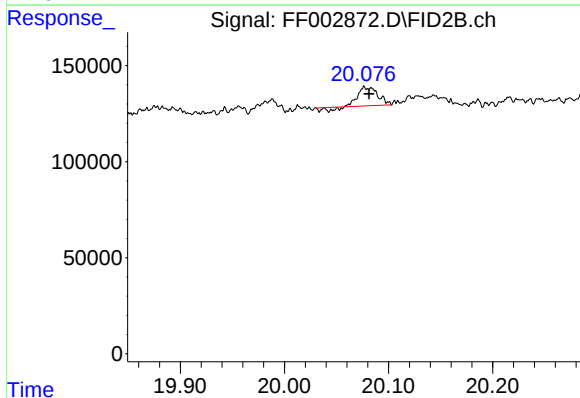


#16 N-HEXATRIACONTANE

R.T.: 20.077 min
Delta R.T.: -0.004 min
Response: 114355
Conc: 1.20 ug/ml

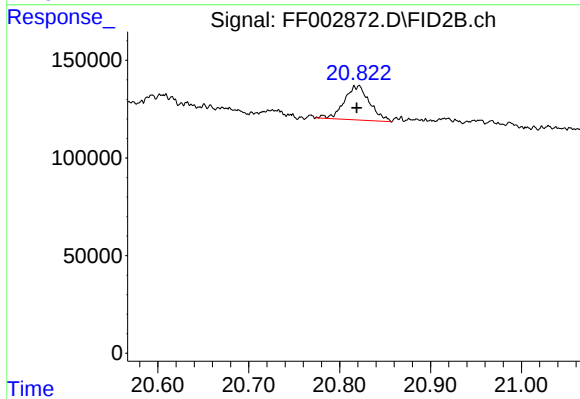

#17 N-OCTATRIACONTANE

R.T.: 20.822 min
Delta R.T.: 0.003 min
Response: 339255
Conc: 3.86 ug/ml

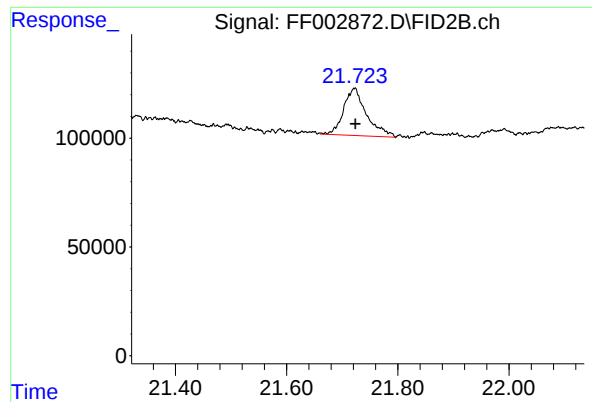

#18 N-TETRACONTANE

R.T.: 21.723 min
Delta R.T.: 0.000 min
Response: 618751
Conc: 7.06 ug/ml