

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002873.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 14:02
 Operator : AJ\SJ
 Sample : J5764-25 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:32:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.646	334441	4.281 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.184	87693	0.759 ug/ml
5)	N-HEXADECANE	9.785	103997	0.951 ug/ml
6)	N-OCTADECANE	11.229	86113	0.830 ug/ml
7)	N-EICOSANE	12.590	244441	2.525 ug/ml
10)	N-TETRACOSANE	14.812	108466	1.218 ug/ml
12)	N-OCTACOSANE	16.829	133982	1.405 ug/ml
13)	N-TRIACONTANE	17.714	199872	2.016 ug/ml
14)	N-DOTRIACONTANE	18.549	199963	2.020 ug/ml
15)	N-TETRATRIACONTANE	19.339	27583	0.279 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002873.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 14:02
Operator : AJ\SJ
Sample : J5764-25 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:32:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

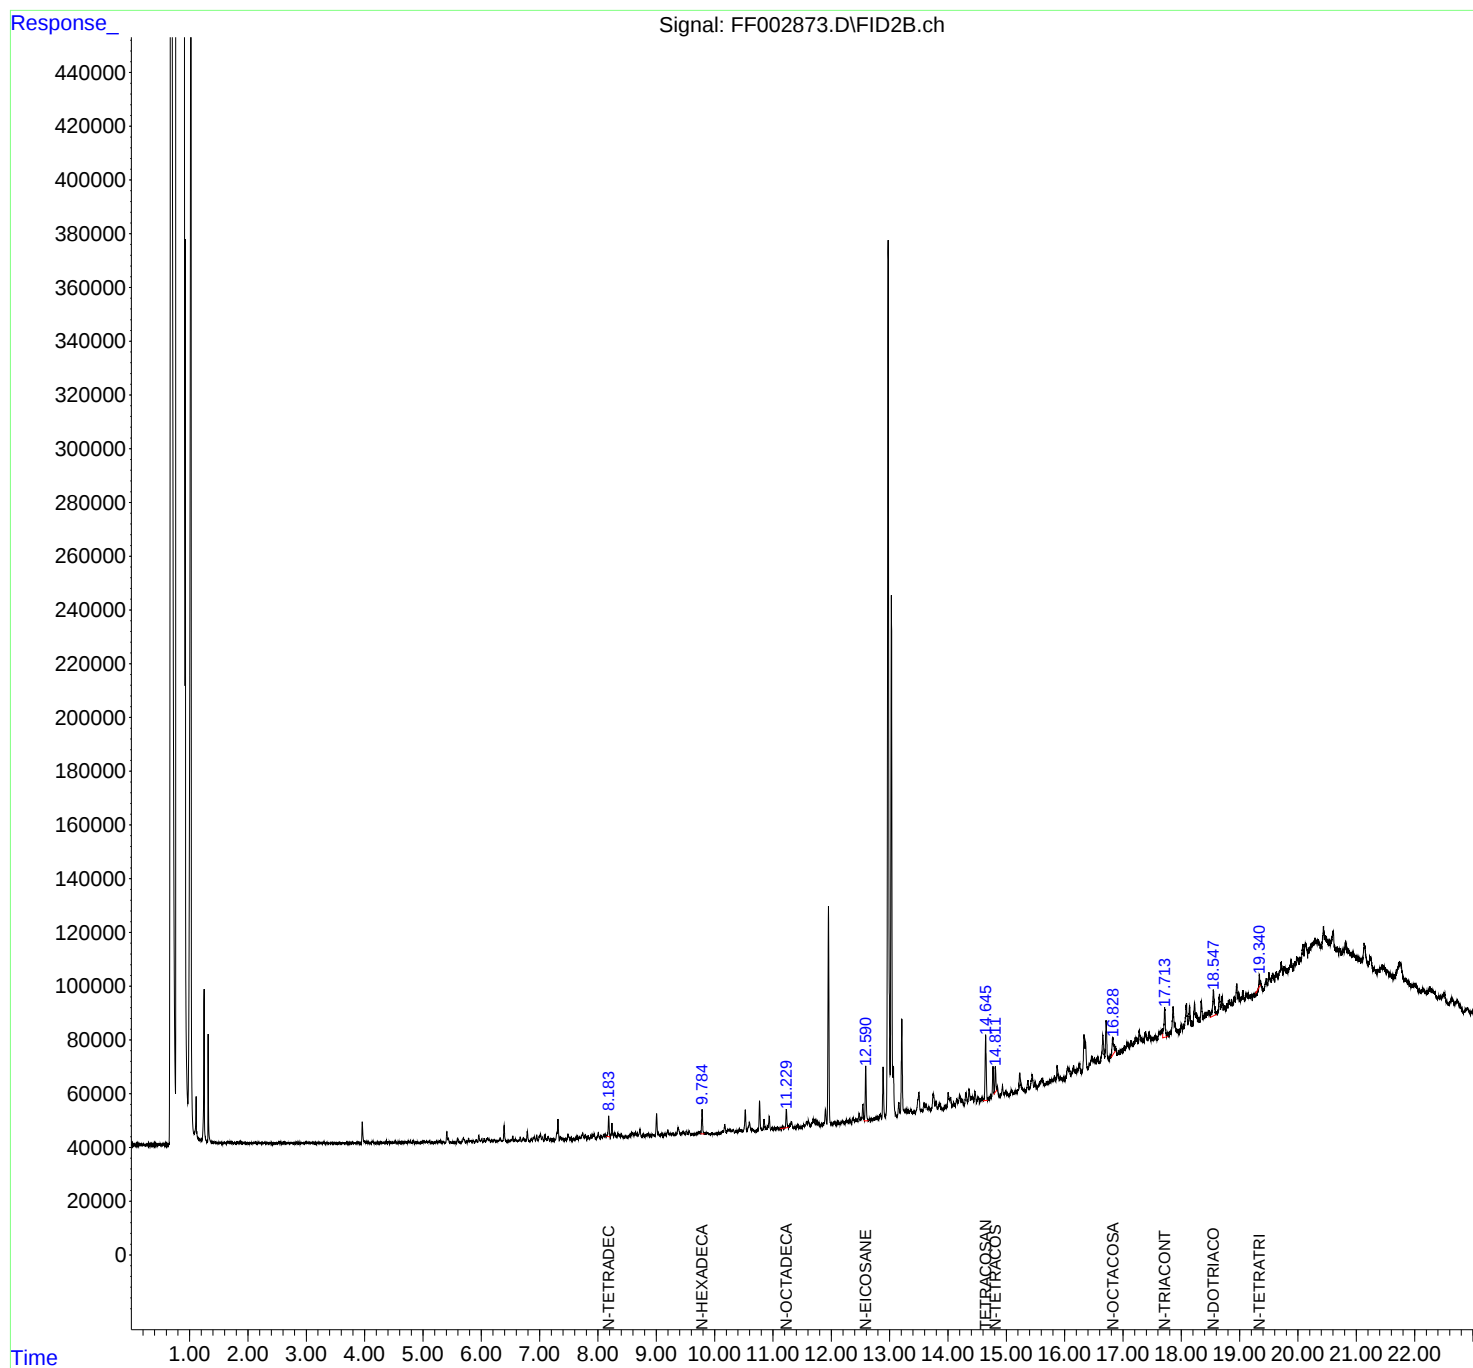

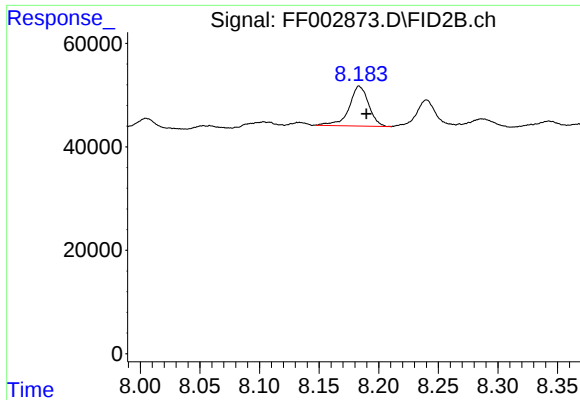


#4 N-TETRADECANE

R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 87693
Conc: 0.76 ug/ml

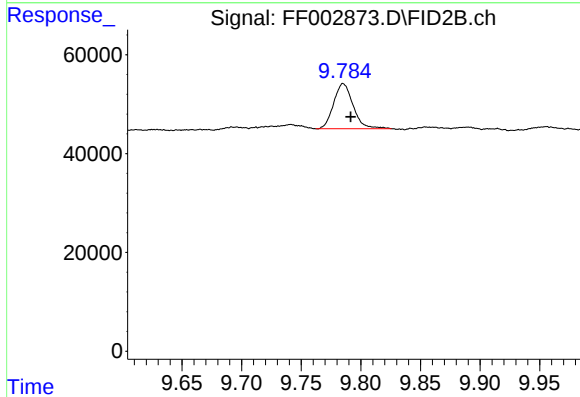


#5 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.006 min
Response: 103997
Conc: 0.95 ug/ml

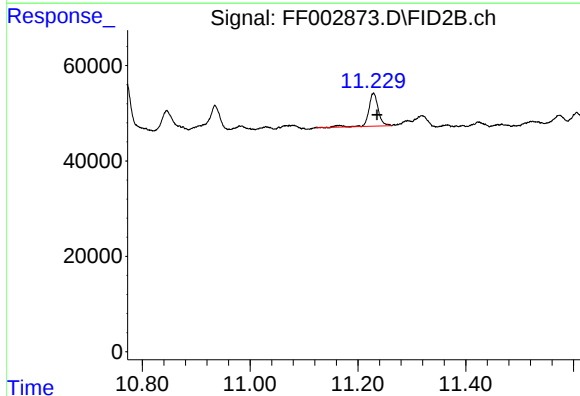


#6 N-OCTADECANE

R.T.: 11.229 min
Delta R.T.: -0.006 min
Response: 86113
Conc: 0.83 ug/ml

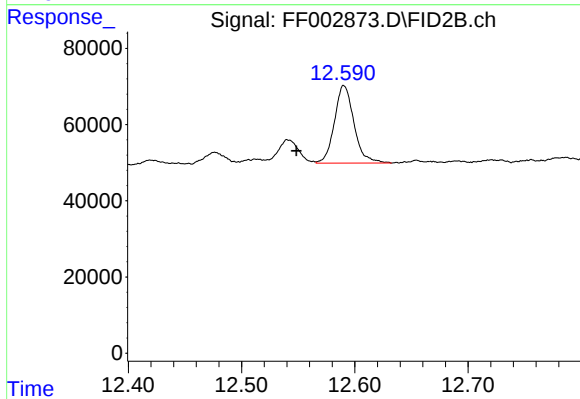


#7 N-EICOSANE

R.T.: 12.590 min
Delta R.T.: 0.042 min
Response: 244441
Conc: 2.52 ug/ml

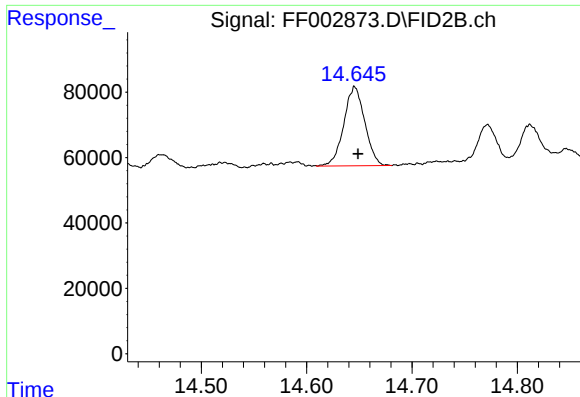


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.646 min
Delta R.T.: -0.003 min
Response: 334441
Conc: 4.28 ug/ml

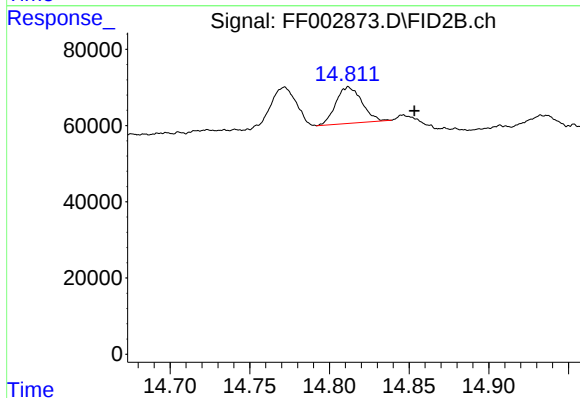


#10 N-TETRACOSANE

R.T.: 14.812 min
Delta R.T.: -0.041 min
Response: 108466
Conc: 1.22 ug/ml

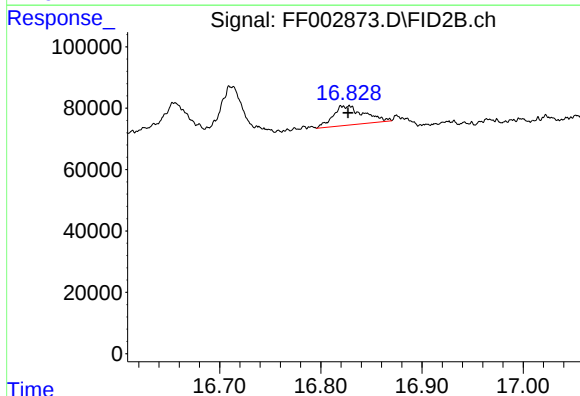


#12 N-OCTACOSANE

R.T.: 16.829 min
Delta R.T.: 0.002 min
Response: 133982
Conc: 1.40 ug/ml

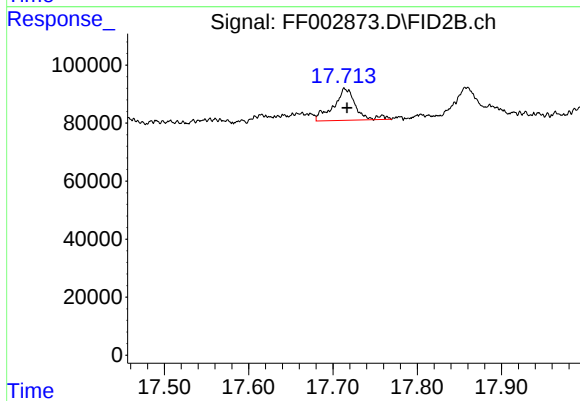


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 199872
Conc: 2.02 ug/ml

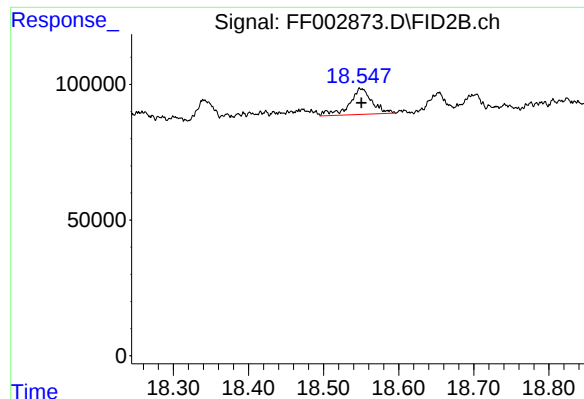

#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: -0.002 min
Response: 199963
Conc: 2.02 ug/ml

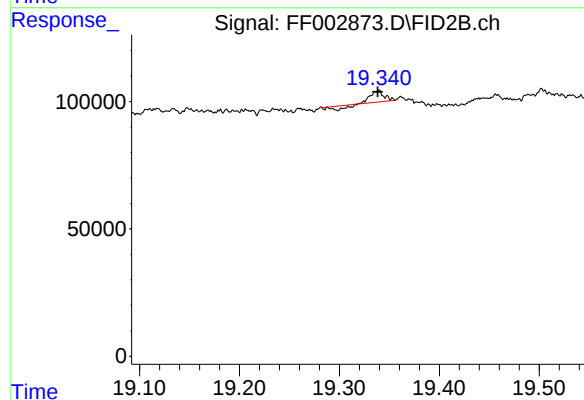

#15 N-TETRATRIACONTANE

R.T.: 19.339 min
Delta R.T.: 0.000 min
Response: 27583
Conc: 0.28 ug/ml