

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002875.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 15:03
 Operator : AJ\SJ
 Sample : J5764-21 2X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:33:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.647	771845	9.881 ug/ml
Target Compounds				
3)	N-DODECANE	6.390	390607	3.223 ug/ml
4)	N-TETRADECANE	8.184	755008	6.536 ug/ml
5)	N-HEXADECANE	9.785	790629	7.231 ug/ml
6)	N-OCTADECANE	11.229	623673	6.008 ug/ml
7)	N-EICOSANE	12.542	515114	5.320 ug/ml
8)	N-DOCOSANE	13.745	497361	5.432 ug/ml
10)	N-TETRACOSANE	14.844	490460	5.505 ug/ml
11)	N-HEXACOSANE	15.874	339994	3.746 ug/ml
12)	N-OCTACOSANE	16.825	425184	4.458 ug/ml
13)	N-TRIACONTANE	17.716	556160	5.610 ug/ml
14)	N-DOTRIACONTANE	18.552	614920	6.212 ug/ml
15)	N-TETRATRIACONTANE	19.335	419545	4.251 ug/ml
16)	N-HEXATRIACONTANE	20.081	168923	1.773 ug/ml
17)	N-OCTATRIACONTANE	20.824	244138	2.778 ug/ml
18)	N-TETRACONTANE	21.728	367994	4.201 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002875.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 15:03
Operator : AJ\SJ
Sample : J5764-21 2X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:33:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

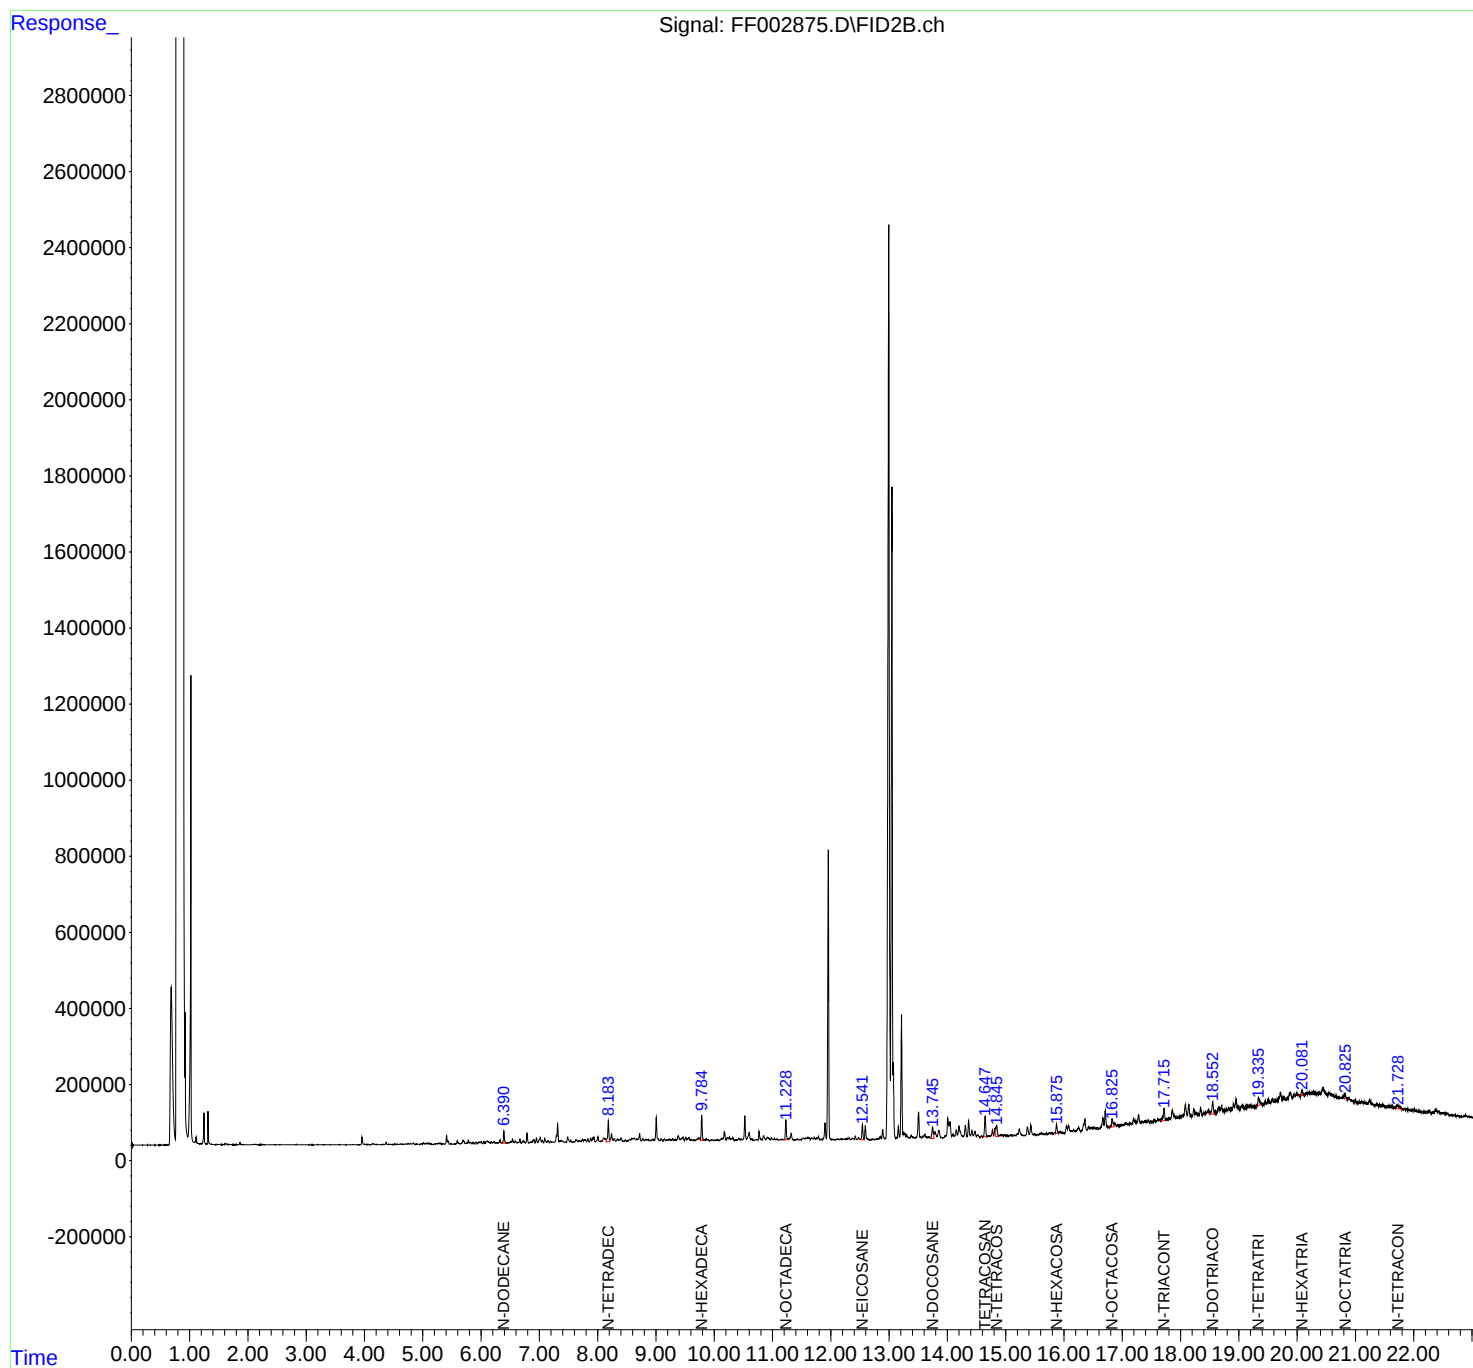

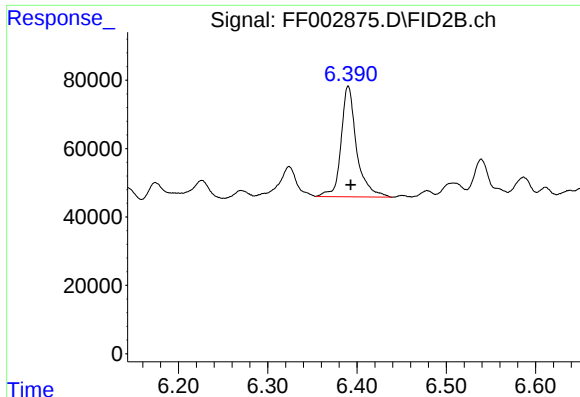


#3 N-DODECANE

R.T.: 6.390 min
Delta R.T.: -0.003 min
Response: 390607
Conc: 3.22 ug/ml

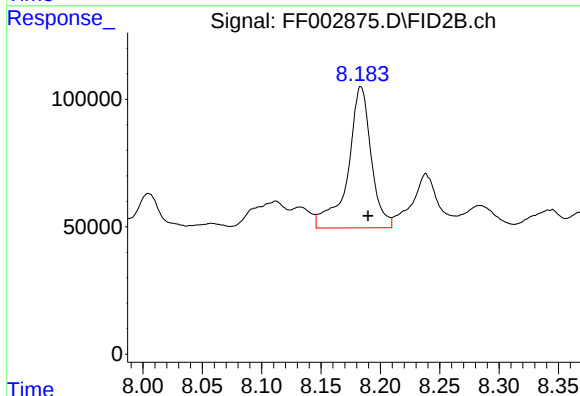


#4 N-TETRADECANE

R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 755008
Conc: 6.54 ug/ml

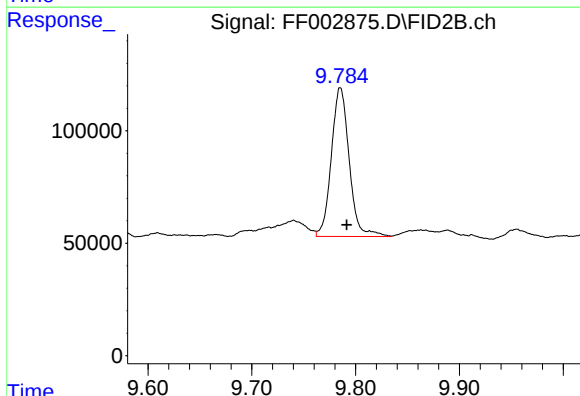


#5 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.006 min
Response: 790629
Conc: 7.23 ug/ml

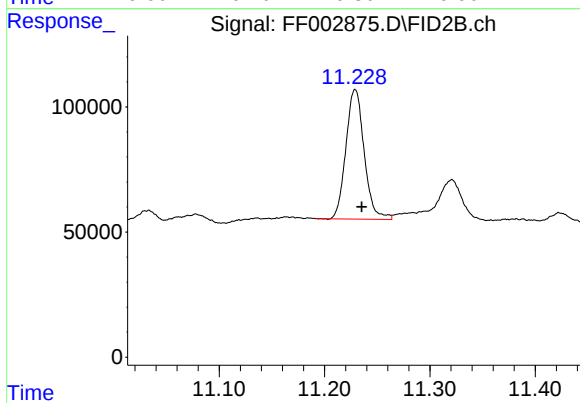


#6 N-OCTADECANE

R.T.: 11.229 min
Delta R.T.: -0.006 min
Response: 623673
Conc: 6.01 ug/ml

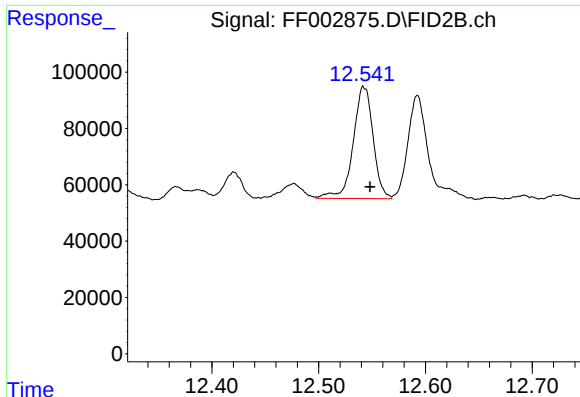


#7 N-EICOSANE

R.T.: 12.542 min
Delta R.T.: -0.006 min
Response: 515114
Conc: 5.32 ug/ml

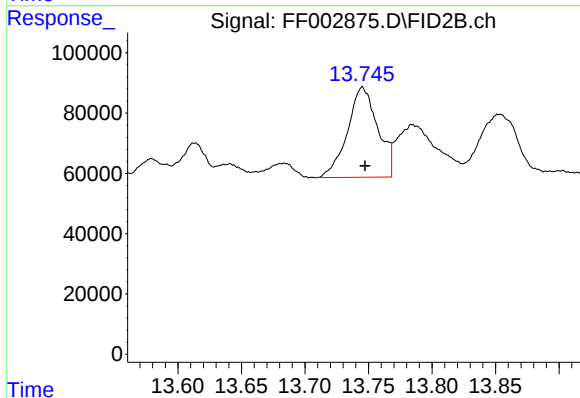


#8 N-DOCOSANE

R.T.: 13.745 min
Delta R.T.: -0.002 min
Response: 497361
Conc: 5.43 ug/ml

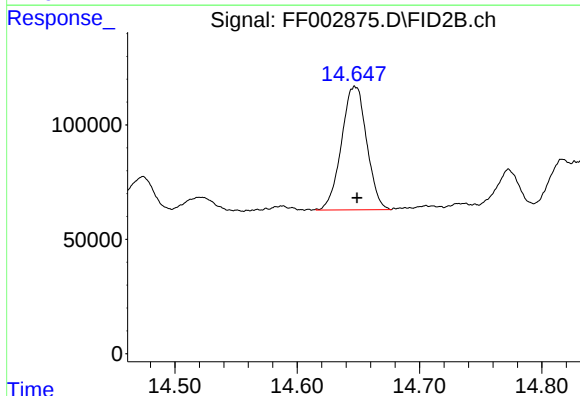


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.001 min
Response: 771845
Conc: 9.88 ug/ml

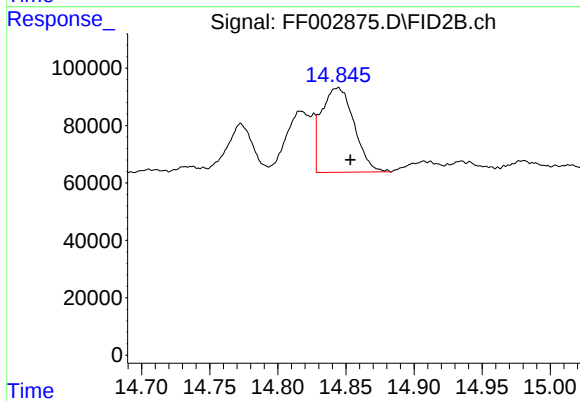


#10 N-TETRACOSANE

R.T.: 14.844 min
Delta R.T.: -0.010 min
Response: 490460
Conc: 5.51 ug/ml

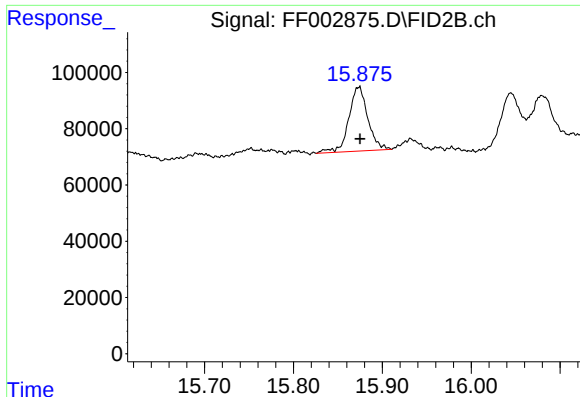


#11 N-HEXACOSANE

R.T.: 15.874 min
Delta R.T.: -0.001 min
Response: 339994
Conc: 3.75 ug/ml

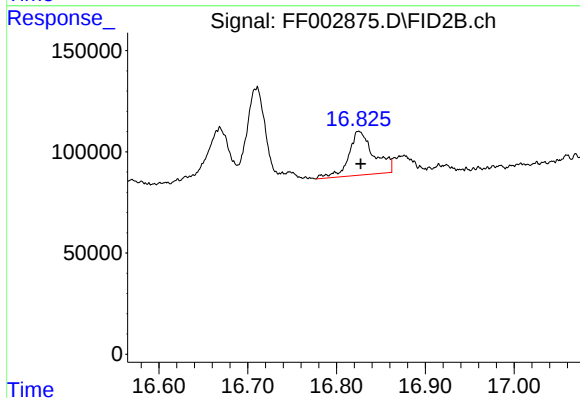


#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.002 min
Response: 425184
Conc: 4.46 ug/ml

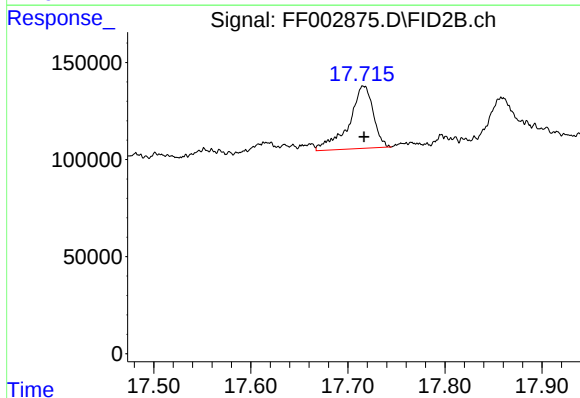


#13 N-TRIACONTANE

R.T.: 17.716 min
Delta R.T.: 0.000 min
Response: 556160
Conc: 5.61 ug/ml

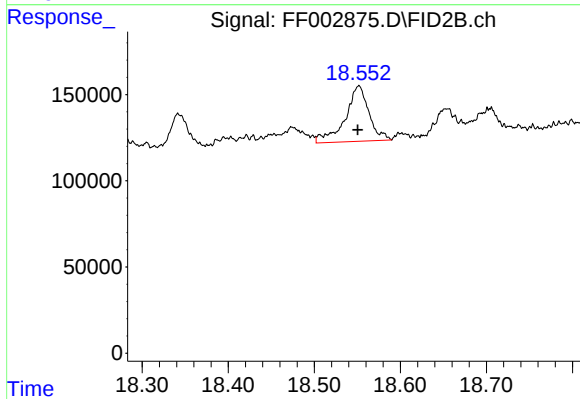


#14 N-DOTRIACONTANE

R.T.: 18.552 min
Delta R.T.: 0.001 min
Response: 614920
Conc: 6.21 ug/ml

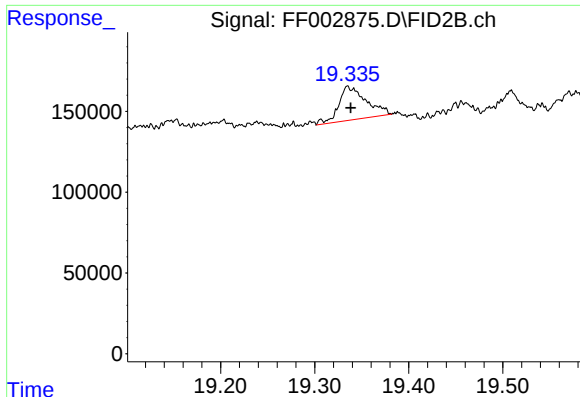


#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: -0.004 min
Response: 419545
Conc: 4.25 ug/ml

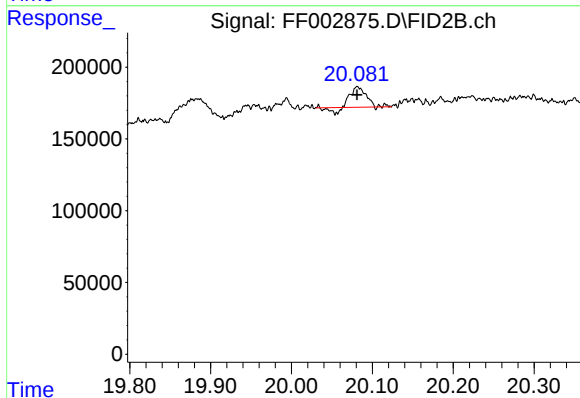


#16 N-HEXATRIACONTANE

R.T.: 20.081 min
Delta R.T.: 0.000 min
Response: 168923
Conc: 1.77 ug/ml

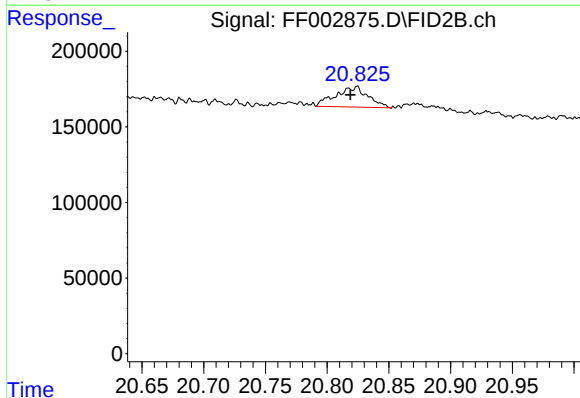

#17 N-OCTATRIACONTANE

R.T.: 20.824 min
Delta R.T.: 0.006 min
Response: 244138
Conc: 2.78 ug/ml

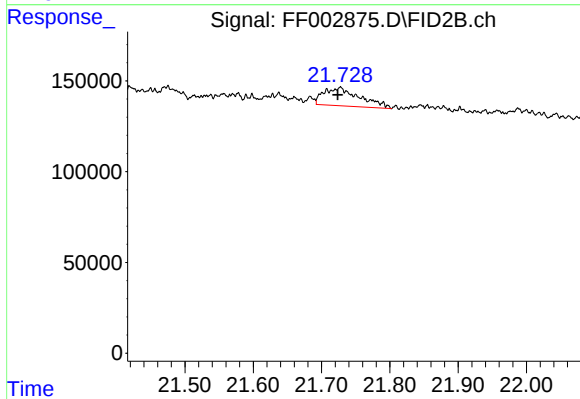

#18 N-TETRACONTANE

R.T.: 21.728 min
Delta R.T.: 0.004 min
Response: 367994
Conc: 4.20 ug/ml