

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002877.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 16:04
 Operator : AJ\SJ
 Sample : J5764-29 2X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:33:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.647	953525	12.206 ug/ml
Target Compounds				
3)	N-DODECANE	6.391	372373	3.072 ug/ml
4)	N-TETRADECANE	8.184	732195	6.338 ug/ml
5)	N-HEXADECANE	9.785	729957	6.676 ug/ml
6)	N-OCTADECANE	11.230	620019	5.973 ug/ml
7)	N-EICOSANE	12.542	475168	4.908 ug/ml
8)	N-DOCOSANE	13.744	462653	5.053 ug/ml
10)	N-TETRACOSANE	14.846	387809	4.353 ug/ml
11)	N-HEXACOSANE	15.873	368428	4.060 ug/ml
12)	N-OCTACOSANE	16.828	742183	7.781 ug/ml
13)	N-TRIACONTANE	17.717	553074	5.579 ug/ml
14)	N-DOTRIACONTANE	18.553	800435	8.086 ug/ml
15)	N-TETRATRIACONTANE	19.338	534123	5.412 ug/ml
16)	N-HEXATRIACONTANE	20.081	190492	1.999 ug/ml
17)	N-OCTATRIACONTANE	20.822	680951	7.748 ug/ml
18)	N-TETRACONTANE	21.722	292773	3.342 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002877.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 16:04
Operator : AJ\SJ
Sample : J5764-29 2X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:33:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

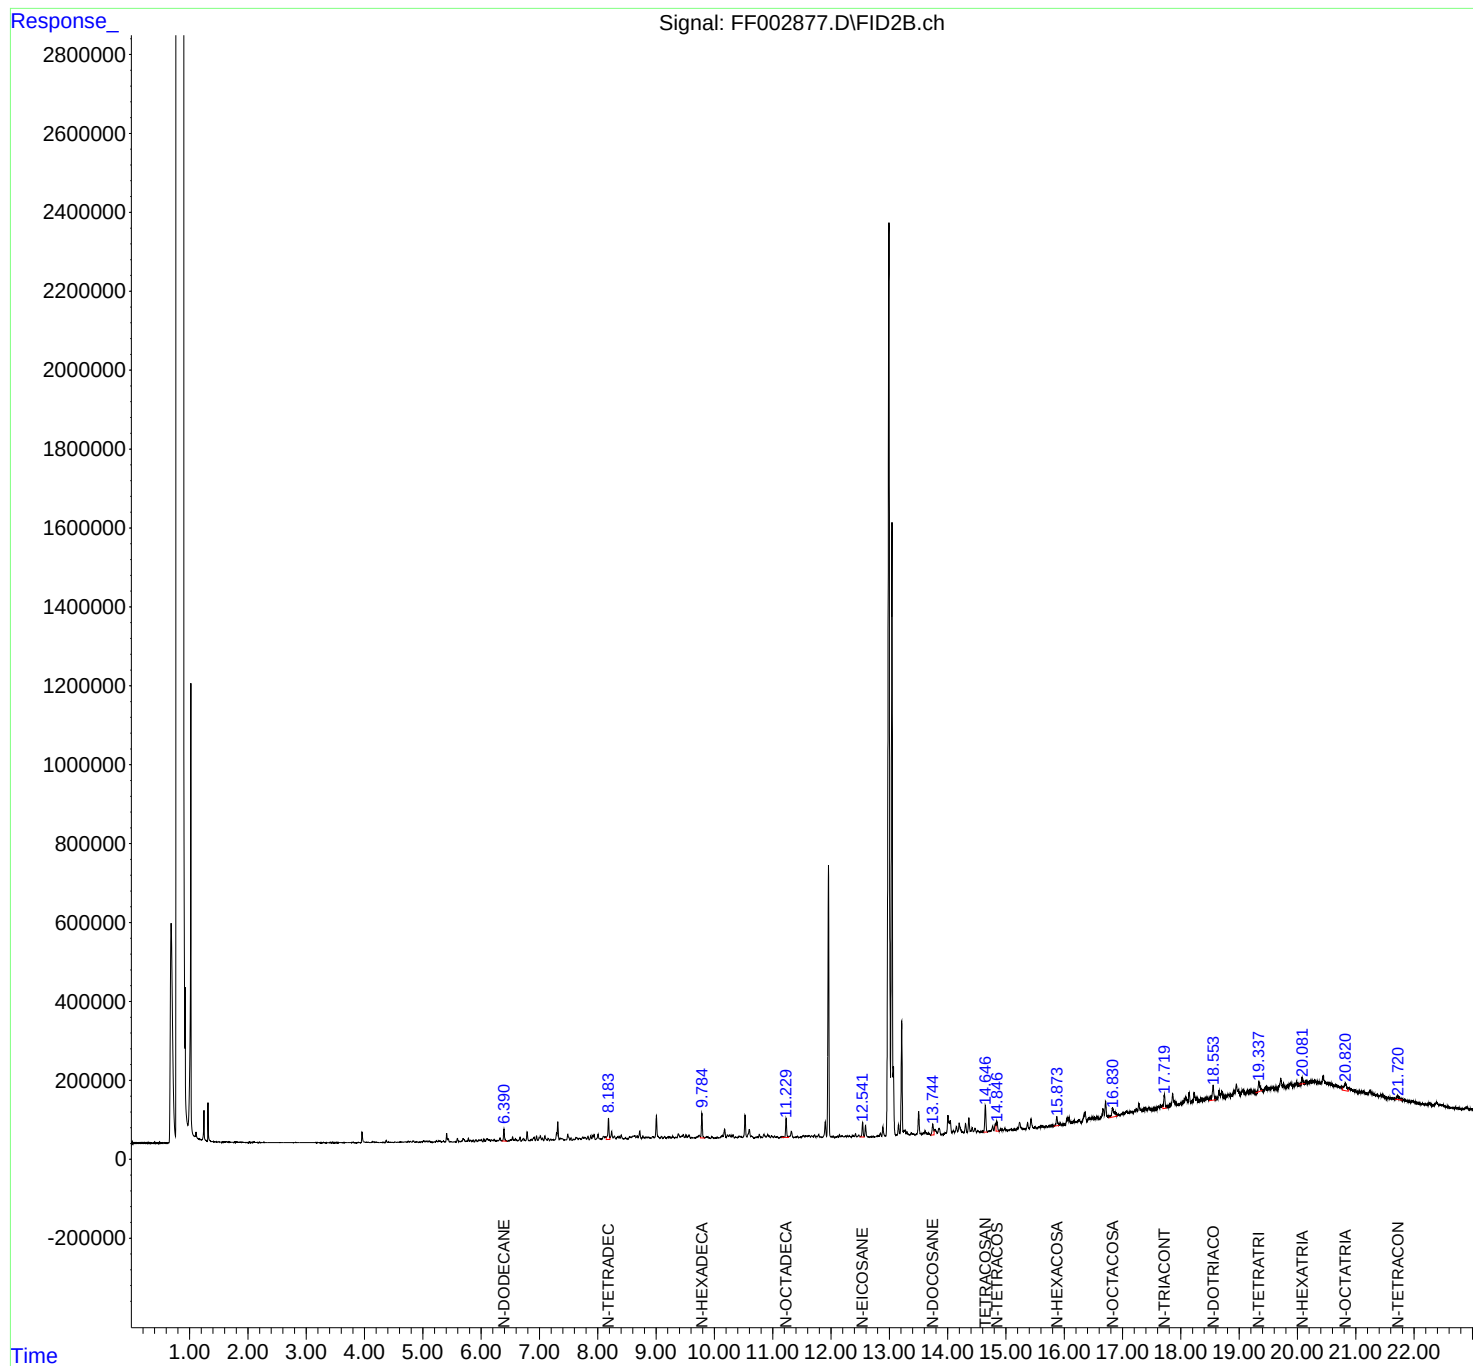

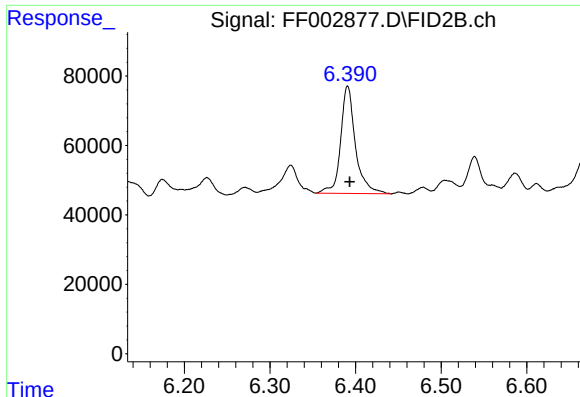


#3 N-DODECANE

R.T.: 6.391 min
Delta R.T.: -0.002 min
Response: 372373
Conc: 3.07 ug/ml

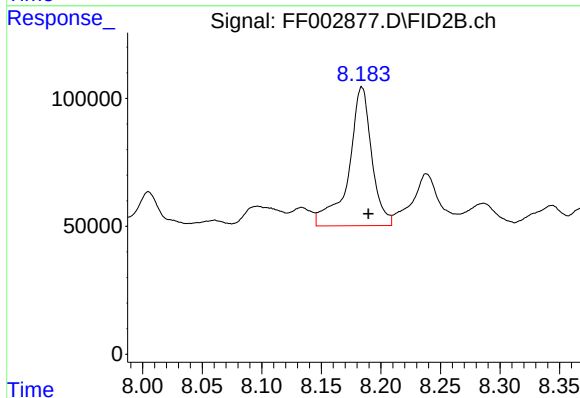


#4 N-TETRADECANE

R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 732195
Conc: 6.34 ug/ml

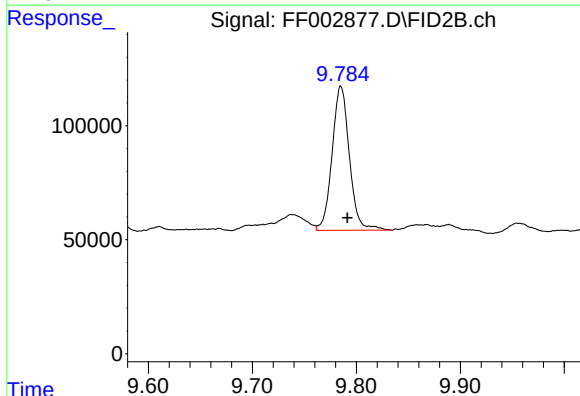


#5 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.006 min
Response: 729957
Conc: 6.68 ug/ml

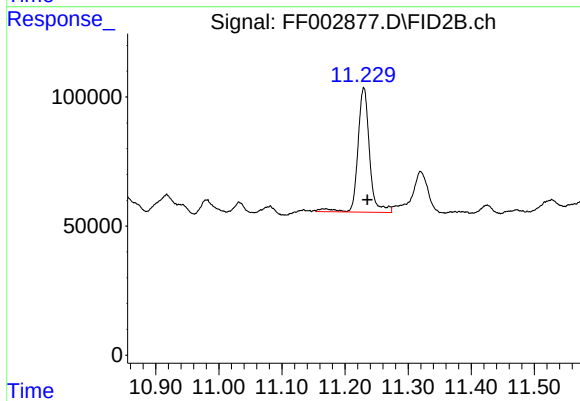


#6 N-OCTADECANE

R.T.: 11.230 min
Delta R.T.: -0.006 min
Response: 620019
Conc: 5.97 ug/ml

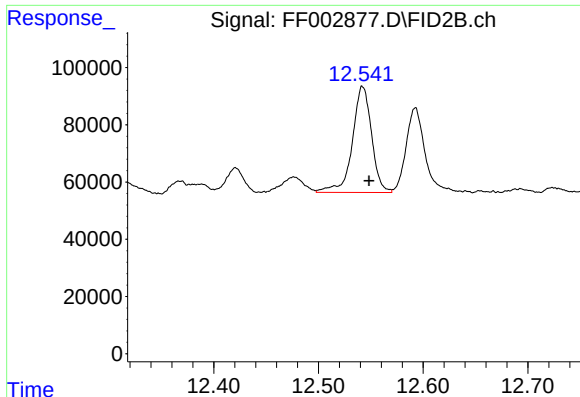


#7 N-EICOSANE

R.T.: 12.542 min
Delta R.T.: -0.006 min
Response: 475168
Conc: 4.91 ug/ml

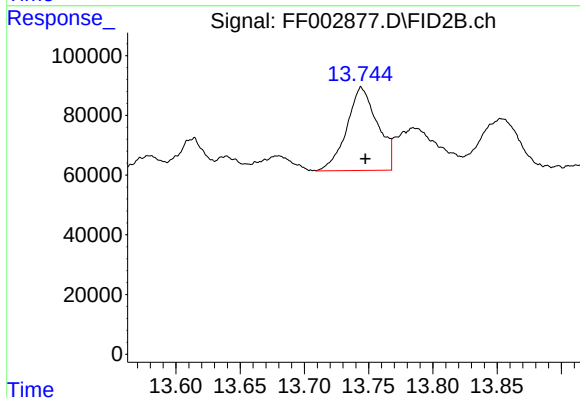


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: -0.003 min
Response: 462653
Conc: 5.05 ug/ml

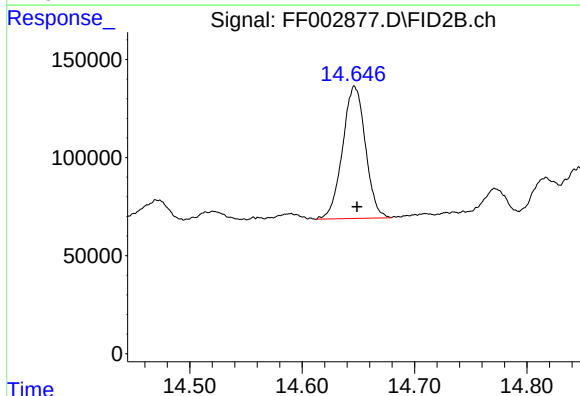


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 953525
Conc: 12.21 ug/ml

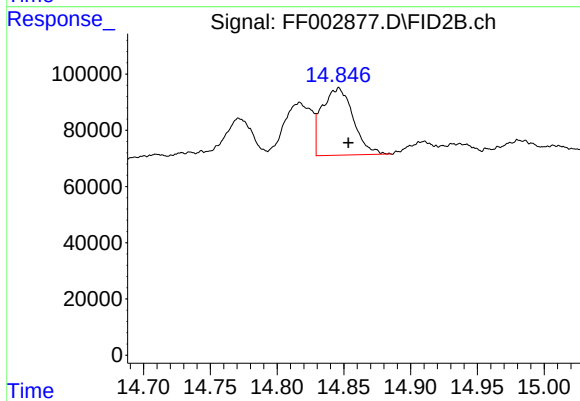


#10 N-TETRACOSANE

R.T.: 14.846 min
Delta R.T.: -0.007 min
Response: 387809
Conc: 4.35 ug/ml

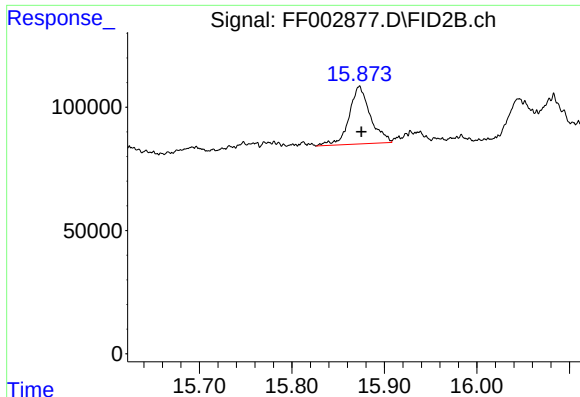


#11 N-HEXACOSANE

R.T.: 15.873 min
Delta R.T.: -0.002 min
Response: 368428
Conc: 4.06 ug/ml

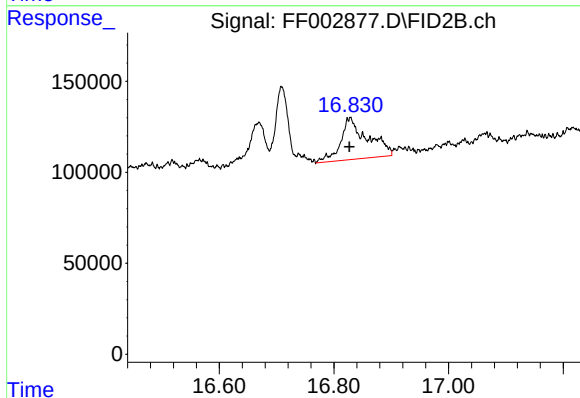


#12 N-OCTACOSANE

R.T.: 16.828 min
Delta R.T.: 0.000 min
Response: 742183
Conc: 7.78 ug/ml

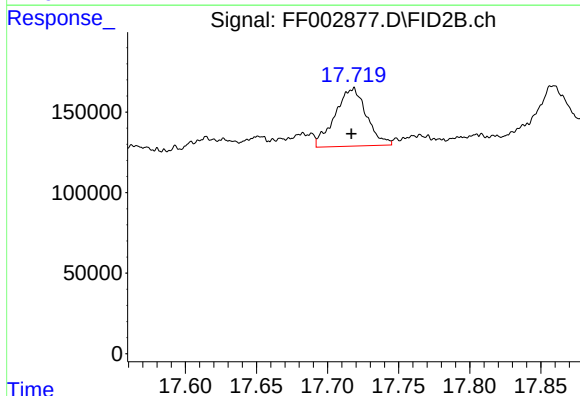


#13 N-TRIACONTANE

R.T.: 17.717 min
Delta R.T.: 0.000 min
Response: 553074
Conc: 5.58 ug/ml

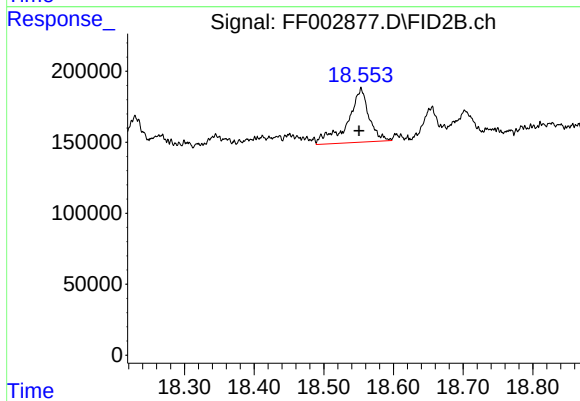


#14 N-DOTRIACONTANE

R.T.: 18.553 min
Delta R.T.: 0.003 min
Response: 800435
Conc: 8.09 ug/ml

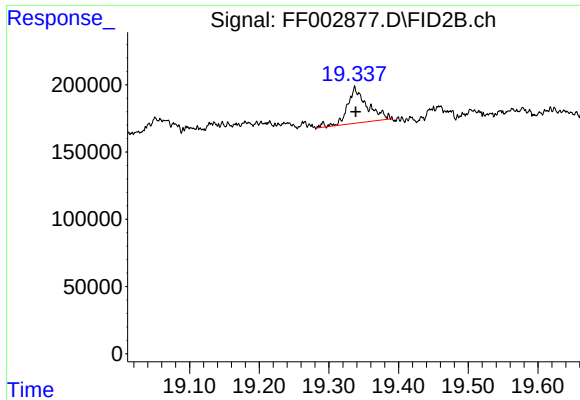


#15 N-TETRATRIACONTANE

R.T.: 19.338 min
Delta R.T.: 0.000 min
Response: 534123
Conc: 5.41 ug/ml

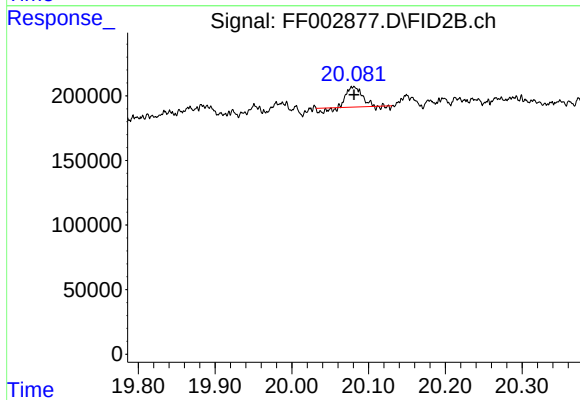


#16 N-HEXATRIACONTANE

R.T.: 20.081 min
Delta R.T.: 0.000 min
Response: 190492
Conc: 2.00 ug/ml

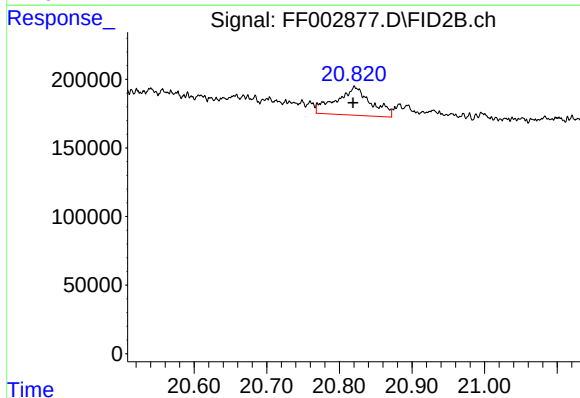

#17 N-OCTATRIACONTANE

R.T.: 20.822 min
Delta R.T.: 0.003 min
Response: 680951
Conc: 7.75 ug/ml

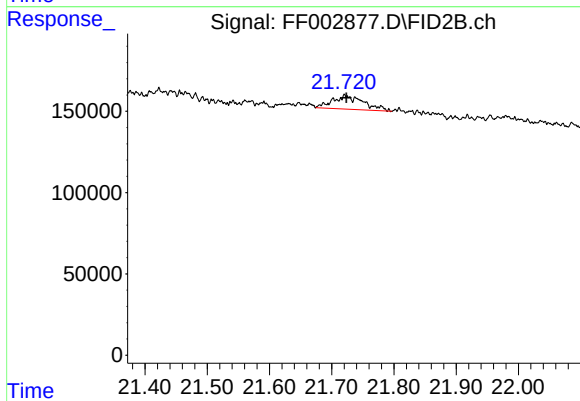

#18 N-TETRACONTANE

R.T.: 21.722 min
Delta R.T.: -0.001 min
Response: 292773
Conc: 3.34 ug/ml