

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120318\  
Data File : FF002880.D  
Signal(s) : FID2B.ch  
Acq On : 03 Dec 2018 17:36  
Operator : AJ\SJ  
Sample : J5775-03 20X  
Misc :  
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Dec 04 01:33:57 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF111418.M  
Quant Title :  
QLast Update : Wed Nov 14 13:46:00 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 7) N-EICOSANE               | 12.591 | 363387   | 3.753 ug/ml |
| 10) N-TETRACOSANE           | 14.839 | 117576   | 1.320 ug/ml |
| 12) N-OCTACOSANE            | 16.822 | 137943   | 1.446 ug/ml |
| 13) N-TRIACONTANE           | 17.714 | 224495   | 2.265 ug/ml |
| 14) N-DOTRIACONTANE         | 18.548 | 352428   | 3.560 ug/ml |
| 15) N-TETRATRIACONTANE      | 19.333 | 25790    | 0.261 ug/ml |
| 16) N-HEXATRIACONTANE       | 20.076 | 95910    | 1.006 ug/ml |
| 17) N-OCTATRIACONTANE       | 20.822 | 134760   | 1.533 ug/ml |
| 18) N-TETRACONTANE          | 21.756 | 495910   | 5.661 ug/ml |
| -----                       |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120318\  
Data File : FF002880.D  
Signal(s) : FID2B.ch  
Acq On : 03 Dec 2018 17:36  
Operator : AJ\SJ  
Sample : J5775-03 20X  
Misc :  
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Dec 04 01:33:57 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF111418.M  
Quant Title :  
QLast Update : Wed Nov 14 13:46:00 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

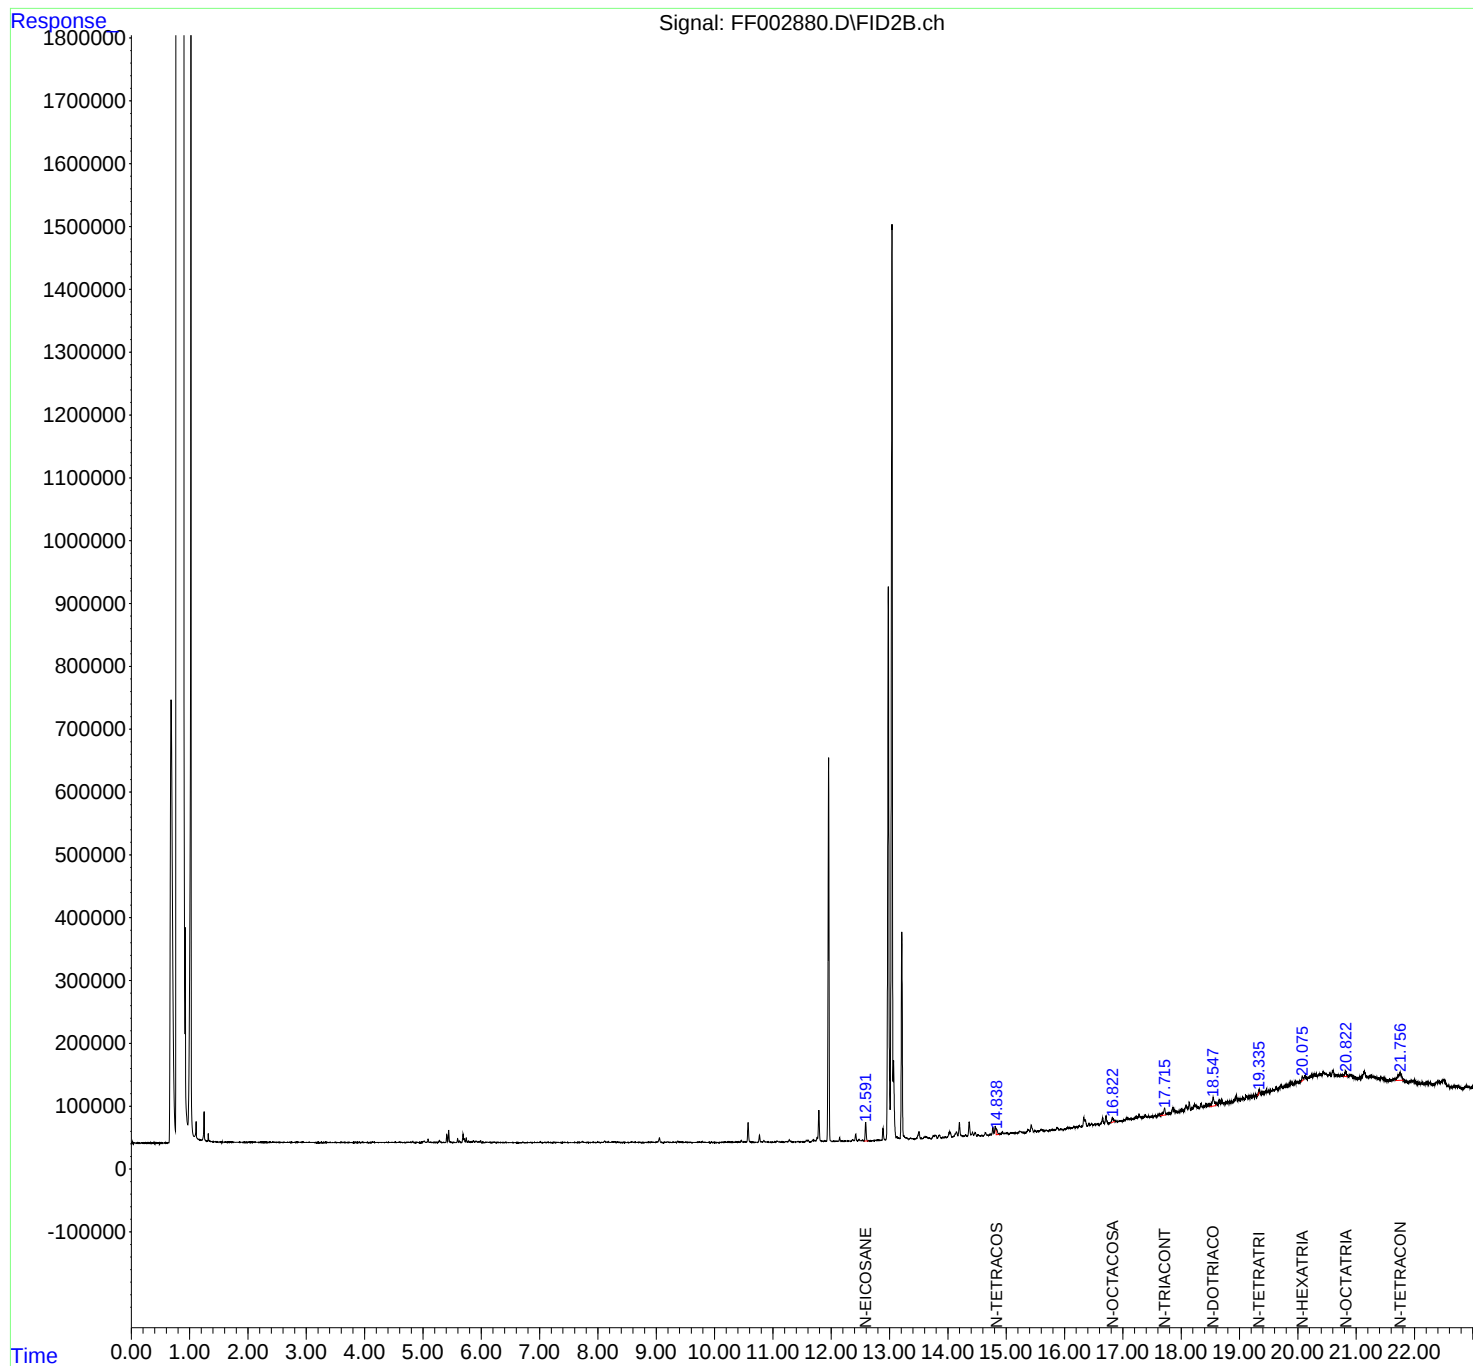

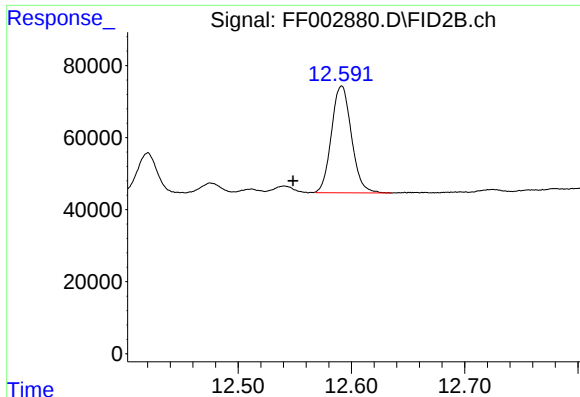


#7 N-EICOSANE

R.T.: 12.591 min  
Delta R.T.: 0.043 min  
Response: 363387  
Conc: 3.75 ug/ml

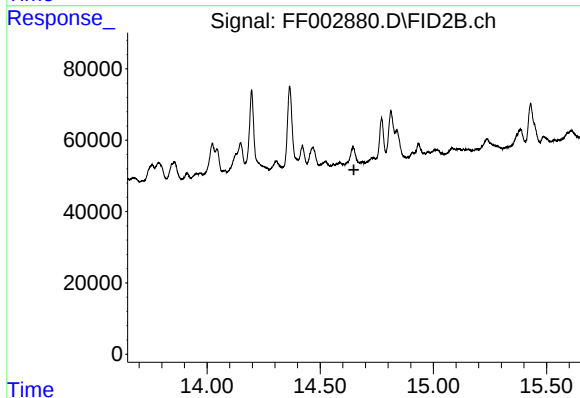


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.649 min  
Response: 0  
Conc: N.D.

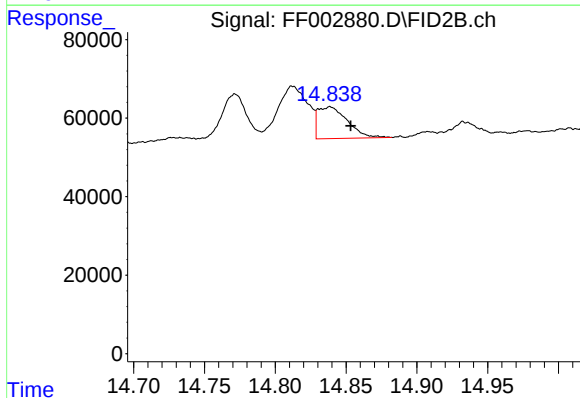


#10 N-TETRACOSANE

R.T.: 14.839 min  
Delta R.T.: -0.015 min  
Response: 117576  
Conc: 1.32 ug/ml

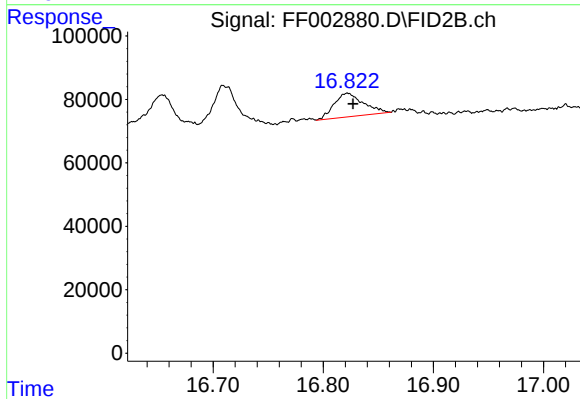


#12 N-OCTACOSANE

R.T.: 16.822 min  
Delta R.T.: -0.005 min  
Response: 137943  
Conc: 1.45 ug/ml

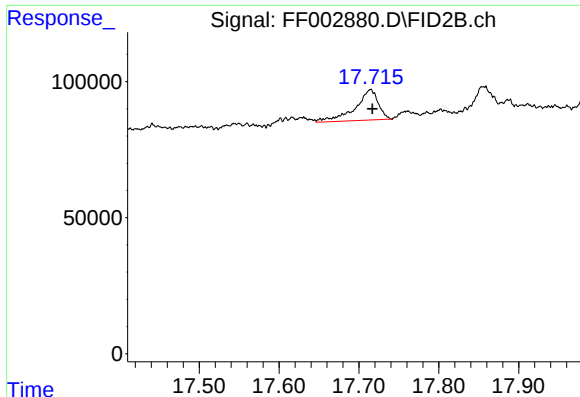


#13 N-TRIACONTANE

R.T.: 17.714 min  
Delta R.T.: -0.002 min  
Response: 224495  
Conc: 2.26 ug/ml

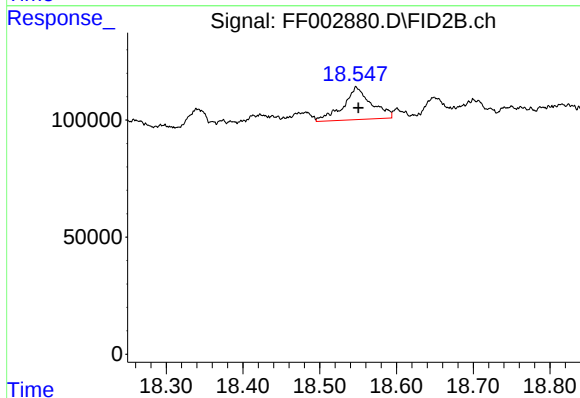


#14 N-DOTRIACONTANE

R.T.: 18.548 min  
Delta R.T.: -0.003 min  
Response: 352428  
Conc: 3.56 ug/ml

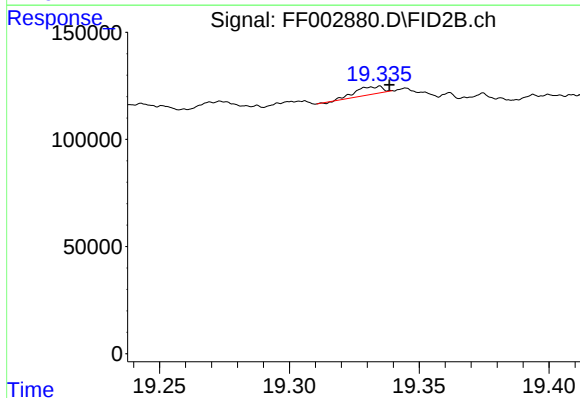


#15 N-TETRATRIACONTANE

R.T.: 19.333 min  
Delta R.T.: -0.005 min  
Response: 25790  
Conc: 0.26 ug/ml

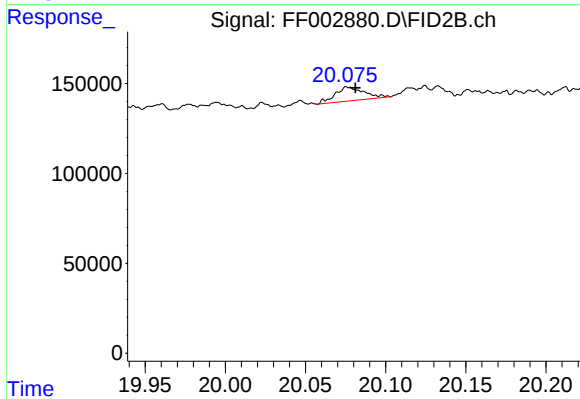


#16 N-HEXATRIACONTANE

R.T.: 20.076 min  
Delta R.T.: -0.005 min  
Response: 95910  
Conc: 1.01 ug/ml

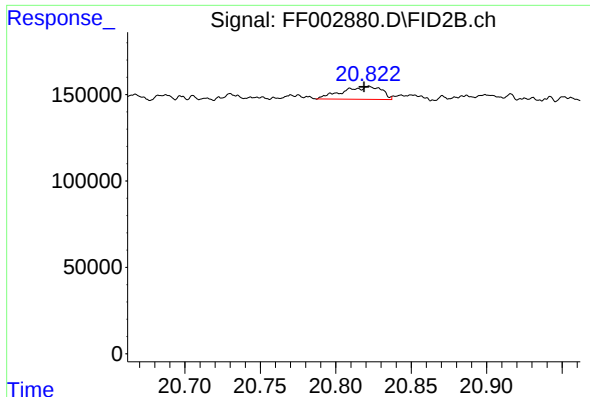

#17 N-OCTATRIACONTANE

R.T.: 20.822 min  
Delta R.T.: 0.003 min  
Response: 134760  
Conc: 1.53 ug/ml

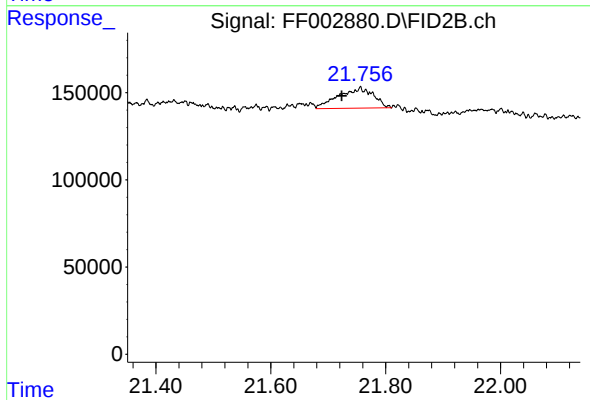

#18 N-TETRACONTANE

R.T.: 21.756 min  
Delta R.T.: 0.032 min  
Response: 495910  
Conc: 5.66 ug/ml