

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002882.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 18:37
 Operator : AJ\SJ
 Sample : J5764-21 10X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:34:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.644	150834	1.931 ug/ml
Target Compounds			
4) N-TETRADECANE	8.183	110111	0.953 ug/ml
5) N-HEXADECANE	9.785	140609	1.286 ug/ml
6) N-OCTADECANE	11.228	112488	1.084 ug/ml
7) N-EICOSANE	12.541	92364	0.954 ug/ml
13) N-TRIACONTANE	17.713	157363	1.587 ug/ml
14) N-DOTRIACONTANE	18.549	218467	2.207 ug/ml
15) N-TETRATRIACONTANE	19.333	148174	1.501 ug/ml
16) N-HEXATRIACONTANE	20.082	68688	0.721 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002882.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 18:37
Operator : AJ\SJ
Sample : J5764-21 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:34:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

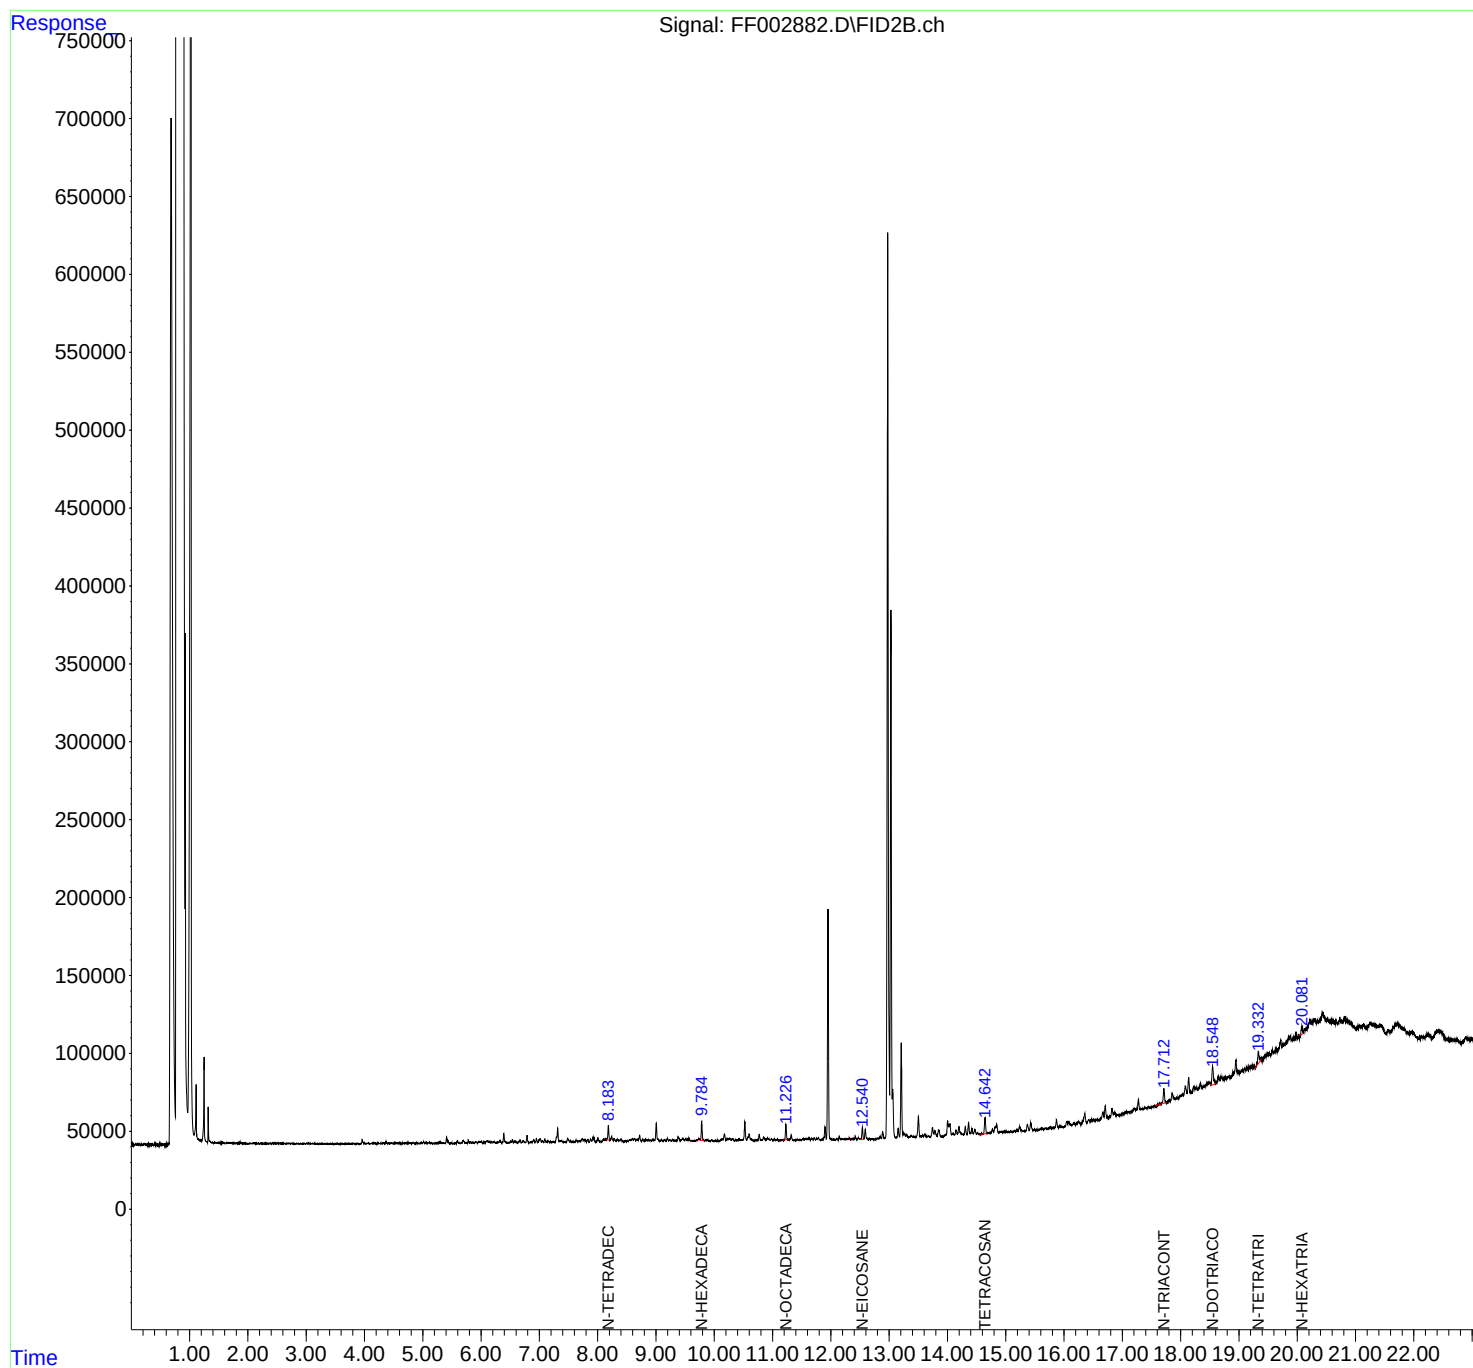

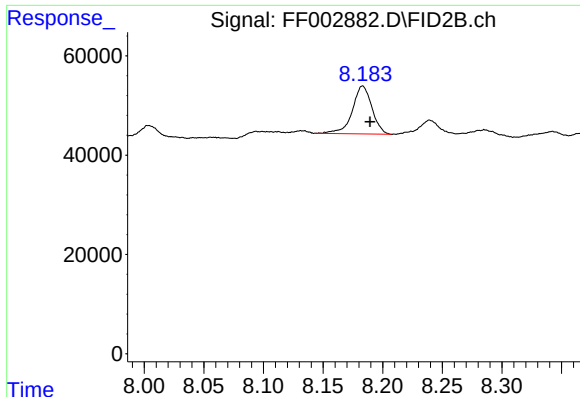


#4 N-TETRADECANE

R.T.: 8.183 min
Delta R.T.: -0.006 min
Response: 110111
Conc: 0.95 ug/ml

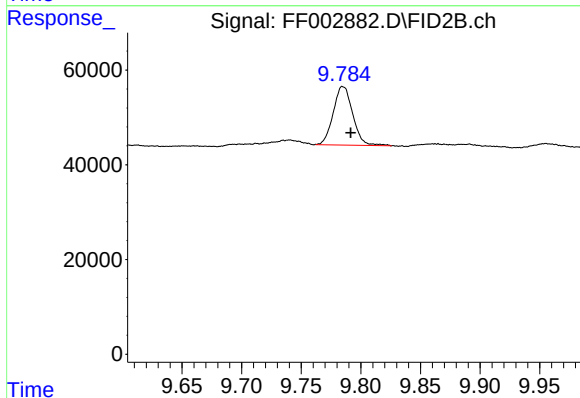


#5 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.006 min
Response: 140609
Conc: 1.29 ug/ml

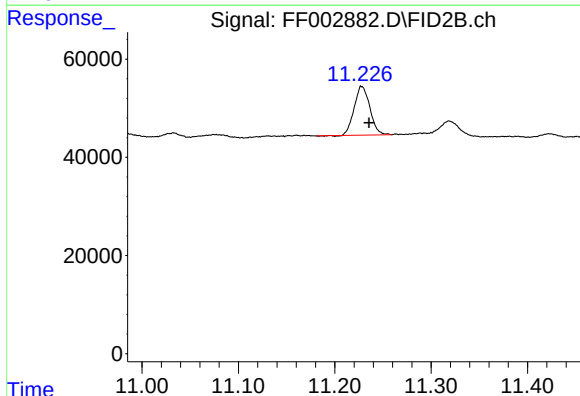


#6 N-OCTADECANE

R.T.: 11.228 min
Delta R.T.: -0.007 min
Response: 112488
Conc: 1.08 ug/ml

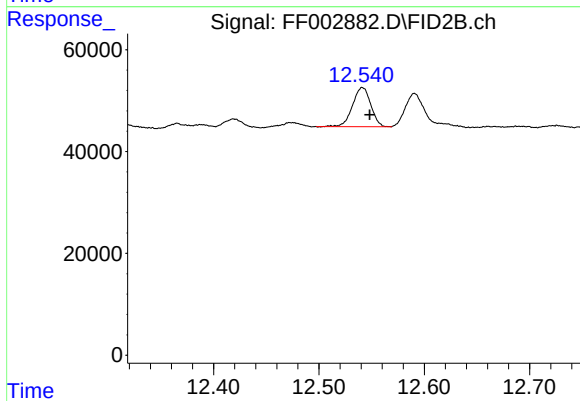


#7 N-EICOSANE

R.T.: 12.541 min
Delta R.T.: -0.007 min
Response: 92364
Conc: 0.95 ug/ml

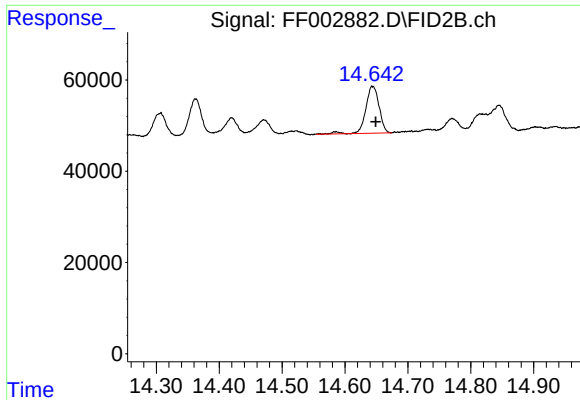


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.644 min
Delta R.T.: -0.005 min
Response: 150834
Conc: 1.93 ug/ml

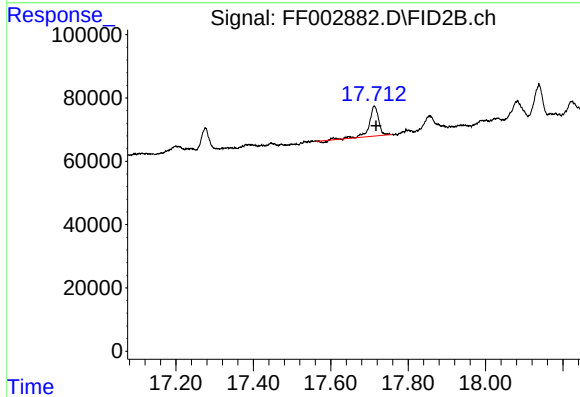


#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.004 min
Response: 157363
Conc: 1.59 ug/ml

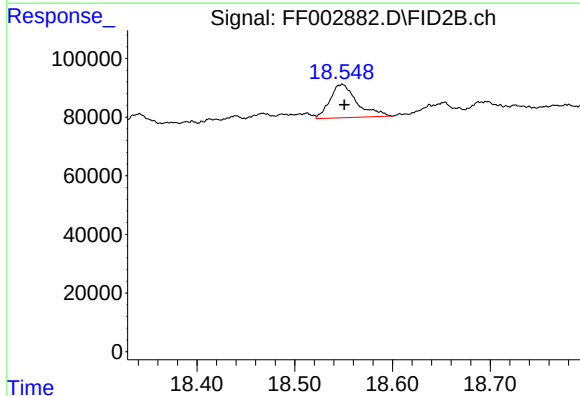


#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: -0.002 min
Response: 218467
Conc: 2.21 ug/ml

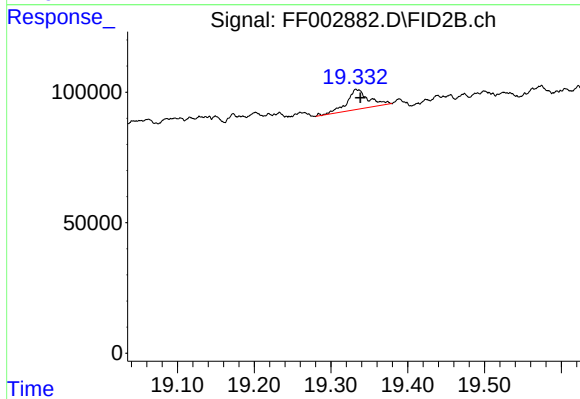

#15 N-TETRATRIACONTANE

R.T.: 19.333 min
Delta R.T.: -0.006 min
Response: 148174
Conc: 1.50 ug/ml

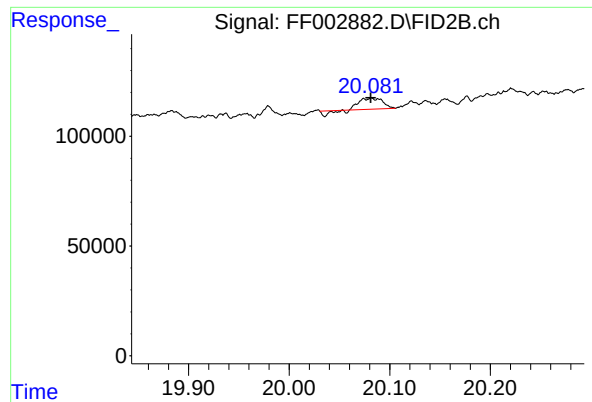

#16 N-HEXATRIACONTANE

R.T.: 20.082 min
Delta R.T.: 0.000 min
Response: 68688
Conc: 0.72 ug/ml