

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002883.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 19:08
 Operator : AJ\SJ
 Sample : J5764-29 10X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:34:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.644	177346	2.270 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.183	117374	1.016 ug/ml
5)	N-HEXADECANE	9.785	127474	1.166 ug/ml
6)	N-OCTADECANE	11.228	104368	1.005 ug/ml
7)	N-EICOSANE	12.541	87399	0.903 ug/ml
12)	N-OCTACOSANE	16.825	81040	0.850 ug/ml
13)	N-TRIACONTANE	17.714	143667	1.449 ug/ml
14)	N-DOTRIACONTANE	18.548	201465	2.035 ug/ml
15)	N-TETRATRIACONTANE	19.330	108515	1.099 ug/ml
16)	N-HEXATRIACONTANE	20.080	95501	1.002 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002883.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 19:08
Operator : AJ\SJ
Sample : J5764-29 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:34:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

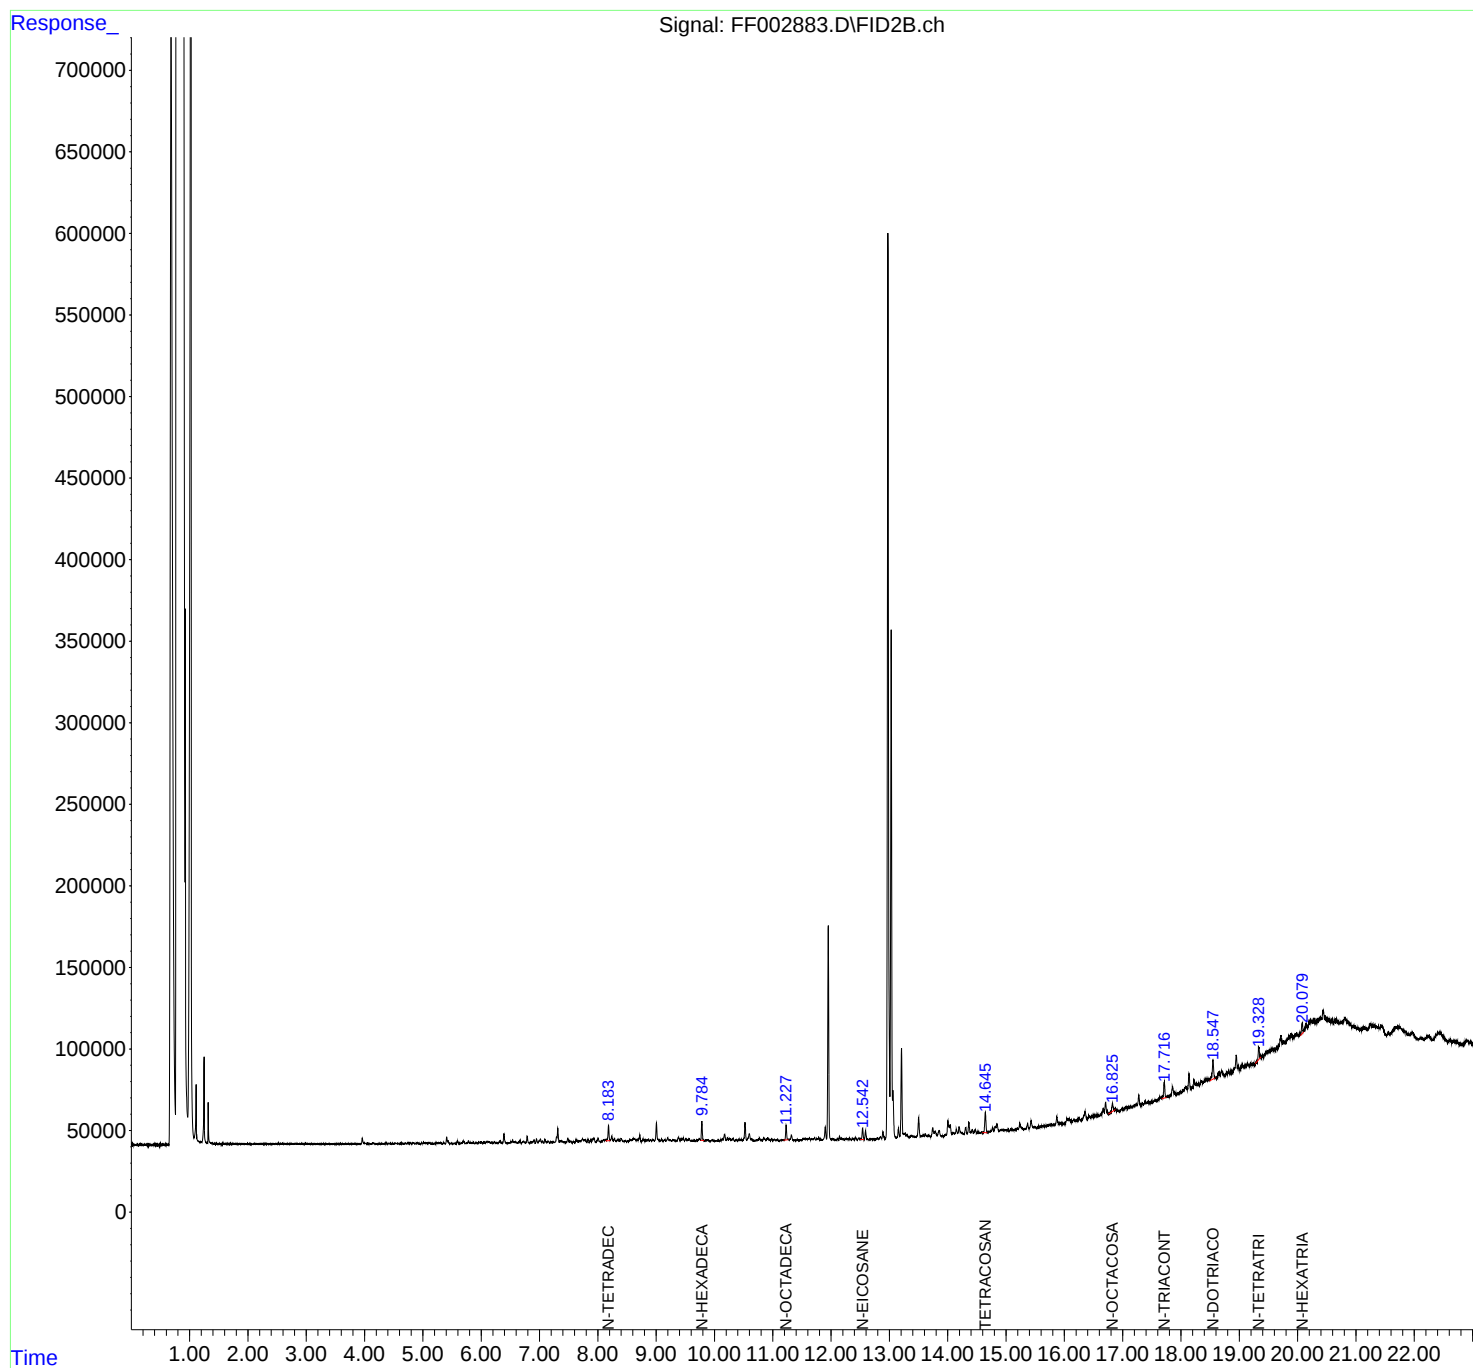

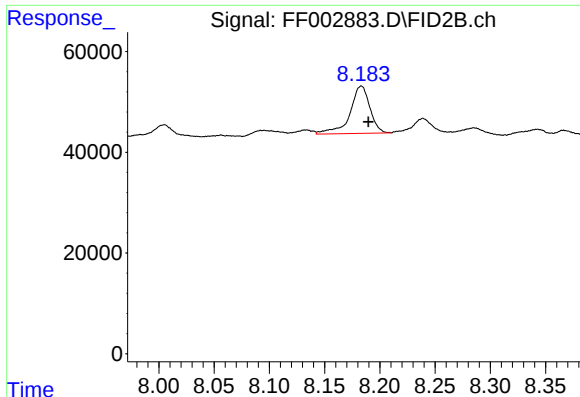


#4 N-TETRADECANE

R.T.: 8.183 min
Delta R.T.: -0.006 min
Response: 117374
Conc: 1.02 ug/ml

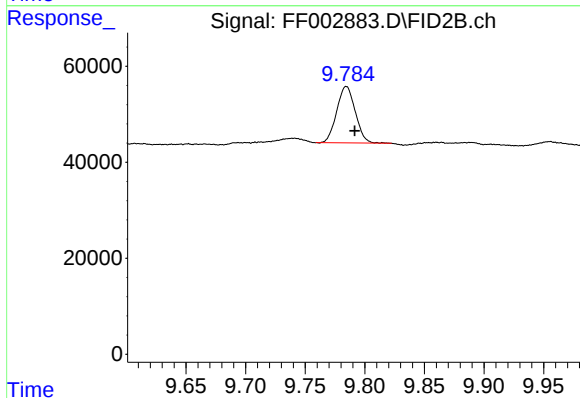


#5 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.007 min
Response: 127474
Conc: 1.17 ug/ml

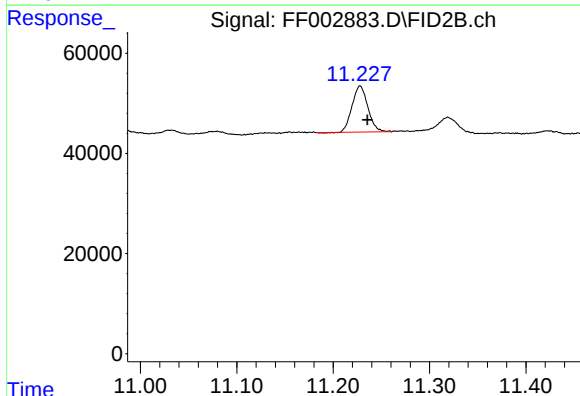


#6 N-OCTADECANE

R.T.: 11.228 min
Delta R.T.: -0.008 min
Response: 104368
Conc: 1.01 ug/ml

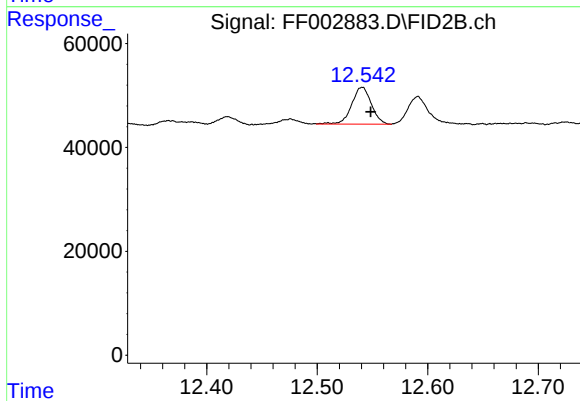


#7 N-EICOSANE

R.T.: 12.541 min
Delta R.T.: -0.008 min
Response: 87399
Conc: 0.90 ug/ml

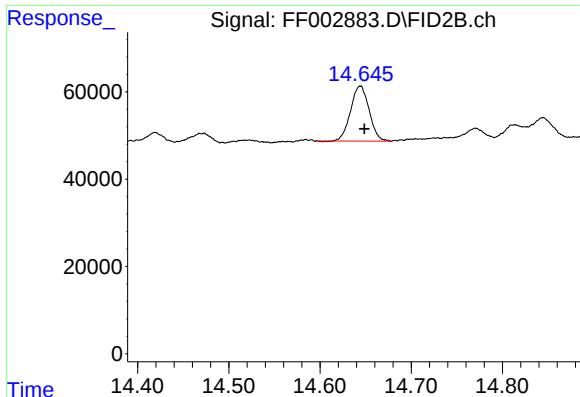


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.644 min
Delta R.T.: -0.005 min
Response: 177346
Conc: 2.27 ug/ml

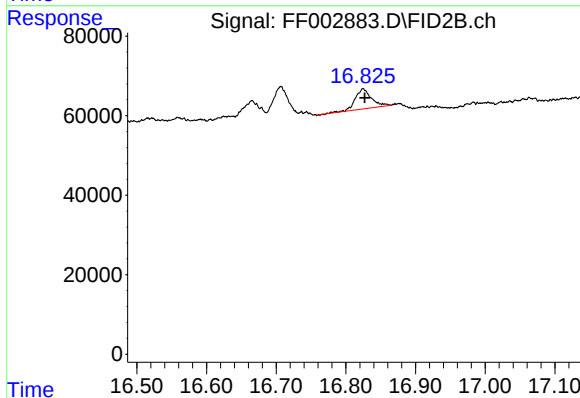


#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.002 min
Response: 81040
Conc: 0.85 ug/ml

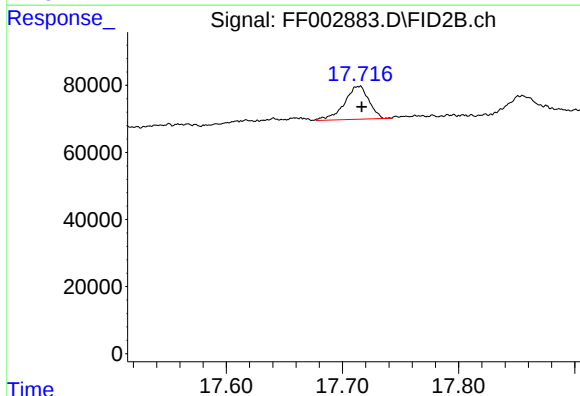


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.002 min
Response: 143667
Conc: 1.45 ug/ml

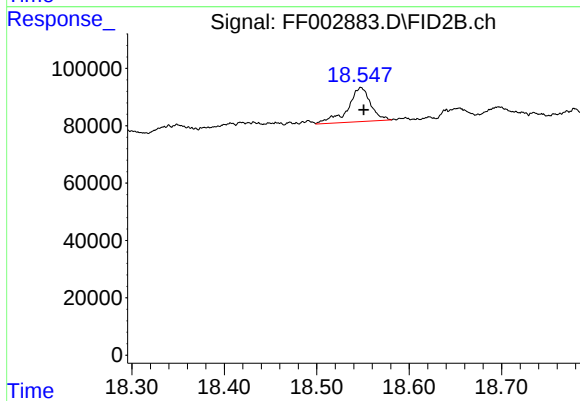


#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: -0.003 min
Response: 201465
Conc: 2.04 ug/ml

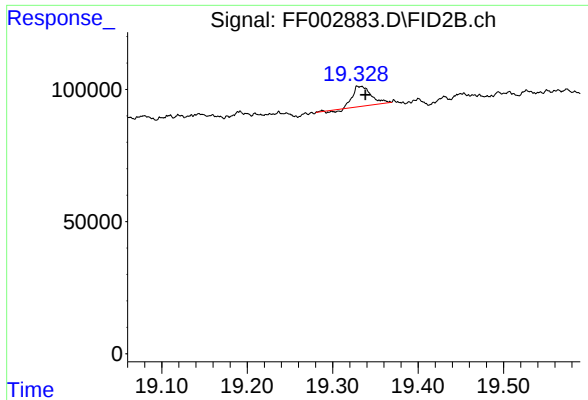

#15 N-TETRATRIACONTANE

R.T.: 19.330 min
Delta R.T.: -0.009 min
Response: 108515
Conc: 1.10 ug/ml

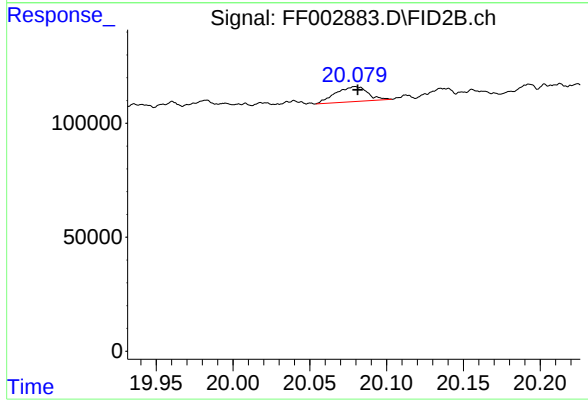

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: -0.002 min
Response: 95501
Conc: 1.00 ug/ml