

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
 Data File : FF002878.D
 Signal(s) : FID2B.ch
 Acq On : 03 Dec 2018 16:35
 Operator : AJ\SJ
 Sample : J5764-25MS 5X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 01:33:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.645	428072	5.480 ug/ml
Target Compounds			
2) N-DECANE	4.371	386581	3.095 ug/ml
3) N-DODECANE	6.390	523932	4.323 ug/ml
4) N-TETRADECANE	8.183	572925	4.960 ug/mlm
5) N-HEXADECANE	9.785	601180	5.498 ug/mlm
6) N-OCTADECANE	11.229	560073	5.395 ug/ml
7) N-EICOSANE	12.540	531946	5.494 ug/mlm
8) N-DOCOSANE	13.744	633127	6.915 ug/mlm
10) N-TETRACOSANE	14.849	611608	6.865 ug/ml
11) N-HEXACOSANE	15.874	556158	6.128 ug/ml
12) N-OCTACOSANE	16.826	660704	6.927 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120318\
Data File : FF002878.D
Signal(s) : FID2B.ch
Acq On : 03 Dec 2018 16:35
Operator : AJ\SJ
Sample : J5764-25MS 5X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 01:33:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

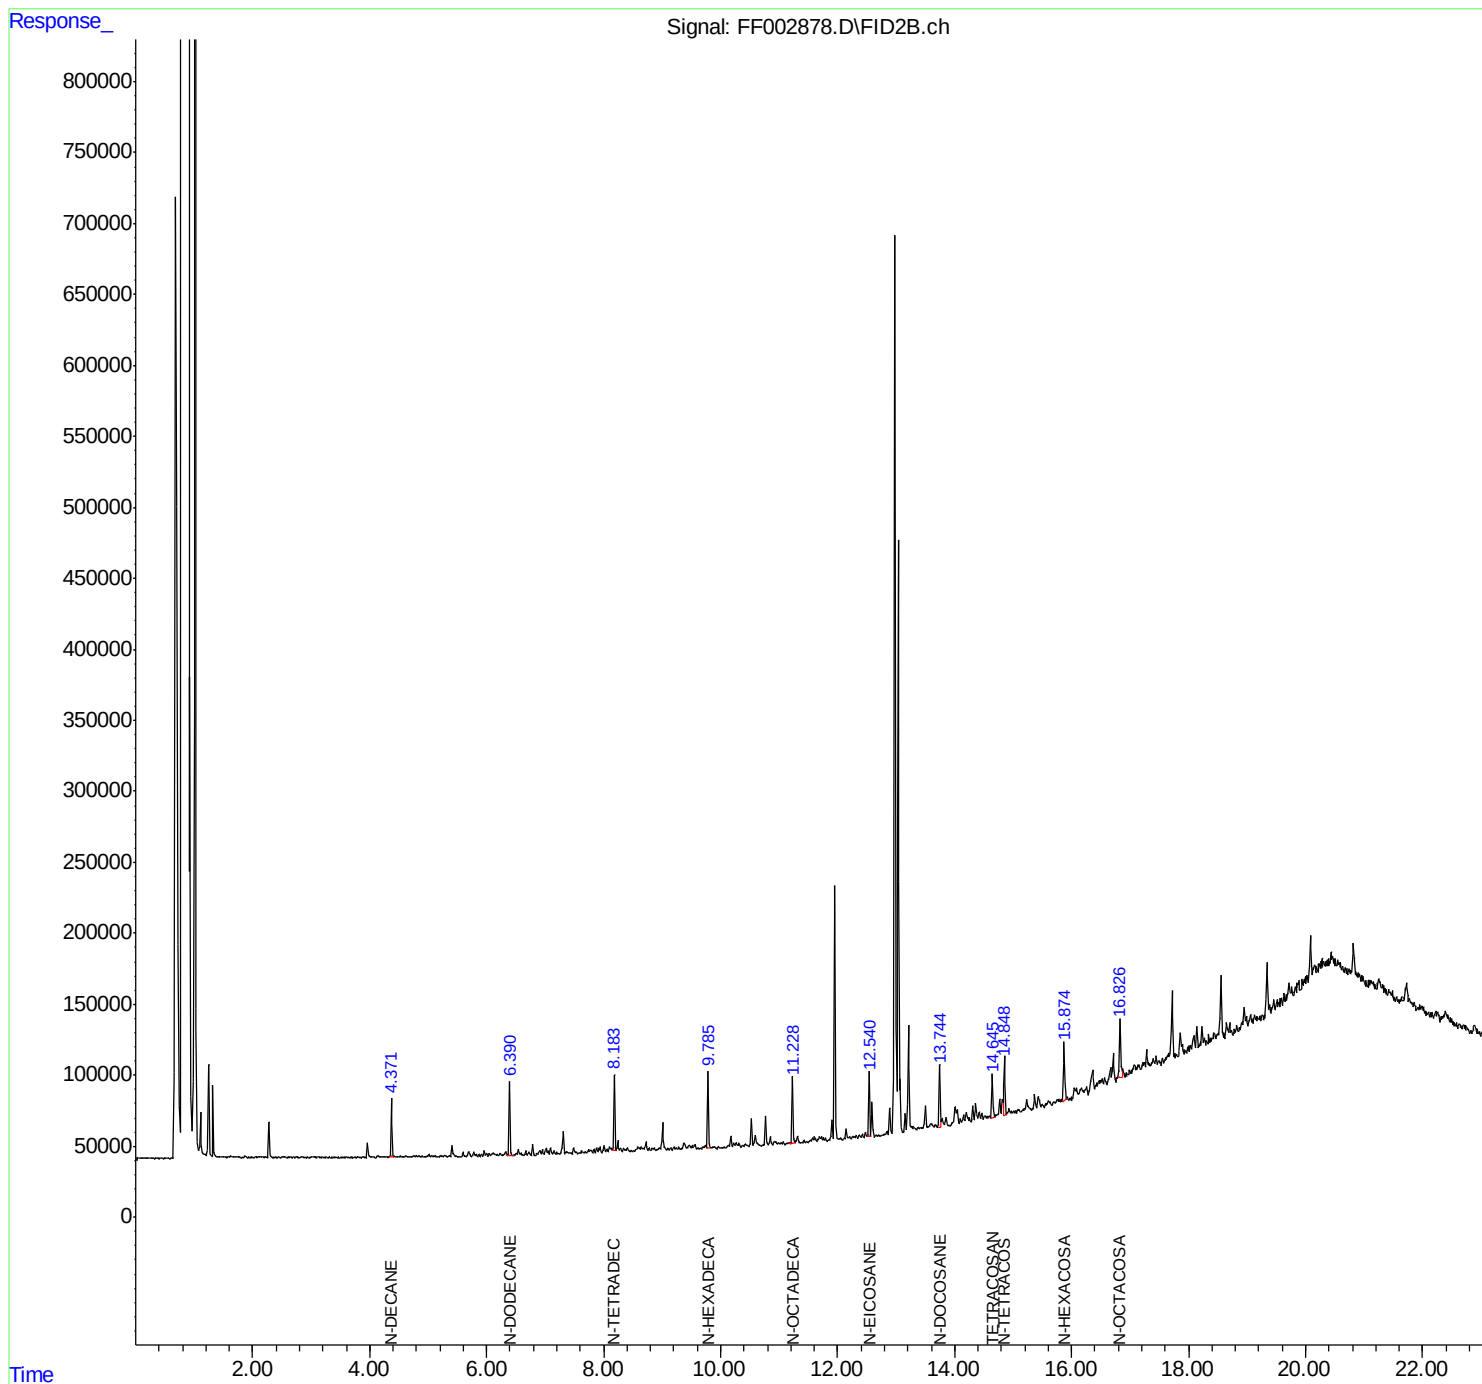

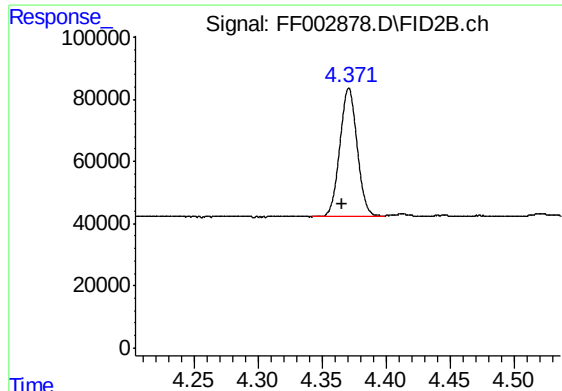


#2 N-DECANE

R.T.: 4.371 min
Delta R.T.: 0.005 min
Response: 386581
Conc: 3.10 ug/ml

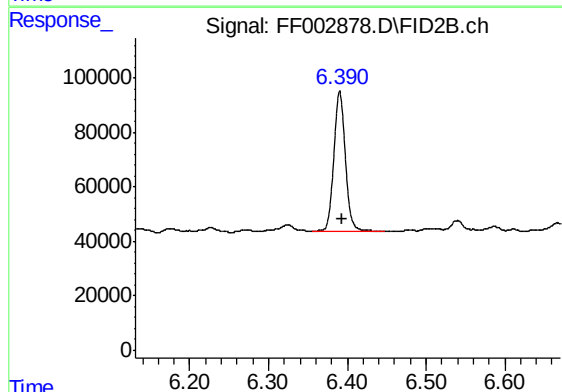


#3 N-DODECANE

R.T.: 6.390 min
Delta R.T.: -0.003 min
Response: 523932
Conc: 4.32 ug/ml

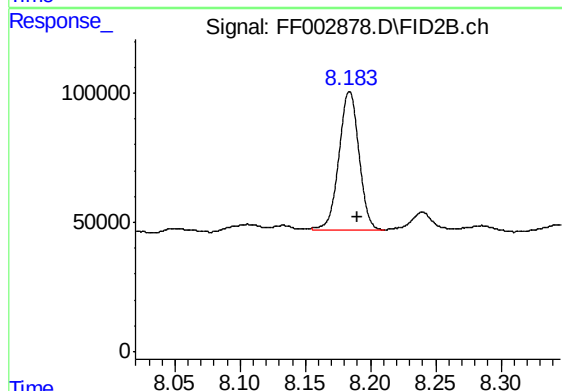


#4 N-TETRADECANE

R.T.: 8.183 min
Delta R.T.: -0.006 min
Response: 572925
Conc: 4.96 ug/ml m

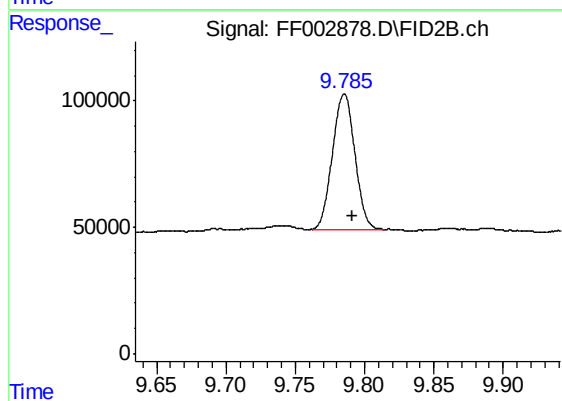


#5 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.006 min
Response: 601180
Conc: 5.50 ug/ml m

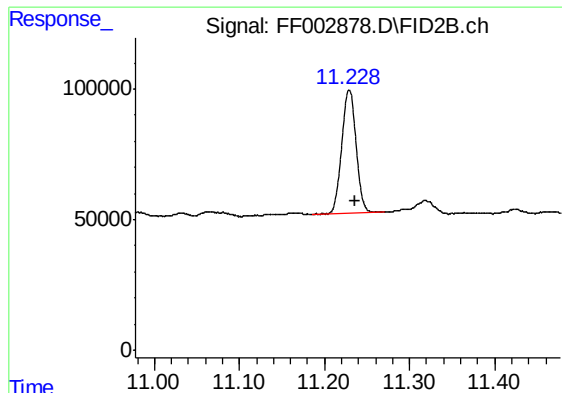


#6 N-OCTADECANE

R.T.: 11.229 min
Delta R.T.: -0.006 min
Response: 560073
Conc: 5.40 ug/ml

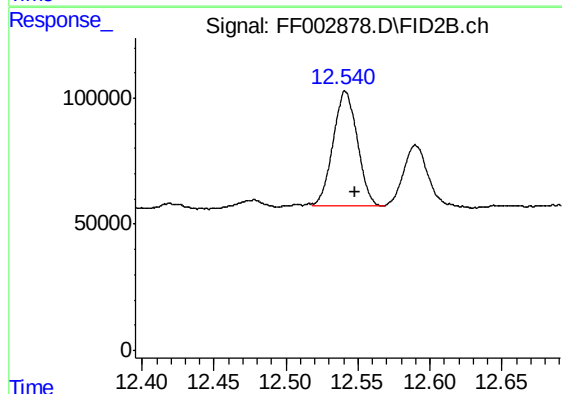


#7 N-EICOSANE

R.T.: 12.540 min
Delta R.T.: -0.008 min
Response: 531946
Conc: 5.49 ug/ml m

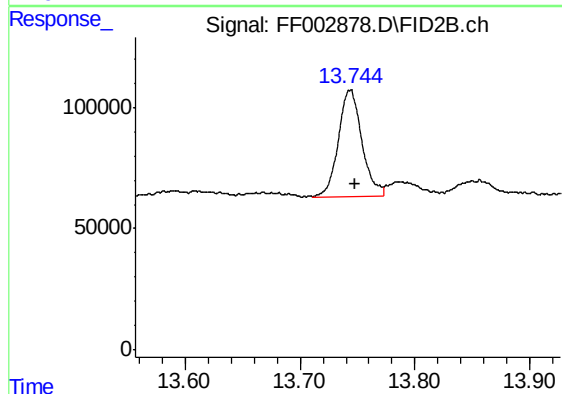


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: -0.004 min
Response: 633127
Conc: 6.92 ug/ml m

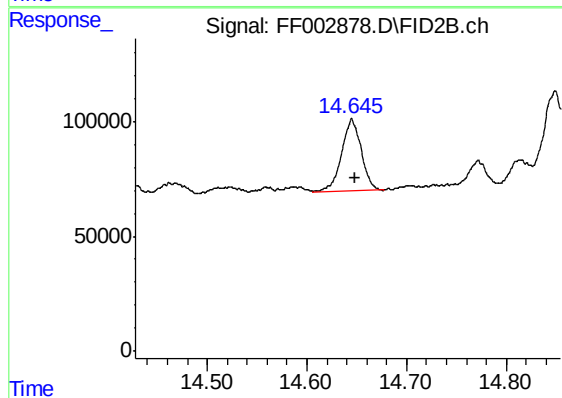


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.645 min
Delta R.T.: -0.004 min
Response: 428072
Conc: 5.48 ug/ml

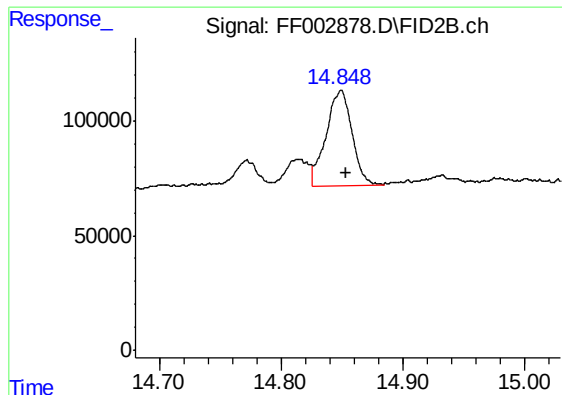


#10 N-TETRACOSANE

R.T.: 14.849 min
Delta R.T.: -0.004 min
Response: 611608
Conc: 6.87 ug/ml

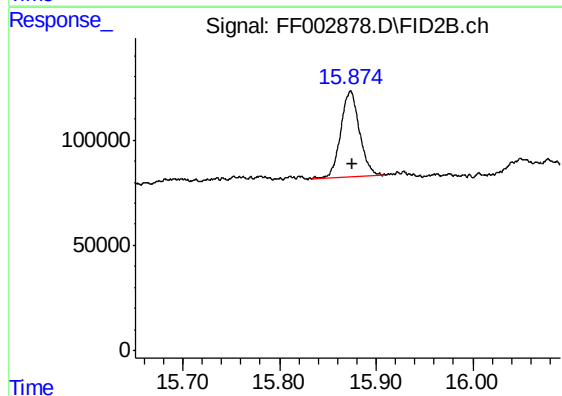

#11 N-HEXACOSANE

R.T.: 15.874 min
Delta R.T.: -0.001 min
Response: 556158
Conc: 6.13 ug/ml

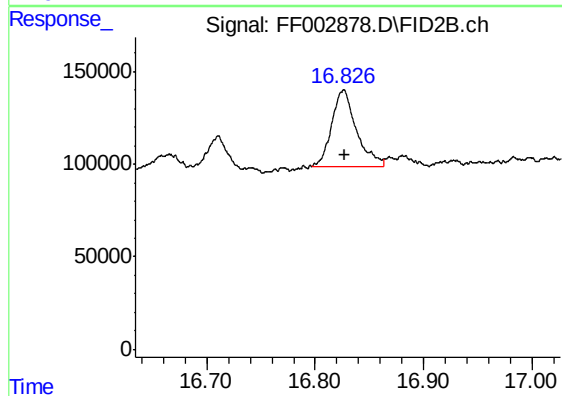

#12 N-OCTACOSANE

R.T.: 16.826 min
Delta R.T.: -0.001 min
Response: 660704
Conc: 6.93 ug/ml m