

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120418\
 Data File : FF002890.D
 Signal(s) : FID2B.ch
 Acq On : 04 Dec 2018 14:48
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 04 15:14:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 15:14:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.645	6491268	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.268	7734729	50.000 ug/ml
2) N-DECANE	4.368	7833405	50.000 ug/ml
3) N-DODECANE	6.391	7939843	50.000 ug/ml
4) N-TETRADECANE	8.186	8014378	50.000 ug/ml
5) N-HEXADECANE	9.788	8007279	50.000 ug/ml
6) N-OCTADECANE	11.231	7920861	50.000 ug/ml
7) N-EICOSANE	12.543	7711495	50.000 ug/ml
8) N-DOCOSANE	13.744	7476507	50.000 ug/ml
10) N-TETRACOSANE	14.850	7225766	50.000 ug/ml
11) N-HEXACOSANE	15.874	6978875	50.000 ug/ml
12) N-OCTACOSANE	16.825	6699314	50.000 ug/ml
13) N-TRIACONTANE	17.715	6406704	50.000 ug/ml
14) N-DOTRIACONTANE	18.548	5971058	50.000 ug/ml
15) N-TETRATRIACONTANE	19.335	5666762	50.000 ug/ml
16) N-HEXATRIACONTANE	20.077	5394880	50.000 ug/ml
17) N-OCTATRIACONTANE	20.816	5074807	50.000 ug/ml
18) N-TETRACONTANE	21.720	5255241	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120418\
Data File : FF002890.D
Signal(s) : FID2B.ch
Acq On : 04 Dec 2018 14:48
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 04 15:14:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 15:14:07 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

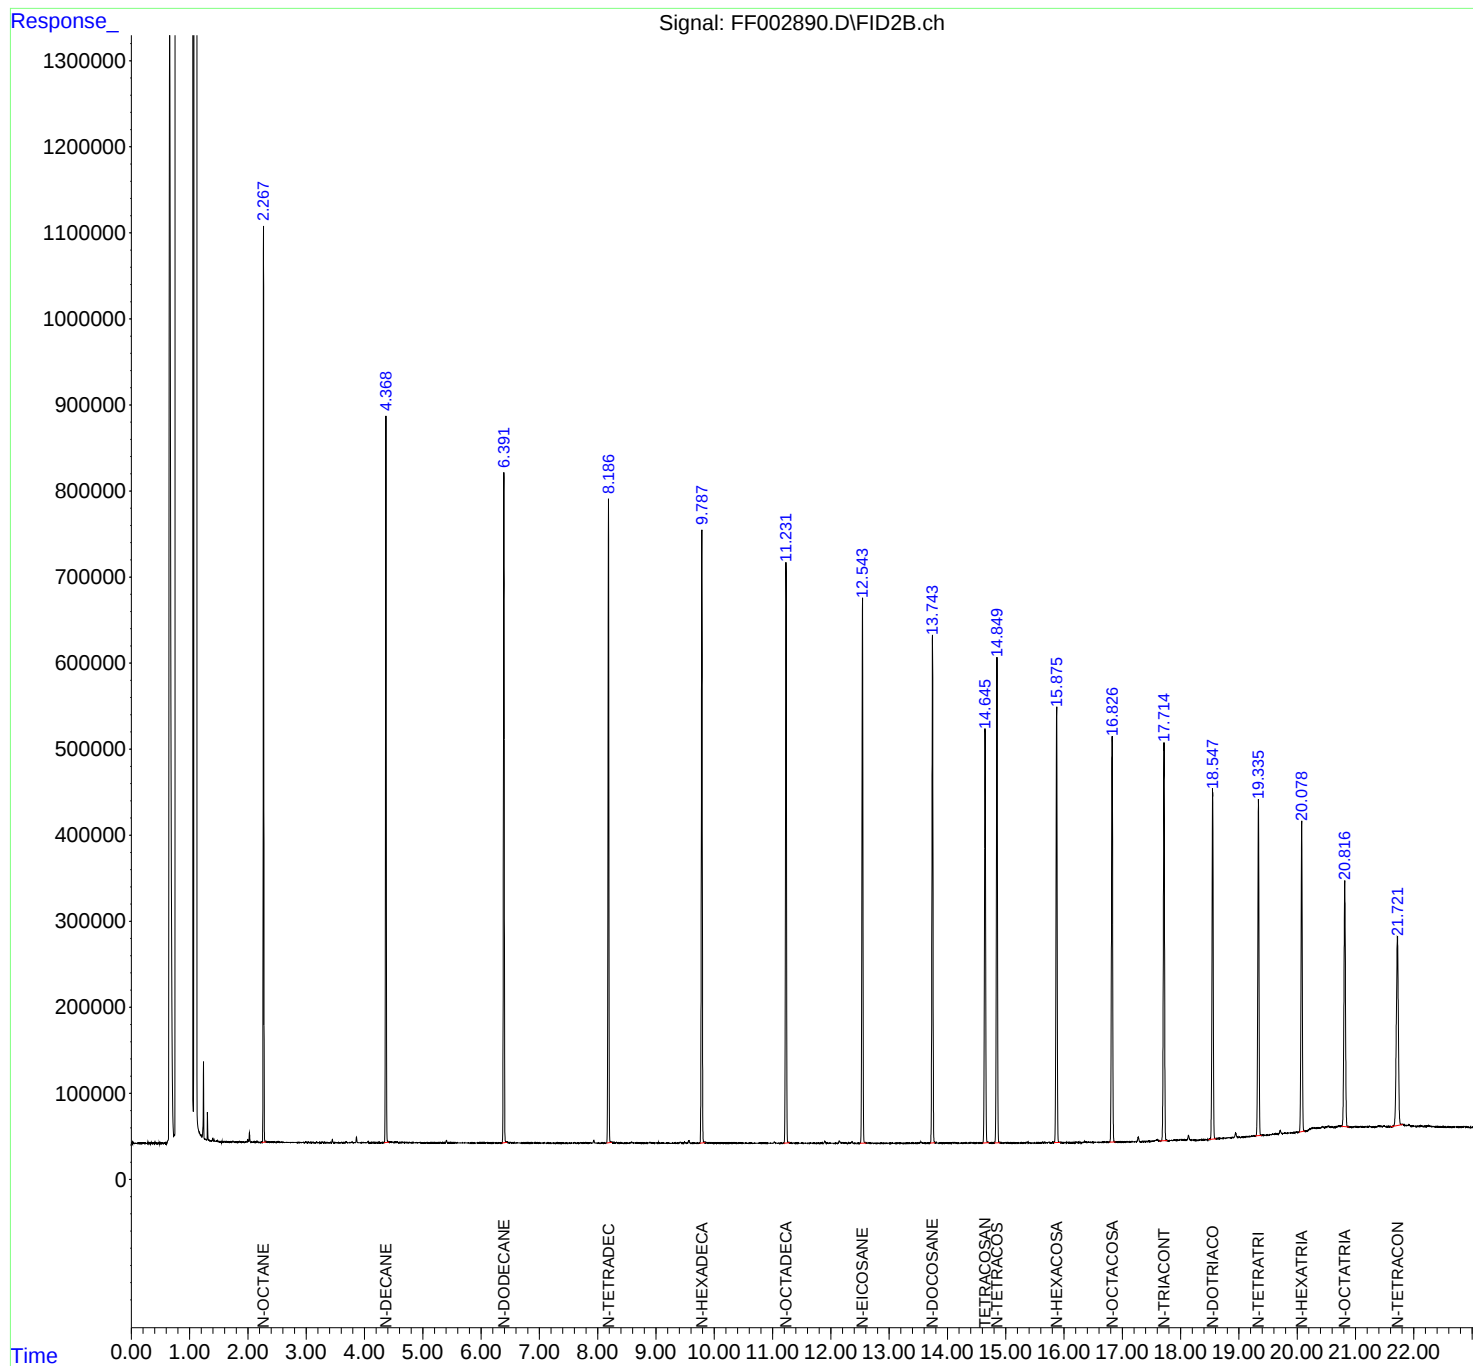

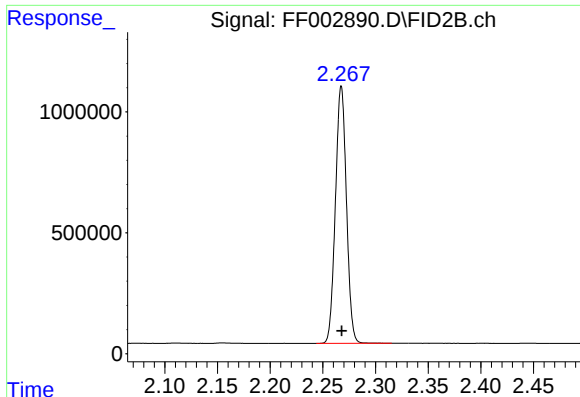


#1 N-OCTANE

R.T.: 2.268 min
Delta R.T.: 0.000 min
Response: 7734729
Conc: 50.00 ug/ml

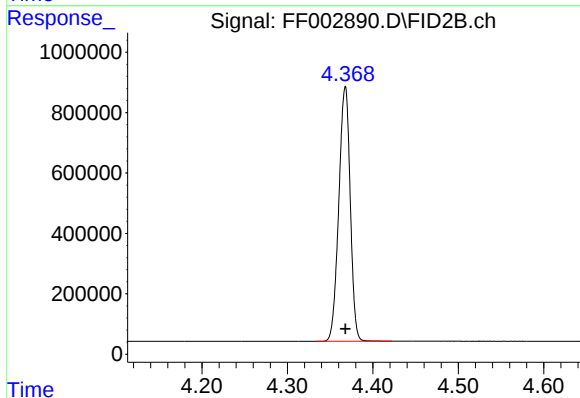


#2 N-DECANE

R.T.: 4.368 min
Delta R.T.: 0.000 min
Response: 7833405
Conc: 50.00 ug/ml

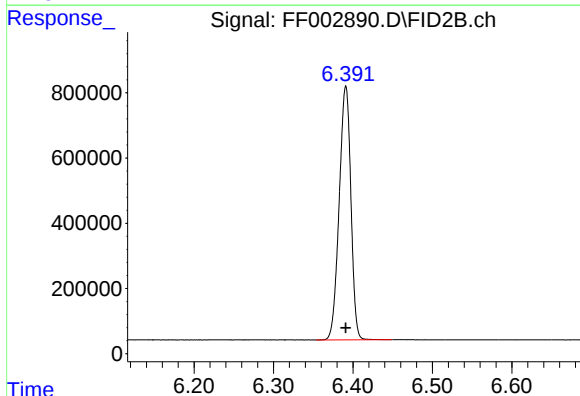


#3 N-DODECANE

R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 7939843
Conc: 50.00 ug/ml

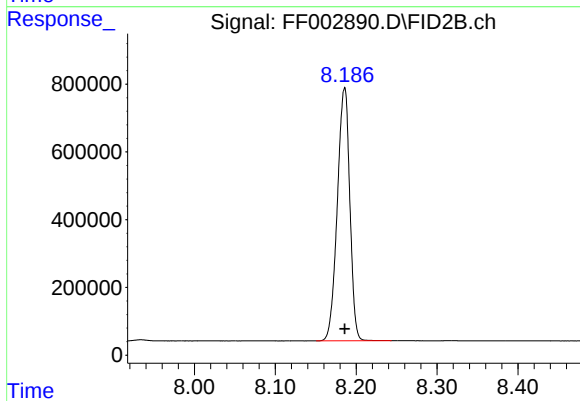


#4 N-TETRADECANE

R.T.: 8.186 min
Delta R.T.: 0.000 min
Response: 8014378
Conc: 50.00 ug/ml

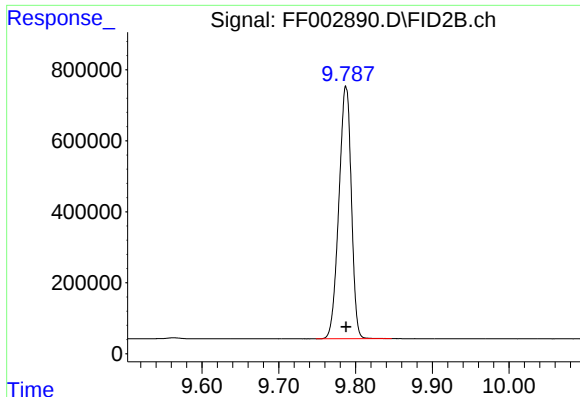


#5 N-HEXADECANE

R.T.: 9.788 min
Delta R.T.: 0.000 min
Response: 8007279
Conc: 50.00 ug/ml

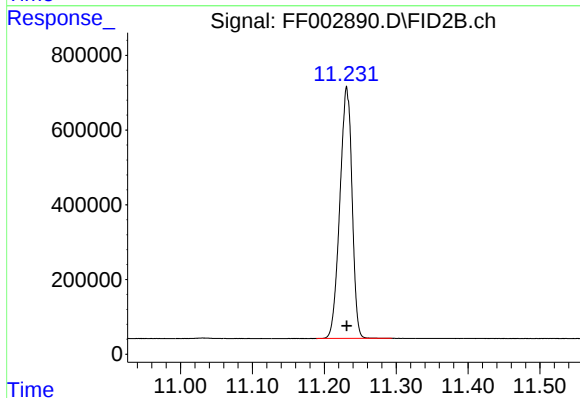


#6 N-OCTADECANE

R.T.: 11.231 min
Delta R.T.: 0.000 min
Response: 7920861
Conc: 50.00 ug/ml

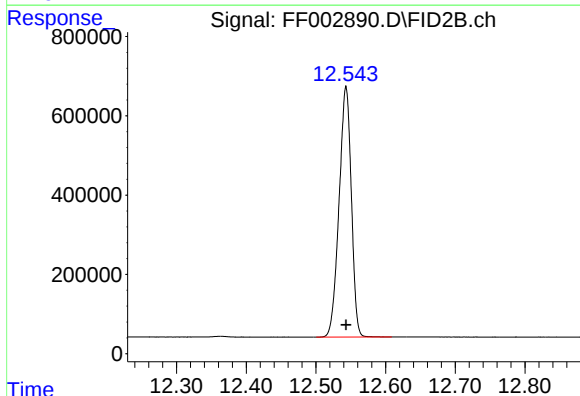


#7 N-EICOSANE

R.T.: 12.543 min
Delta R.T.: 0.000 min
Response: 7711495
Conc: 50.00 ug/ml

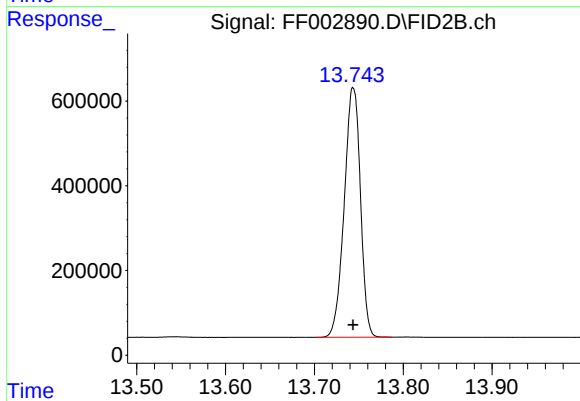


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: 0.000 min
Response: 7476507
Conc: 50.00 ug/ml

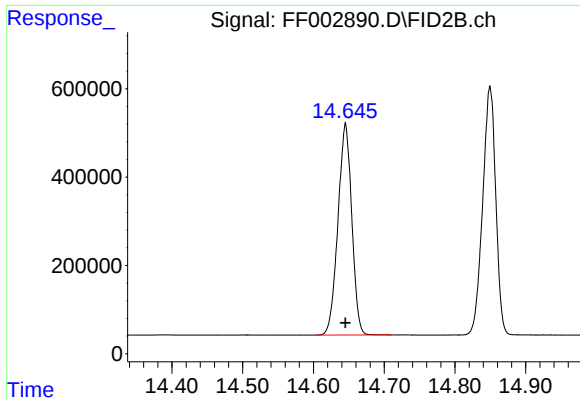


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.645 min
Delta R.T.: 0.000 min
Response: 6491268
Conc: 50.00 ug/ml

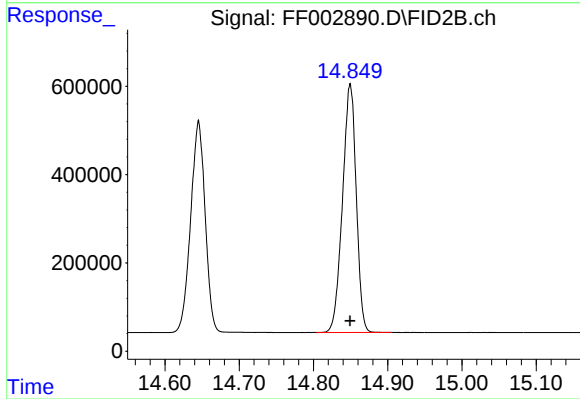


#10 N-TETRACOSANE

R.T.: 14.850 min
Delta R.T.: 0.000 min
Response: 7225766
Conc: 50.00 ug/ml

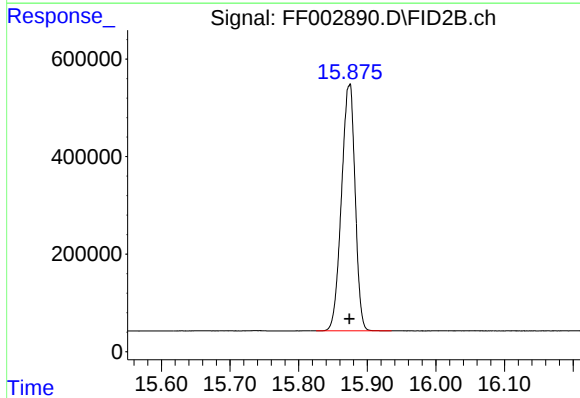


#11 N-HEXACOSANE

R.T.: 15.874 min
Delta R.T.: 0.000 min
Response: 6978875
Conc: 50.00 ug/ml

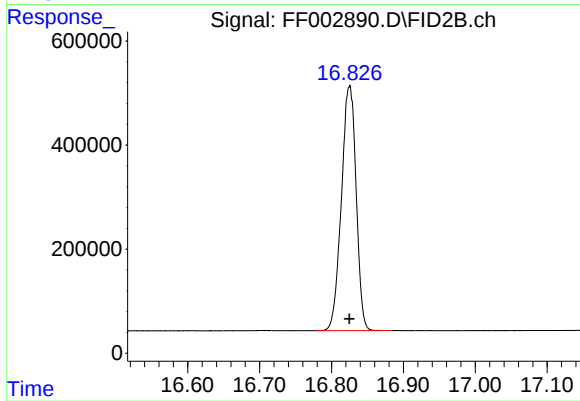


#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: 0.000 min
Response: 6699314
Conc: 50.00 ug/ml

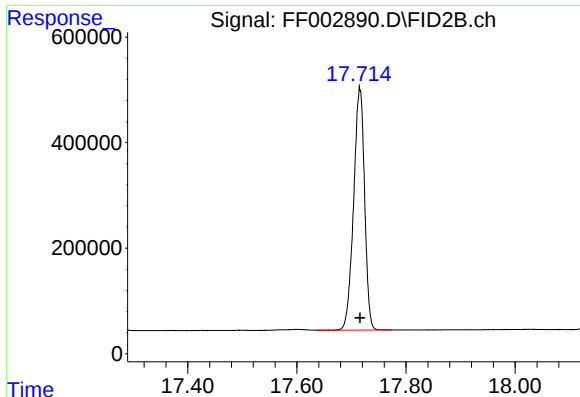


#13 N-TRIACONTANE

R.T.: 17.715 min
Delta R.T.: 0.000 min
Response: 6406704
Conc: 50.00 ug/ml

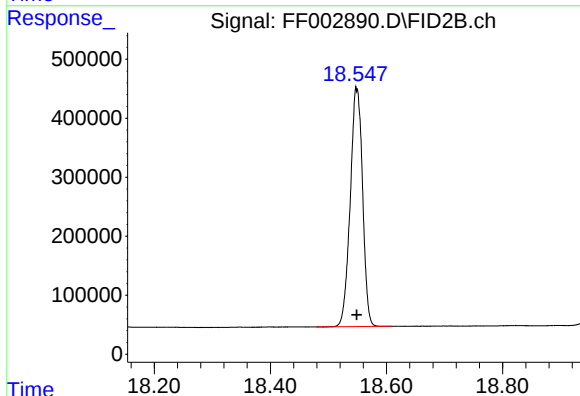


#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: 0.000 min
Response: 5971058
Conc: 50.00 ug/ml

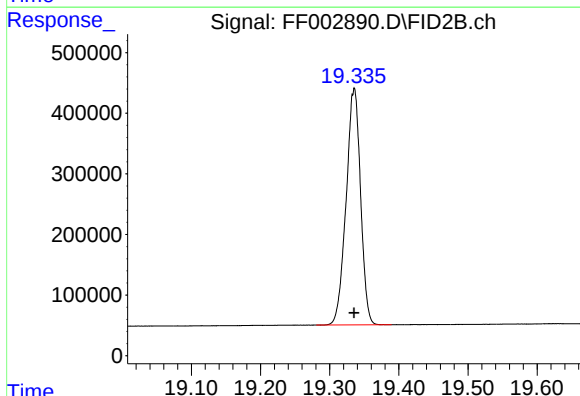


#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: 0.000 min
Response: 5666762
Conc: 50.00 ug/ml

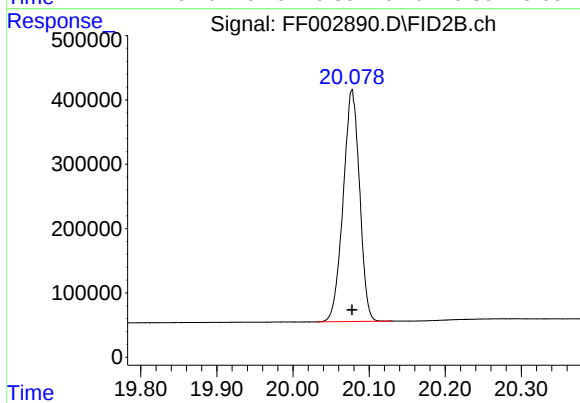


#16 N-HEXATRIACONTANE

R.T.: 20.077 min
Delta R.T.: 0.000 min
Response: 5394880
Conc: 50.00 ug/ml

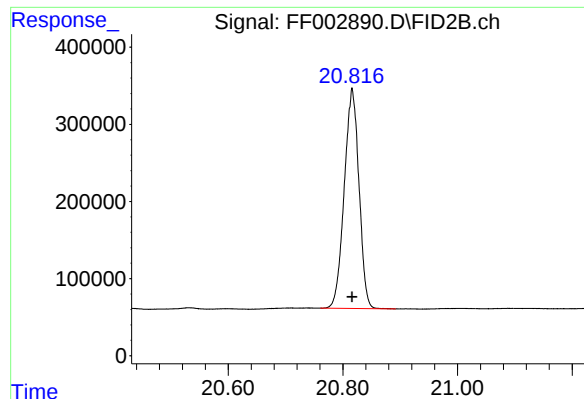

#17 N-OCTATRIACONTANE

R.T.: 20.816 min
Delta R.T.: 0.000 min
Response: 5074807
Conc: 50.00 ug/ml

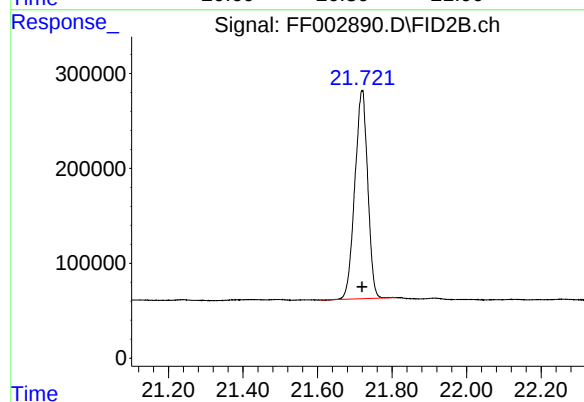

#18 N-TETRACONTANE

R.T.: 21.720 min
Delta R.T.: 0.000 min
Response: 5255241
Conc: 50.00 ug/ml