

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
 Data File : FF005993.D
 Signal(s) : FID2B.ch
 Acq On : 04 Dec 2019 16:14
 Operator : DD\AJ
 Sample : K6119-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 05 00:17:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	2170442	19.312 ug/ml
Target Compounds			
4) N-TETRADECANE	8.176	127761	0.980 ug/ml
7) N-EICOSANE	12.558	129319	0.986 ug/ml
8) N-DOCOSANE	13.754	100564	0.776 ug/ml
10) N-TETRACOSANE	14.852	89318	0.697 ug/ml
11) N-HEXACOSANE	15.872	325301	2.578 ug/ml
12) N-OCTACOSANE	16.821	728856	5.893 ug/ml
13) N-TRIACONTANE	17.710	1356393	11.174 ug/ml
14) N-DOTRIACONTANE	18.541	1092974	9.548 ug/ml
15) N-TETRATRIACONTANE	19.327	555086	5.162 ug/ml
16) N-HEXATRIACONTANE	20.070	300048	2.987 ug/ml
17) N-OCTATRIACONTANE	20.798	623077	7.031 ug/ml
18) N-TETRACONTANE	21.692	484972	5.418 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
Data File : FF005993.D
Signal(s) : FID2B.ch
Acq On : 04 Dec 2019 16:14
Operator : DD\AJ
Sample : K6119-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 05 00:17:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

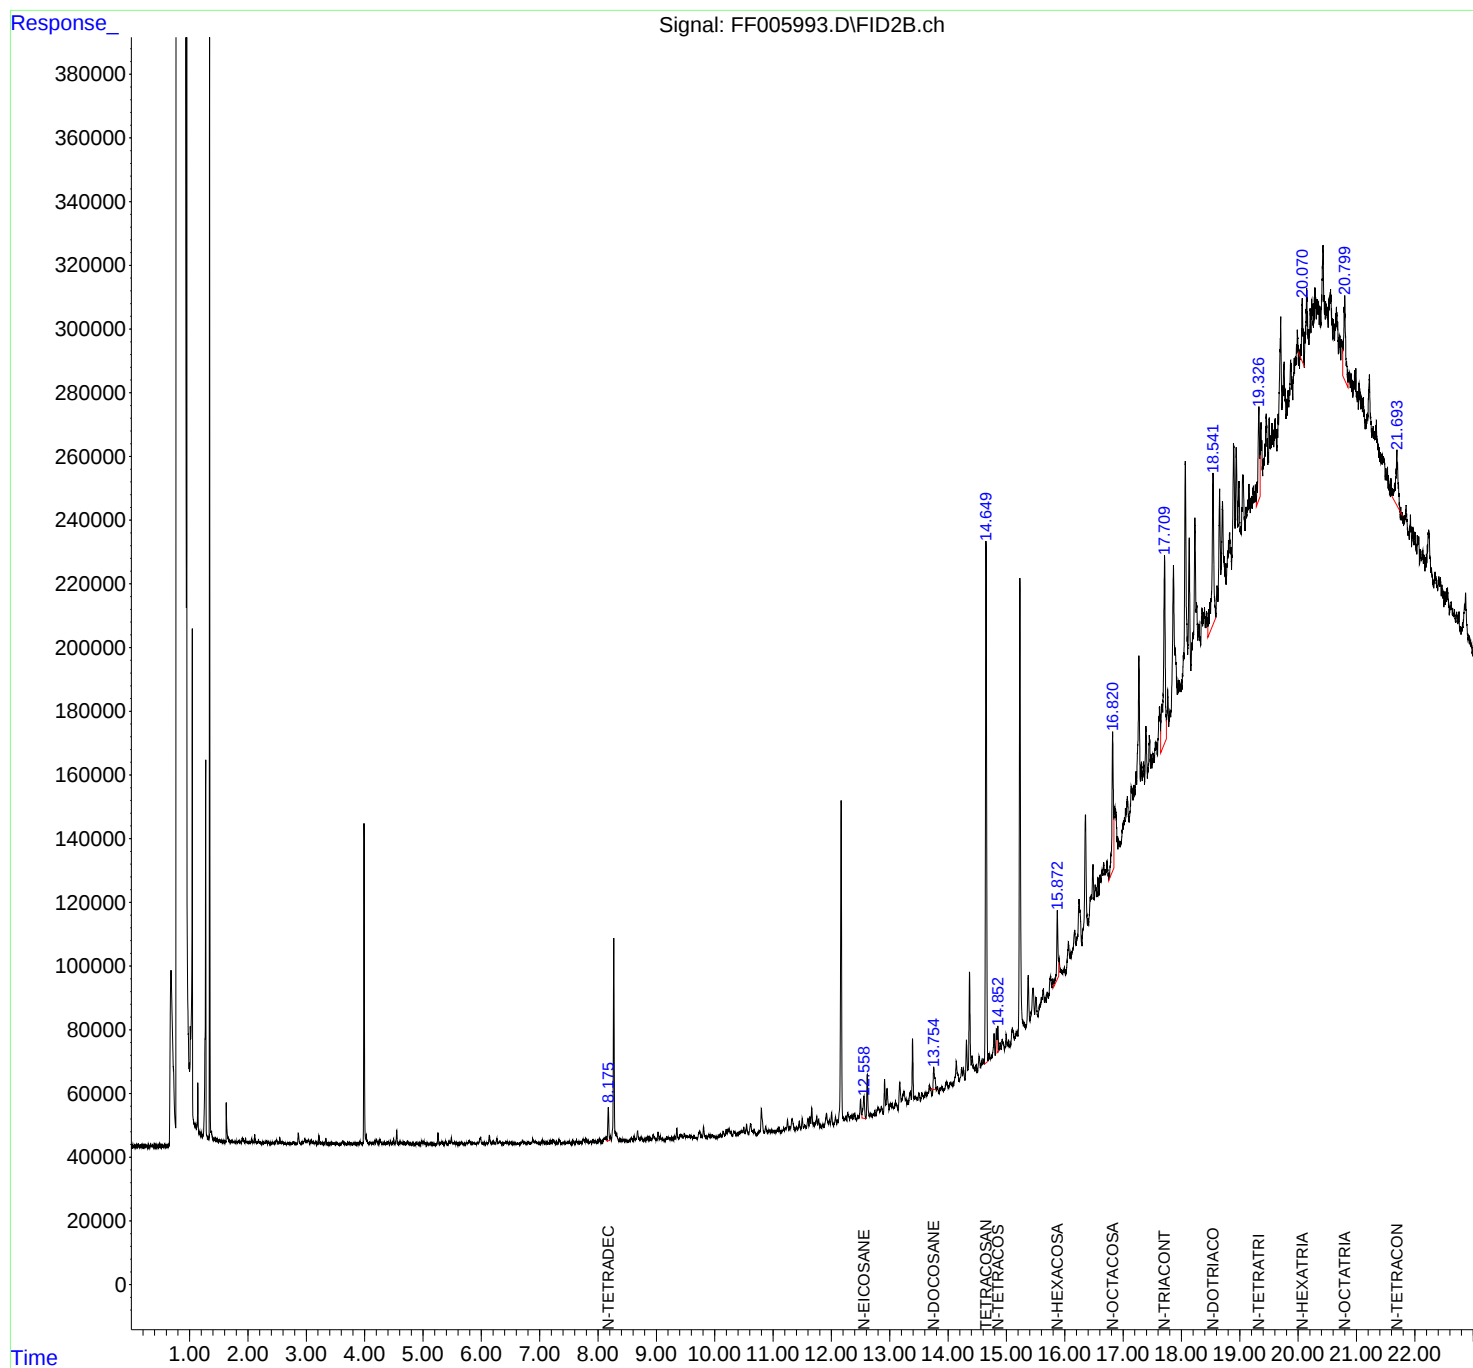


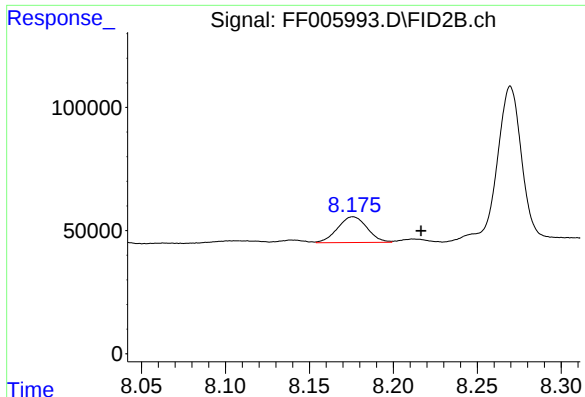

#4 N-TETRADECANE


R.T.: 8.176 min
Delta R.T.: -0.040 min
Response: 127761
Conc: 0.98 ug/ml

Instrument :
FID_F
ClientSampleId :

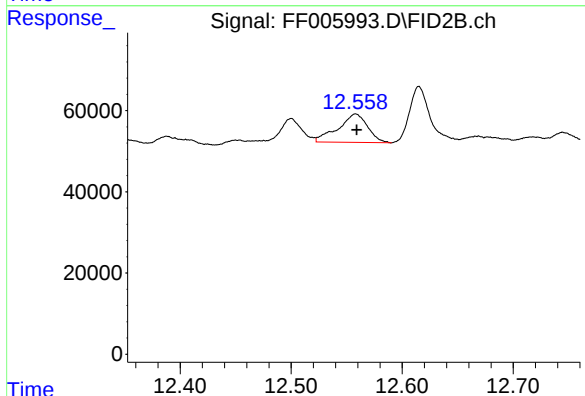


#7 N-EICOSANE

R.T.: 12.558 min
Delta R.T.: 0.000 min
Response: 129319
Conc: 0.99 ug/ml

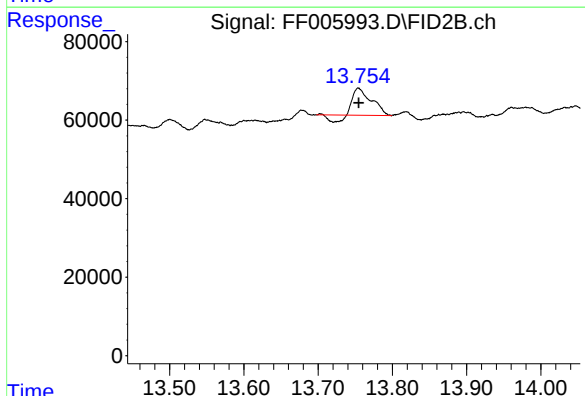


#8 N-DOCOSANE

R.T.: 13.754 min
Delta R.T.: 0.000 min
Response: 100564
Conc: 0.78 ug/ml

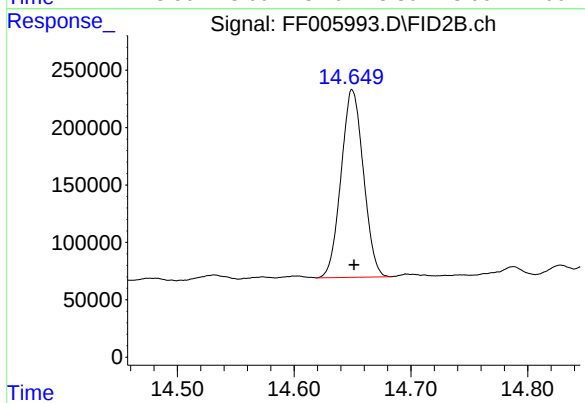

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.650 min
Delta R.T.: -0.002 min
Response: 2170442
Conc: 19.31 ug/ml

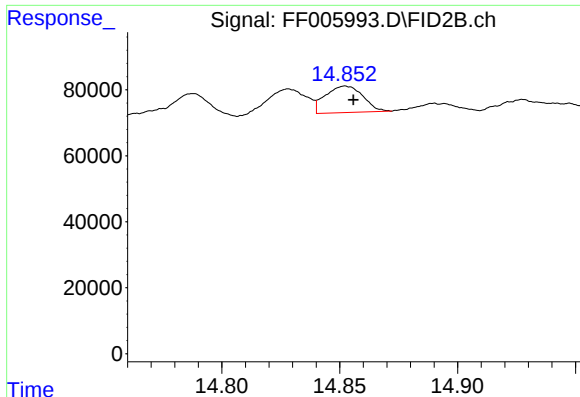

#10 N-TETRACOSANE


R.T.: 14.852 min
Delta R.T.: -0.003 min
Response: 89318
Conc: 0.70 ug/ml

Instrument :
FID_F
ClientSampleId :

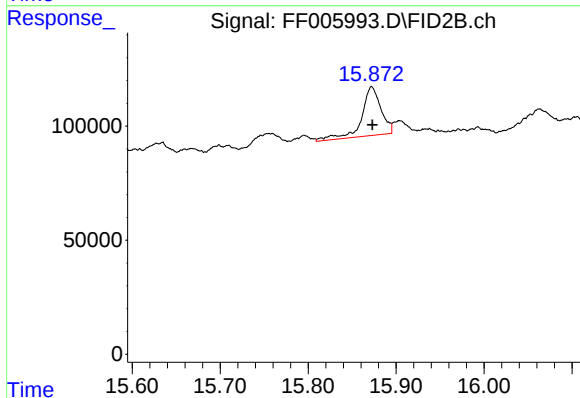


#11 N-HEXACOSANE

R.T.: 15.872 min
Delta R.T.: 0.000 min
Response: 325301
Conc: 2.58 ug/ml

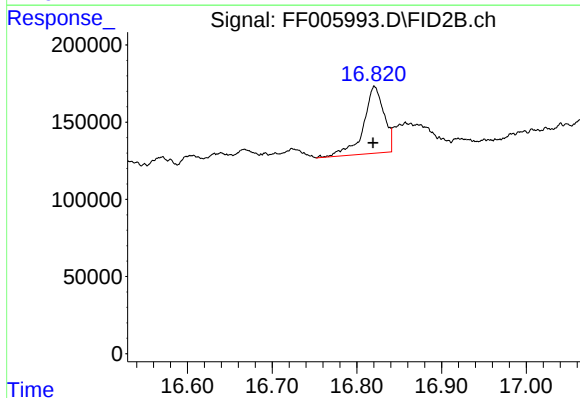


#12 N-OCTACOSANE

R.T.: 16.821 min
Delta R.T.: 0.002 min
Response: 728856
Conc: 5.89 ug/ml

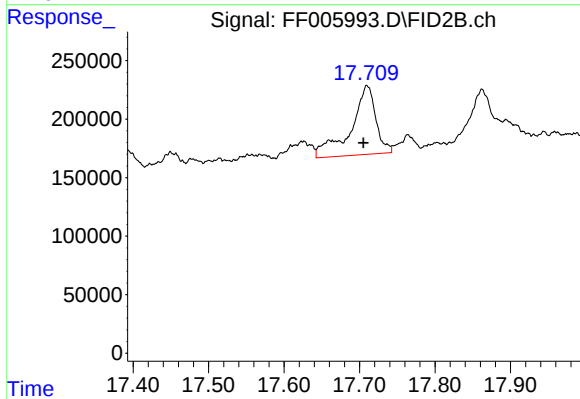

#13 N-TRIACONTANE


R.T.: 17.710 min
Delta R.T.: 0.005 min
Response: 1356393
Conc: 11.17 ug/ml

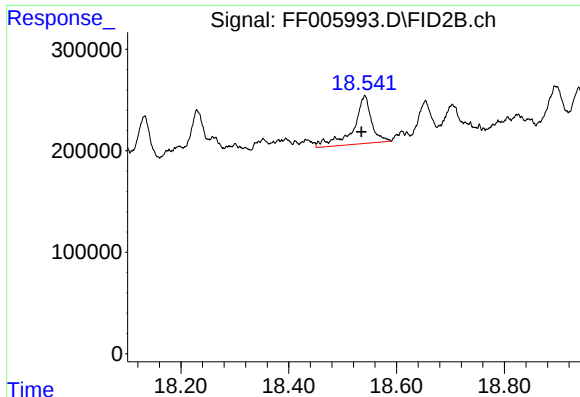

#14 N-DOTRIACONTANE


R.T.: 18.541 min
Delta R.T.: 0.006 min
Response: 1092974
Conc: 9.55 ug/ml

Instrument :
FID_F
ClientSampleId :

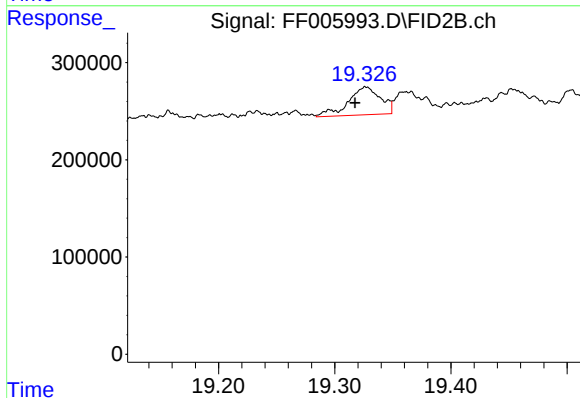


#15 N-TETRATRIACONTANE

R.T.: 19.327 min
Delta R.T.: 0.009 min
Response: 555086
Conc: 5.16 ug/ml

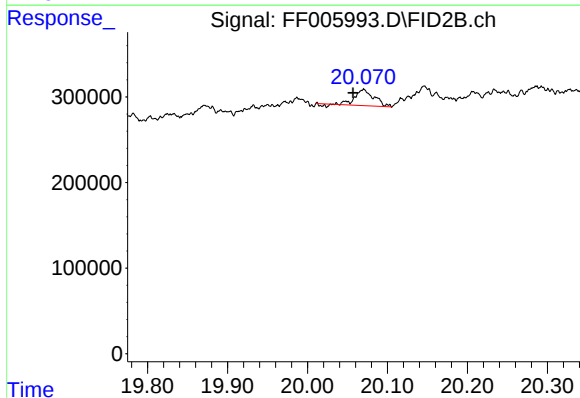


#16 N-HEXATRIACONTANE

R.T.: 20.070 min
Delta R.T.: 0.013 min
Response: 300048
Conc: 2.99 ug/ml

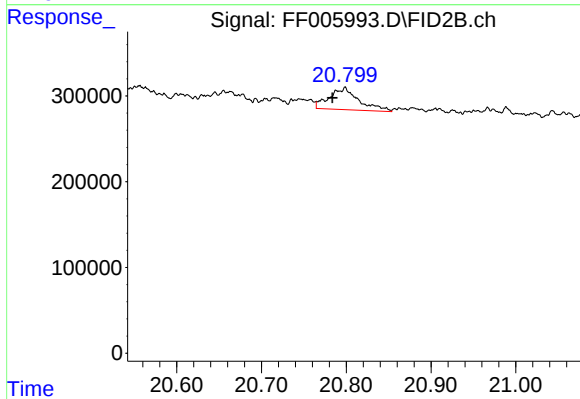

#17 N-OCTATRIACONTANE

R.T.: 20.798 min
Delta R.T.: 0.015 min
Response: 623077
Conc: 7.03 ug/ml

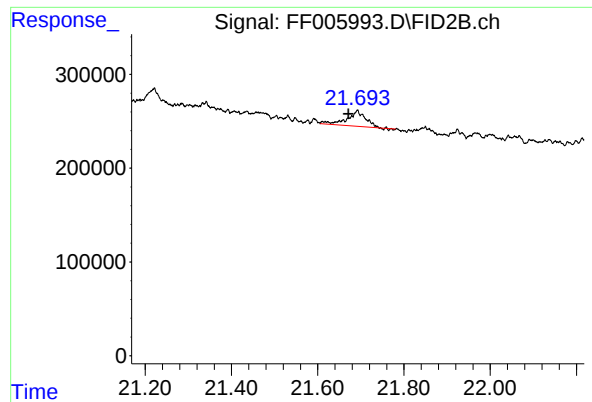

#18 N-TETRACONTANE

R.T.: 21.692 min
Delta R.T.: 0.021 min
Response: 484972
Conc: 5.42 ug/ml

Instrument :
FID_F
ClientSampleId :