

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
 Data File : FF005998.D
 Signal(s) : FID2B.ch
 Acq On : 04 Dec 2019 18:45
 Operator : DD\AJ
 Sample : K6119-09
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 05 00:18:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.653	2100059	18.686 ug/ml
Target Compounds			
4) N-TETRADECANE	8.273f	627039	4.811 ug/ml
7) N-EICOSANE	12.505f	79237	0.604 ug/ml
8) N-DOCOSANE	13.755	114813	0.886 ug/ml
10) N-TETRACOSANE	14.835	1168412	9.123 ug/ml
11) N-HEXACOSANE	15.875	285998	2.267 ug/ml
12) N-OCTACOSANE	16.825	716113	5.790 ug/ml
13) N-TRIACONTANE	17.707	659248	5.431 ug/ml
14) N-DOTRIACONTANE	18.535	531708	4.645 ug/ml
15) N-TETRATRIACONTANE	19.321	125041	1.163 ug/ml
16) N-HEXATRIACONTANE	20.086	141336	1.407 ug/ml
17) N-OCTATRIACONTANE	20.766	177415	2.002 ug/ml
18) N-TETRACONTANE	21.682	239233	2.673 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
Data File : FF005998.D
Signal(s) : FID2B.ch
Acq On : 04 Dec 2019 18:45
Operator : DD\AJ
Sample : K6119-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 05 00:18:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

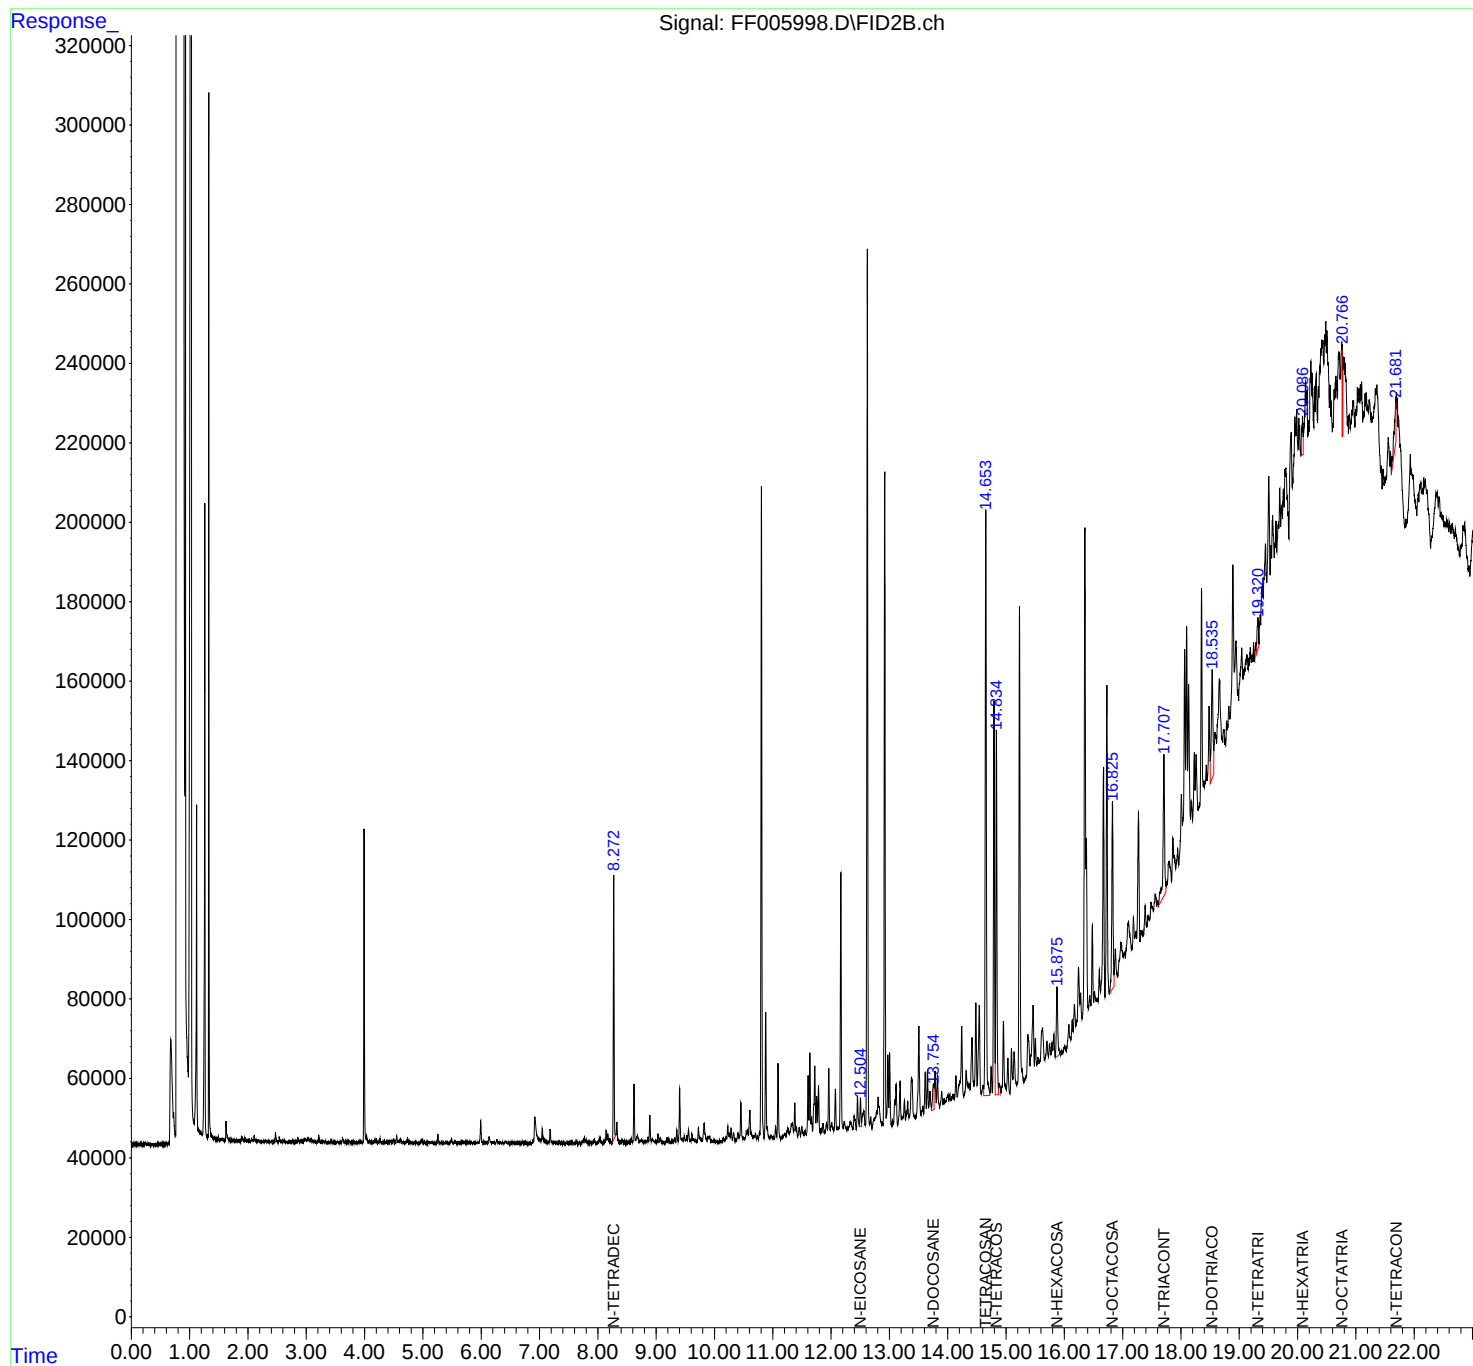


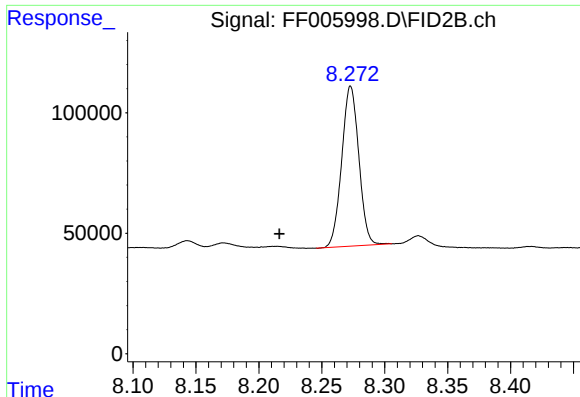

#4 N-TETRADECANE


R.T.: 8.273 min
Delta R.T.: 0.057 min
Response: 627039
Conc: 4.81 ug/ml

Instrument :
FID_F
ClientSampleId :

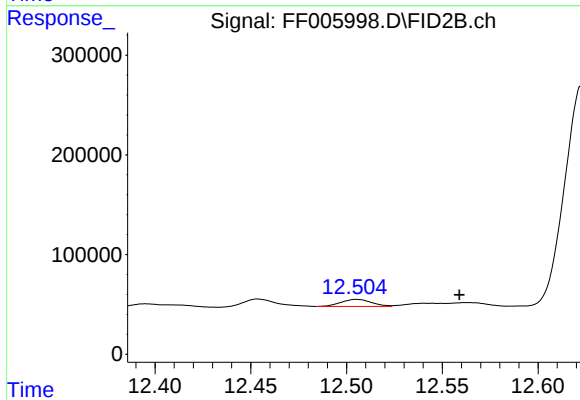


#7 N-EICOSANE

R.T.: 12.505 min
Delta R.T.: -0.054 min
Response: 79237
Conc: 0.60 ug/ml

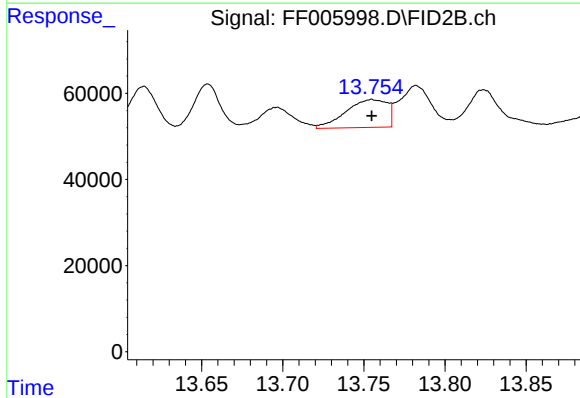


#8 N-DOCOSANE

R.T.: 13.755 min
Delta R.T.: 0.000 min
Response: 114813
Conc: 0.89 ug/ml

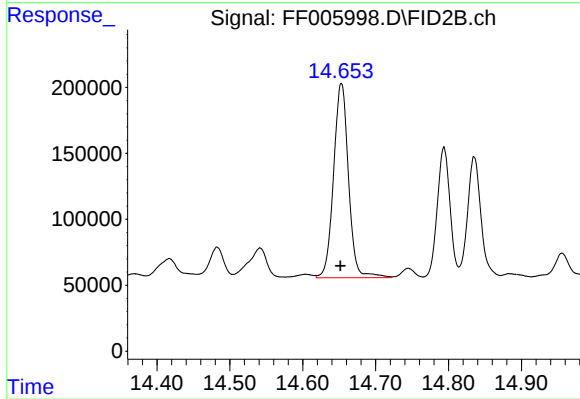

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.653 min
Delta R.T.: 0.002 min
Response: 2100059
Conc: 18.69 ug/ml

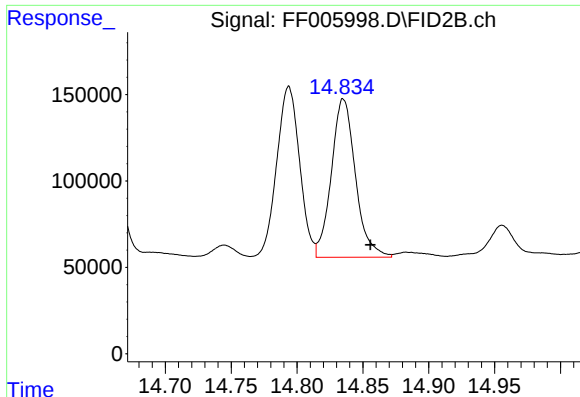

#10 N-TETRACOSANE


R.T.: 14.835 min
Delta R.T.: -0.021 min
Response: 1168412
Conc: 9.12 ug/ml

Instrument :
FID_F
ClientSampleId :

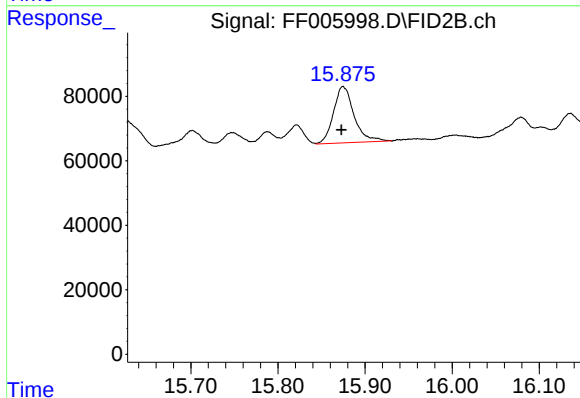


#11 N-HEXACOSANE

R.T.: 15.875 min
Delta R.T.: 0.002 min
Response: 285998
Conc: 2.27 ug/ml

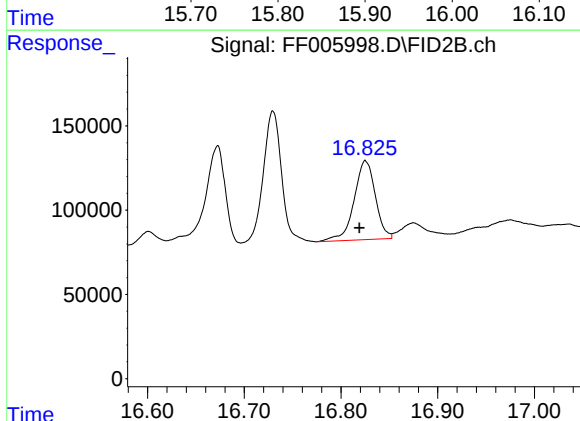


#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: 0.006 min
Response: 716113
Conc: 5.79 ug/ml

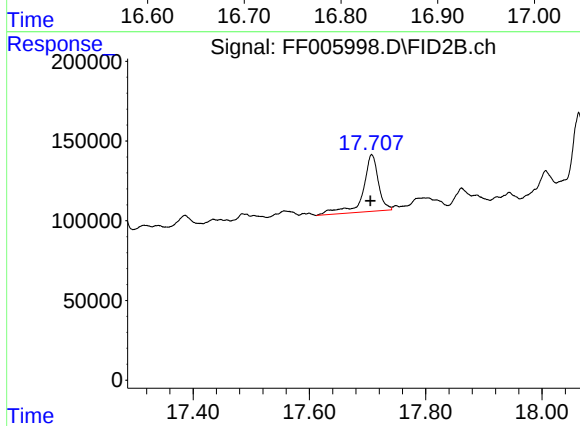

#13 N-TRIACONTANE


R.T.: 17.707 min
Delta R.T.: 0.002 min
Response: 659248
Conc: 5.43 ug/ml

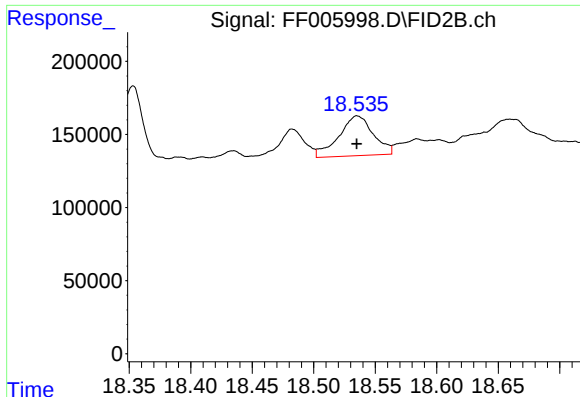

#14 N-DOTRIACONTANE


R.T.: 18.535 min
Delta R.T.: 0.000 min
Response: 531708
Conc: 4.64 ug/ml

Instrument :
FID_F
ClientSampleId :

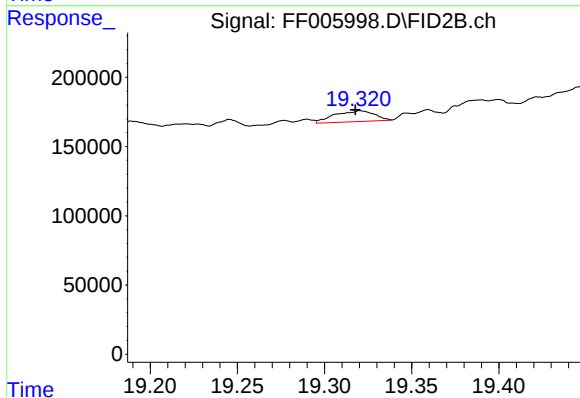


#15 N-TETRATRIACONTANE

R.T.: 19.321 min
Delta R.T.: 0.003 min
Response: 125041
Conc: 1.16 ug/ml

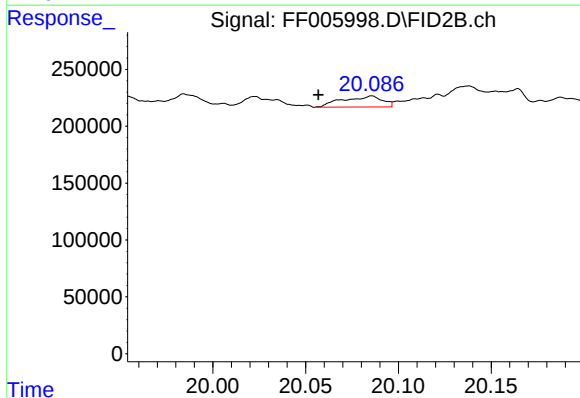


#16 N-HEXATRIACONTANE

R.T.: 20.086 min
Delta R.T.: 0.029 min
Response: 141336
Conc: 1.41 ug/ml

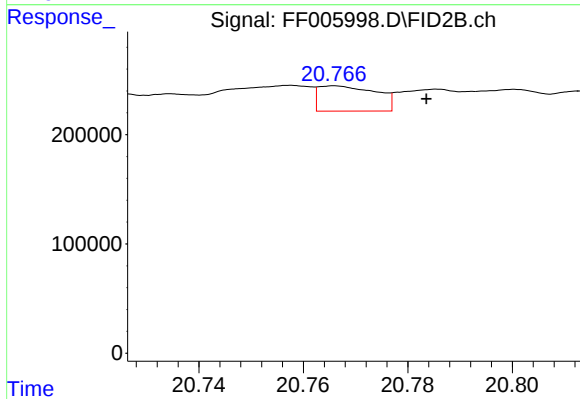

#17 N-OCTATRIACONTANE

R.T.: 20.766 min
Delta R.T.: -0.018 min
Response: 177415
Conc: 2.00 ug/ml

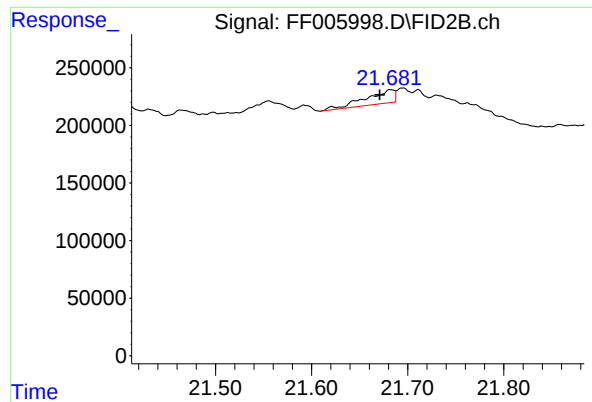

#18 N-TETRACONTANE

R.T.: 21.682 min
Delta R.T.: 0.011 min
Response: 239233
Conc: 2.67 ug/ml

Instrument :
FID_F
ClientSampleId :