

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
 Data File : FF005999.D
 Signal(s) : FID2B.ch
 Acq On : 04 Dec 2019 19:15
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 05 00:18:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	2191972	19.504 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.821	62131	0.502 ug/ml
13) N-TRIACONTANE	17.706	24575	0.202 ug/ml
14) N-DOTRIACONTANE	18.542	284442	2.485 ug/ml
15) N-TETRATRIACONTANE	19.321	230874	2.147 ug/ml
16) N-HEXATRIACONTANE	20.092	747737	7.444 ug/ml
17) N-OCTATRIACONTANE	20.786	111983	1.264 ug/ml
18) N-TETRACONTANE	21.705	1557576	17.400 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
Data File : FF005999.D
Signal(s) : FID2B.ch
Acq On : 04 Dec 2019 19:15
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 05 00:18:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

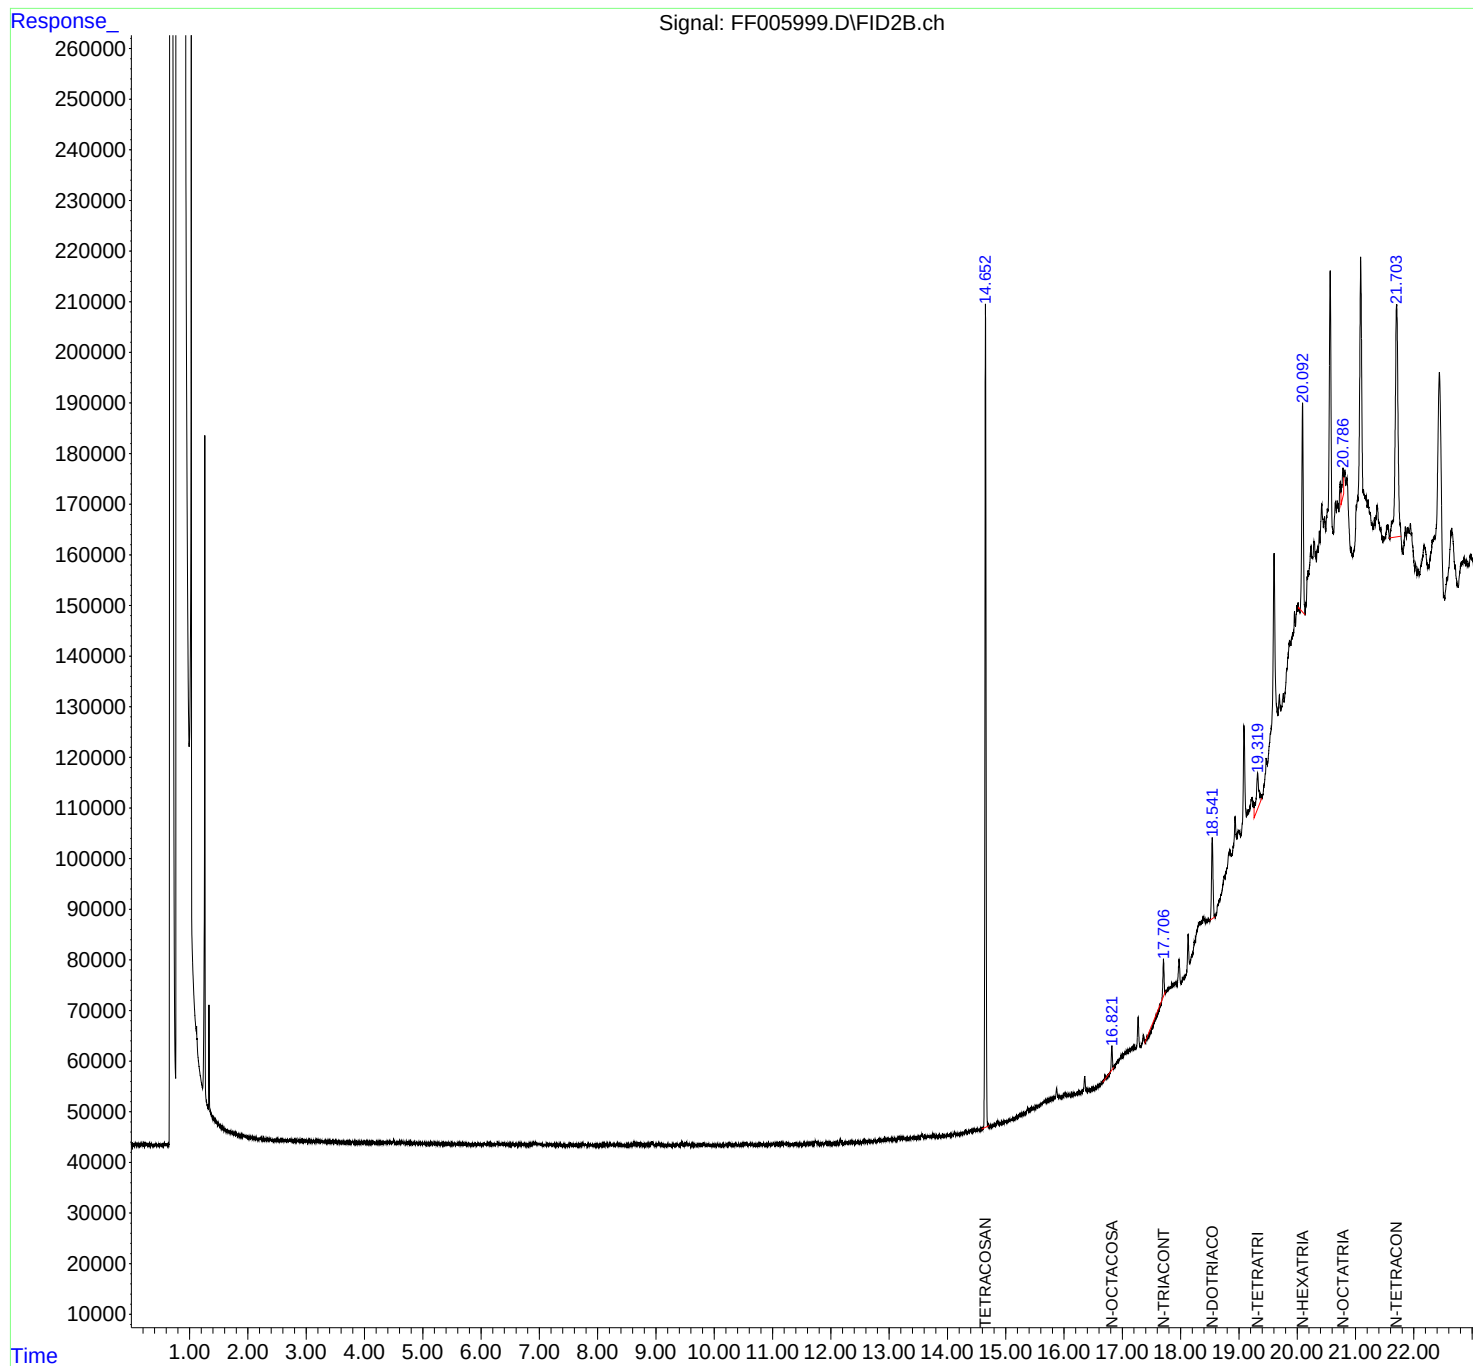


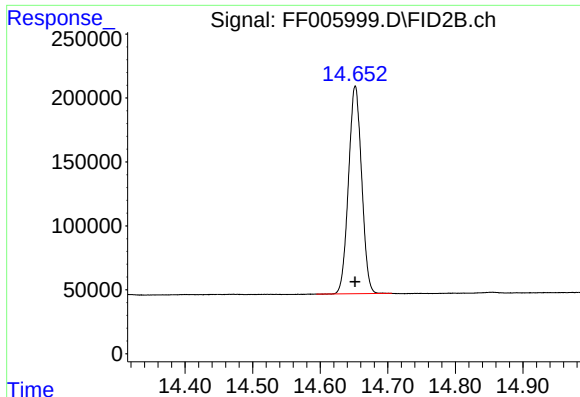

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.652 min
Delta R.T.: 0.000 min
Response: 2191972
Conc: 19.50 ug/ml

Instrument :
FID_F
ClientSampleId :

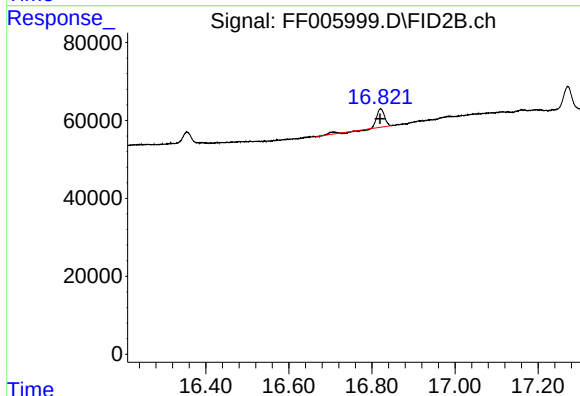


#12 N-OCTACOSANE

R.T.: 16.821 min
Delta R.T.: 0.002 min
Response: 62131
Conc: 0.50 ug/ml

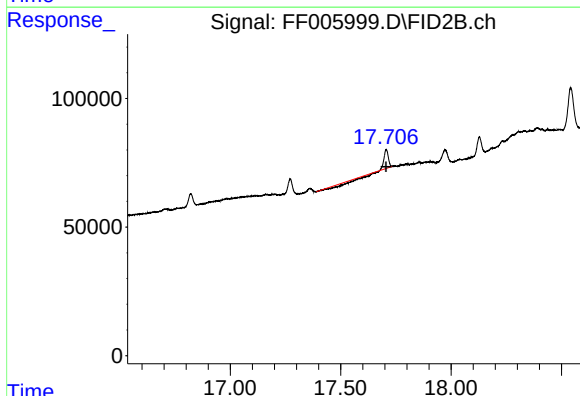


#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: 0.000 min
Response: 24575
Conc: 0.20 ug/ml

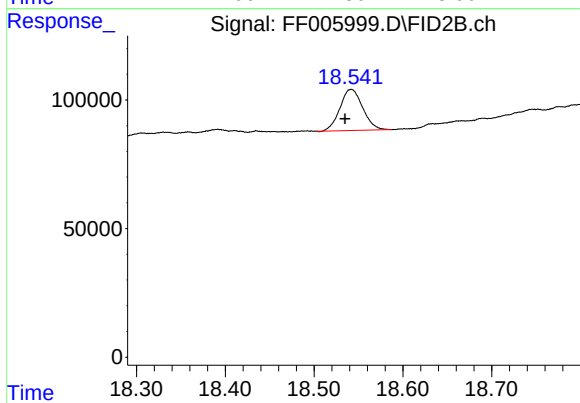

#14 N-DOTRIACONTANE


R.T.: 18.542 min
Delta R.T.: 0.007 min
Response: 284442
Conc: 2.48 ug/ml

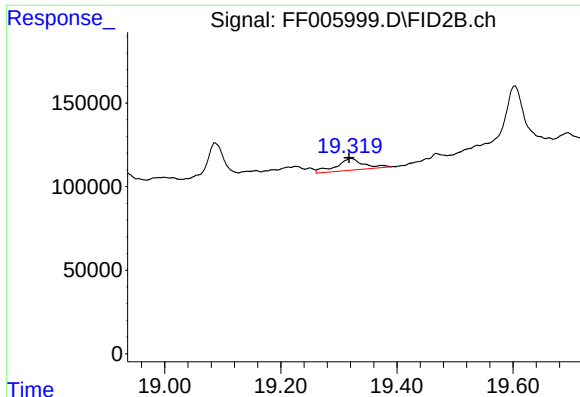

#15 N-TETRATRIACONTANE


R.T.: 19.321 min
Delta R.T.: 0.003 min
Response: 230874
Conc: 2.15 ug/ml

Instrument :
FID_F
ClientSampleId :

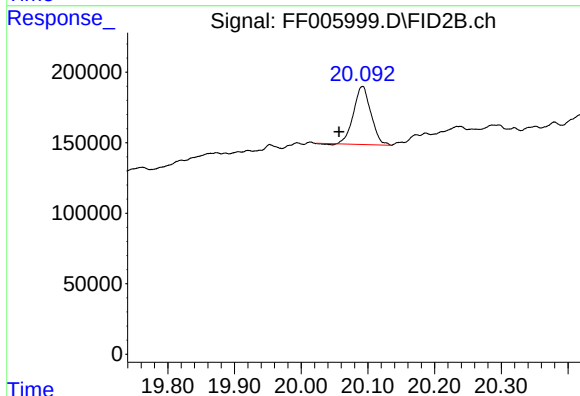


#16 N-HEXATRIACONTANE

R.T.: 20.092 min
Delta R.T.: 0.035 min
Response: 747737
Conc: 7.44 ug/ml

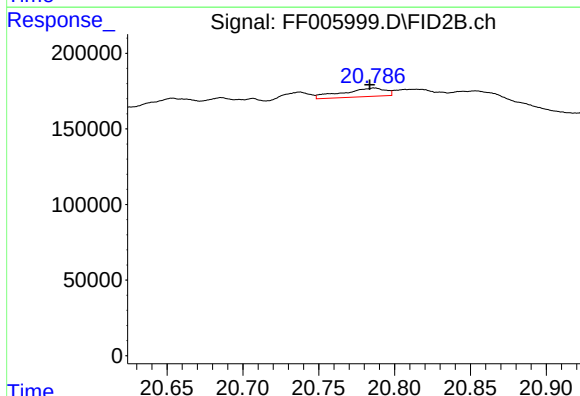

#17 N-OCTATRIACONTANE

R.T.: 20.786 min
Delta R.T.: 0.003 min
Response: 111983
Conc: 1.26 ug/ml

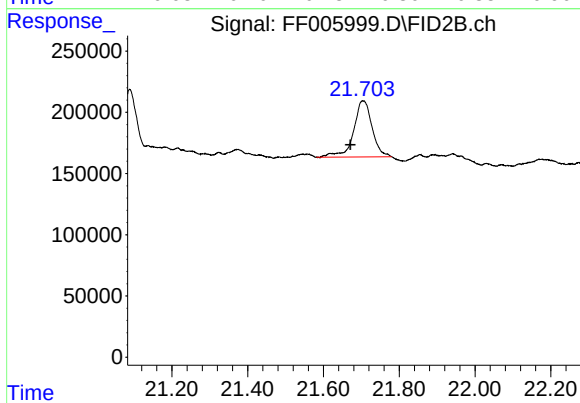

#18 N-TETRACONTANE

R.T.: 21.705 min
Delta R.T.: 0.034 min
Response: 1557576
Conc: 17.40 ug/ml