

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
 Data File : FF005990.D
 Signal(s) : FID2B.ch
 Acq On : 04 Dec 2019 13:15
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Dec 05 00:16:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.421	2746154	21.101 ug/ml
12) N-OCTACOSANE	16.820	2564650	20.737 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
Data File : FF005990.D
Signal(s) : FID2B.ch
Acq On : 04 Dec 2019 13:15
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 05 00:16:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

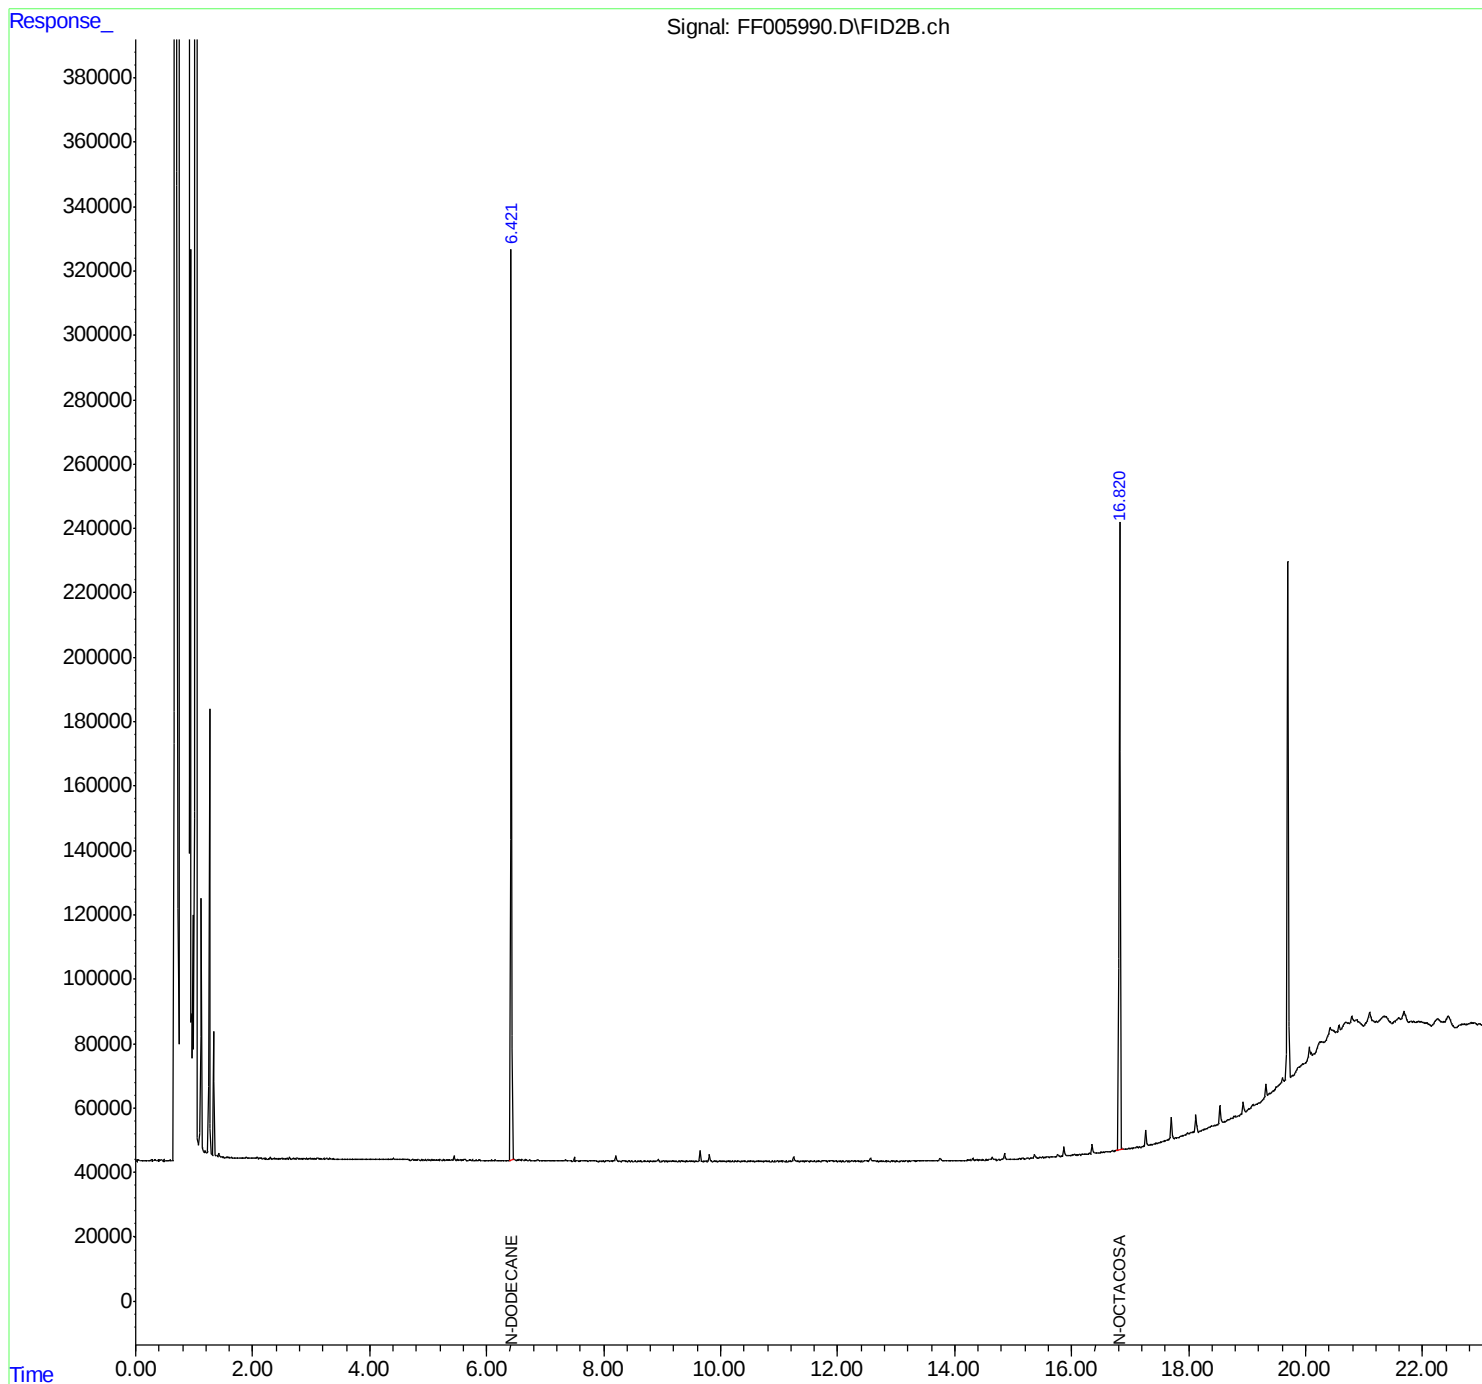


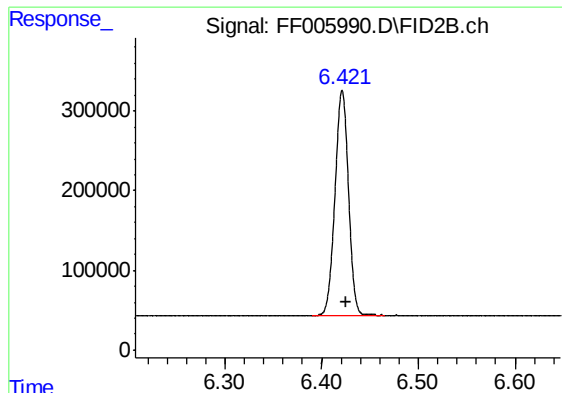

#3 N-DODECANE


R.T.: 6.421 min
Delta R.T.: -0.004 min
Response: 2746154
Conc: 21.10 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

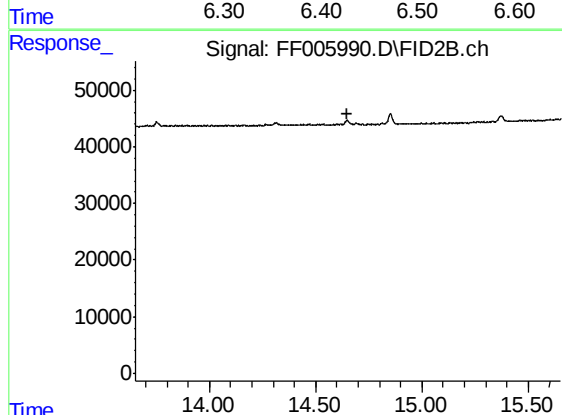

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.651 min
Response: 0
Conc: N.D.

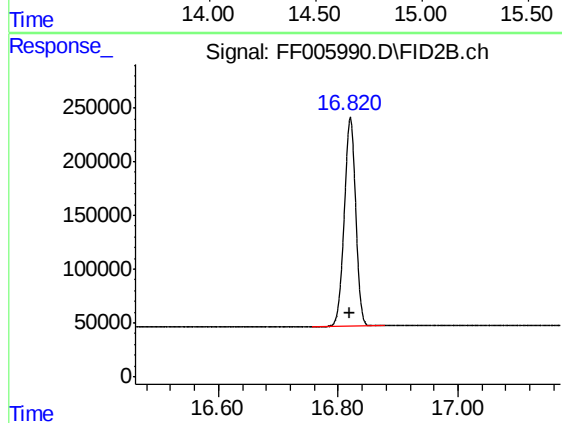

#12 N-OCTACOSANE

R.T.: 16.820 min
Delta R.T.: 0.001 min
Response: 2564650
Conc: 20.74 ug/ml