

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
 Data File : FF005991.D
 Signal(s) : FID2B.ch
 Acq On : 04 Dec 2019 15:14
 Operator : DD\AJ
 Sample : PB125240BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB125240BS

Integration File: autoint1.e
 Quant Time: Dec 05 00:16:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	2189738	19.484 ug/ml
Target Compounds			
2) N-DECANE	4.399	2580868	20.095 ug/ml
3) N-DODECANE	6.417	2676794	20.568 ug/ml
4) N-TETRADECANE	8.209	2697384	20.696 ug/ml
5) N-HEXADECANE	9.807	2724163	20.686 ug/ml
6) N-OCTADECANE	11.246	2704787	20.741 ug/ml
7) N-EICOSANE	12.555	2675435	20.407 ug/ml
8) N-DOCOSANE	13.751	2627454	20.283 ug/ml
10) N-TETRACOSANE	14.852	2591667	20.235 ug/ml
11) N-HEXACOSANE	15.870	2544978	20.169 ug/ml
12) N-OCTACOSANE	16.819	2540791	20.544 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120419\
Data File : FF005991.D
Signal(s) : FID2B.ch
Acq On : 04 Dec 2019 15:14
Operator : DD\AJ
Sample : PB125240BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB125240BS

Integration File: autoint1.e
Quant Time: Dec 05 00:16:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

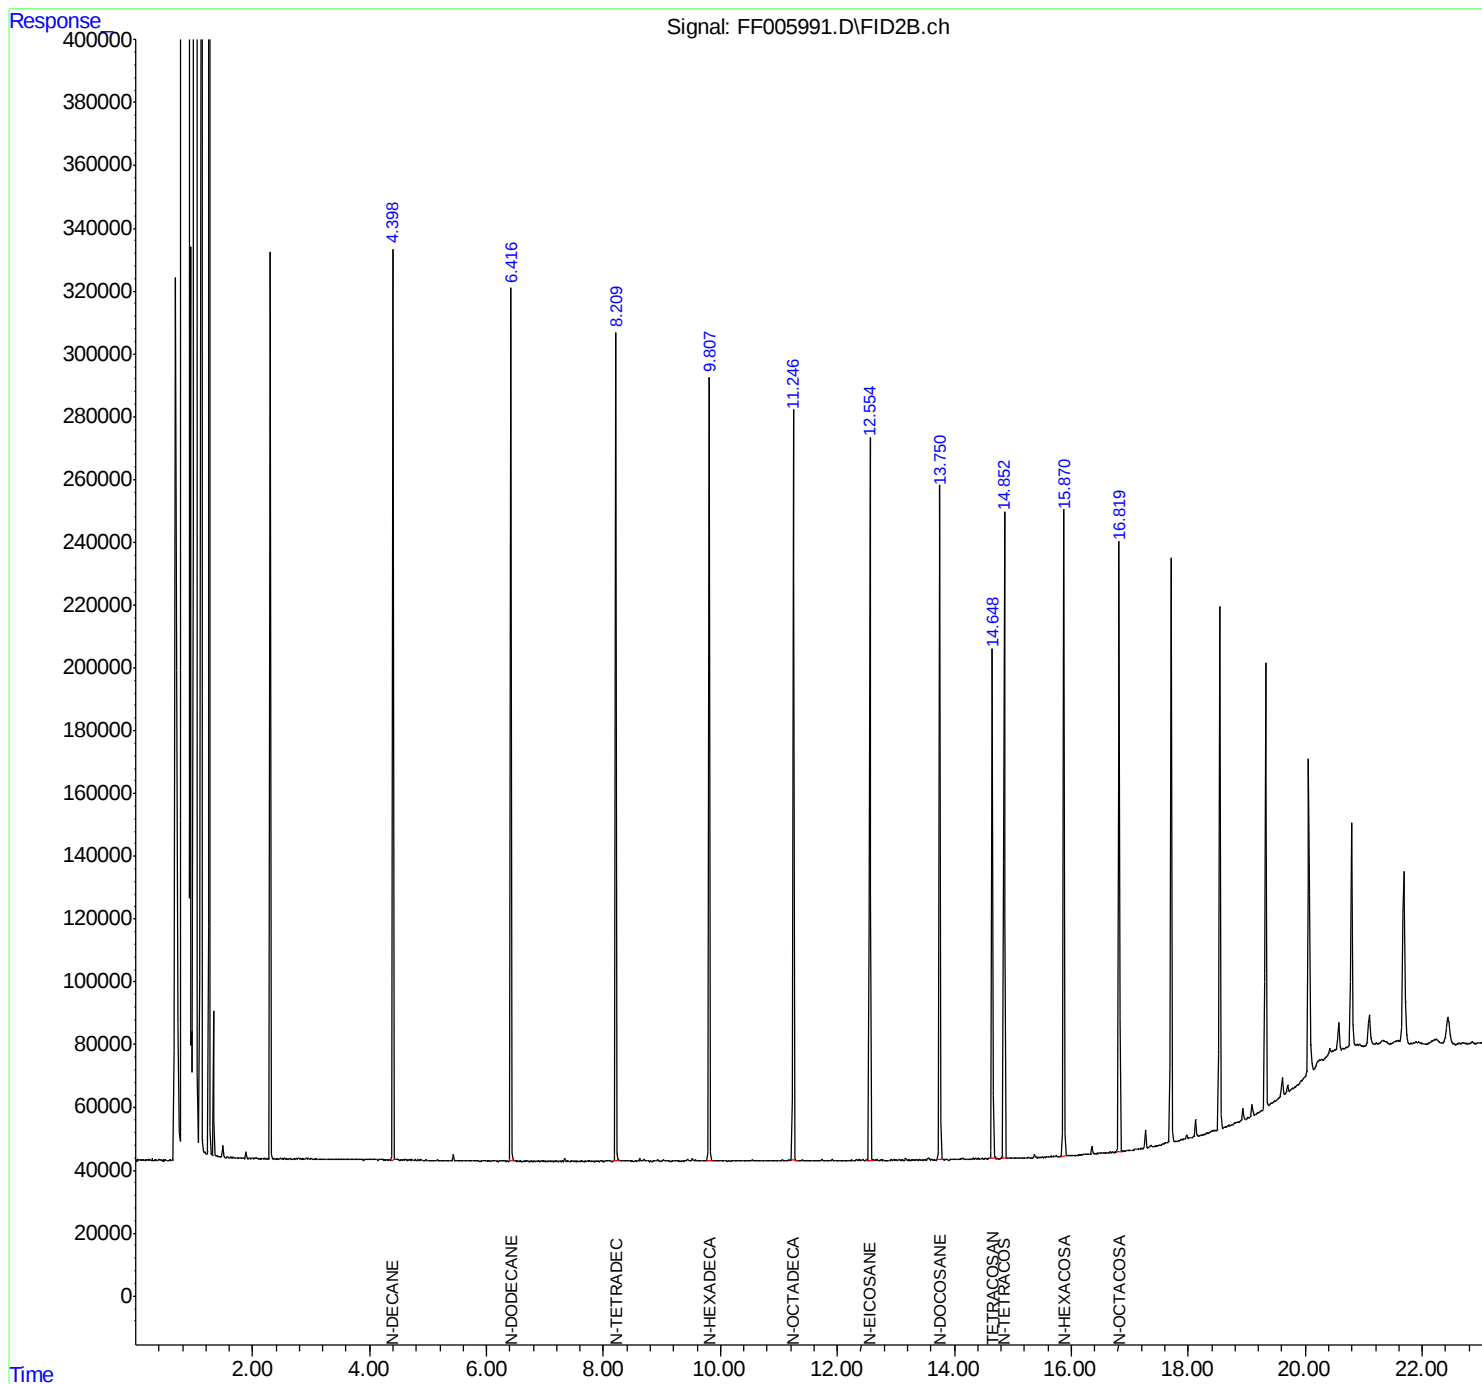


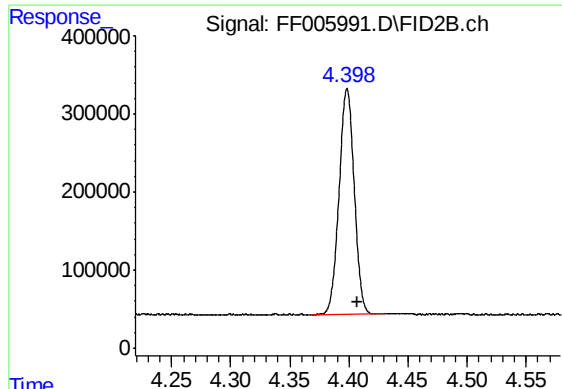

#2 N-DECANE


R.T.: 4.399 min
Delta R.T.: -0.009 min
Response: 2580868
Conc: 20.10 ug/ml

Instrument :
FID_F
ClientSampleId :
PB125240BS

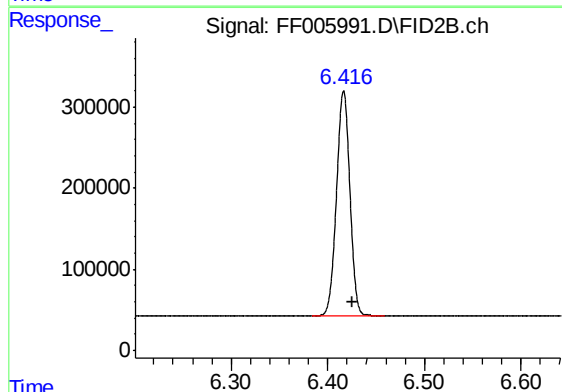


#3 N-DODECANE

R.T.: 6.417 min
Delta R.T.: -0.009 min
Response: 2676794
Conc: 20.57 ug/ml

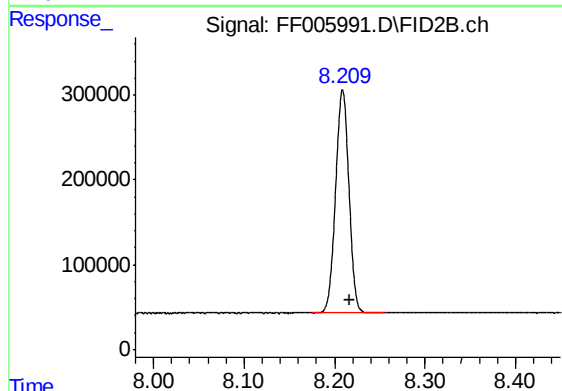


#4 N-TETRADECANE

R.T.: 8.209 min
Delta R.T.: -0.007 min
Response: 2697384
Conc: 20.70 ug/ml

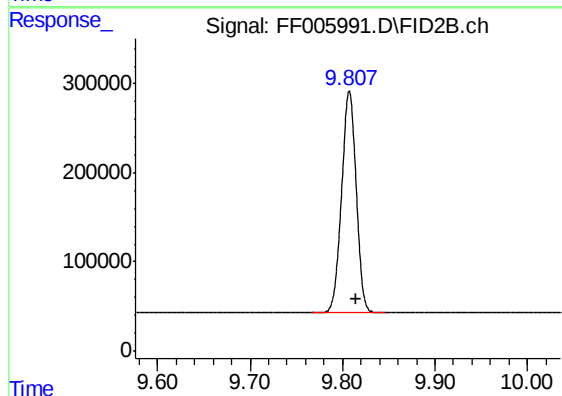

#5 N-HEXADECANE


R.T.: 9.807 min
Delta R.T.: -0.007 min
Response: 2724163
Conc: 20.69 ug/ml

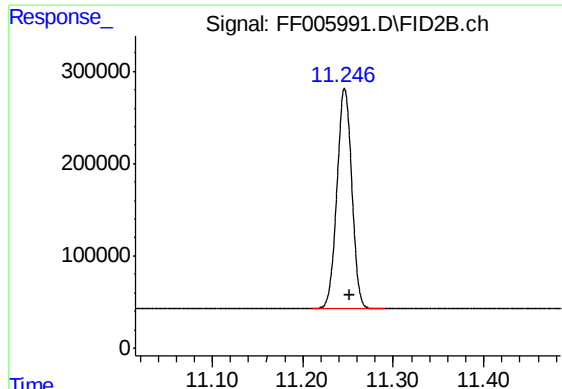

#6 N-OCTADECANE


R.T.: 11.246 min
Delta R.T.: -0.006 min
Response: 2704787
Conc: 20.74 ug/ml

Instrument :
FID_F
ClientSampleId :
PB125240BS

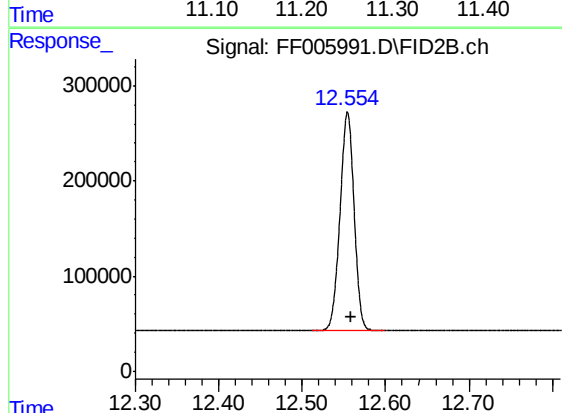


#7 N-EICOSANE

R.T.: 12.555 min
Delta R.T.: -0.004 min
Response: 2675435
Conc: 20.41 ug/ml

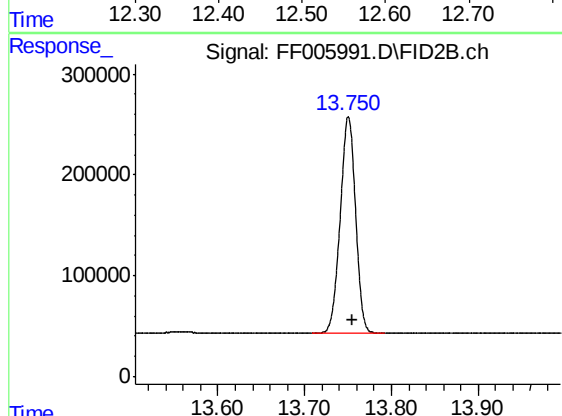


#8 N-DOCOSANE

R.T.: 13.751 min
Delta R.T.: -0.004 min
Response: 2627454
Conc: 20.28 ug/ml

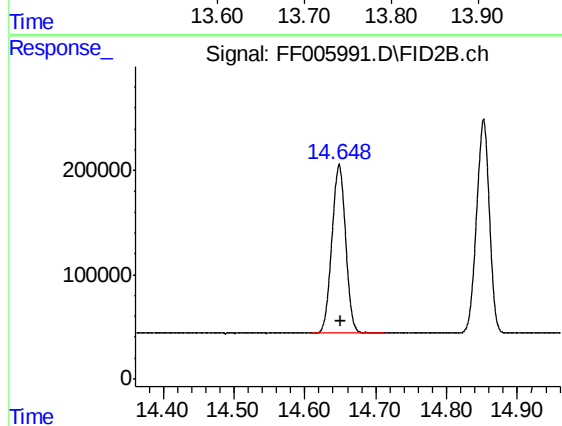

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.649 min
Delta R.T.: -0.003 min
Response: 2189738
Conc: 19.48 ug/ml

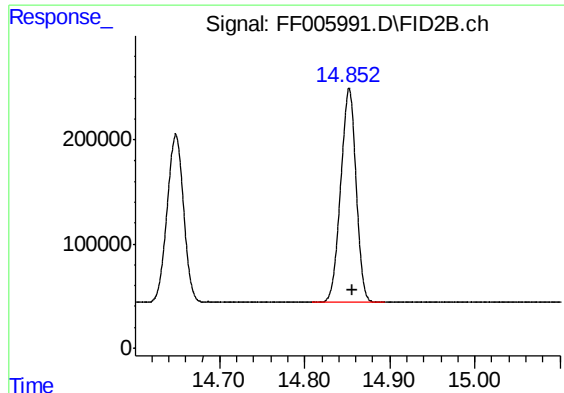

#10 N-TETRACOSANE


R.T.: 14.852 min
Delta R.T.: -0.003 min
Response: 2591667
Conc: 20.24 ug/ml

Instrument :
FID_F
ClientSampleId :
PB125240BS

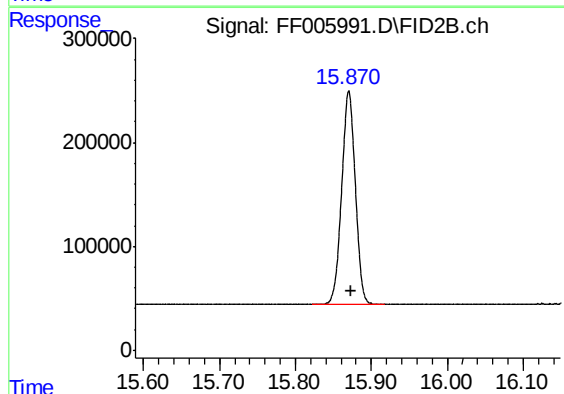

#11 N-HEXACOSANE

R.T.: 15.870 min
Delta R.T.: -0.003 min
Response: 2544978
Conc: 20.17 ug/ml

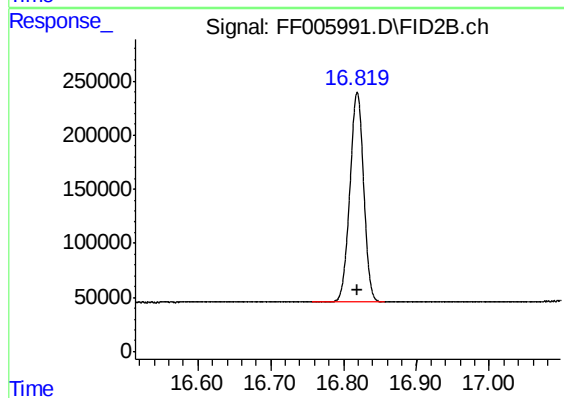

#12 N-OCTACOSANE

R.T.: 16.819 min
Delta R.T.: 0.000 min
Response: 2540791
Conc: 20.54 ug/ml