

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002902.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 14:48
 Operator : AJ\SJ
 Sample : J6208-21
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:05:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.656	3676195	28.316 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242f	1113260	6.945 ug/ml
5) N-HEXADECANE	9.790	193423	1.208 ug/ml
6) N-OCTADECANE	11.249	297857	1.880 ug/ml
7) N-EICOSANE	12.547	519065	3.366 ug/ml
8) N-DOCOSANE	13.768	2160174	14.446 ug/ml
10) N-TETRACOSANE	14.841	8133335	56.280 ug/ml
11) N-HEXACOSANE	15.877	975253	6.987 ug/ml
12) N-OCTACOSANE	16.830	3673061	27.414 ug/ml
13) N-TRIACONTANE	17.716	5672896	44.273 ug/ml
14) N-DOTRIACONTANE	18.516	35343406	295.956 ug/ml
15) N-TETRATRIACONTANE	19.322	379806	3.351 ug/ml
16) N-HEXATRIACONTANE	20.063	6855778	63.540 ug/ml
17) N-OCTATRIACONTANE	20.794	966173	9.519 ug/ml
18) N-TETRACONTANE	21.713	170877	1.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002902.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 14:48
Operator : AJ\SJ
Sample : J6208-21
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Dec 06 03:05:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

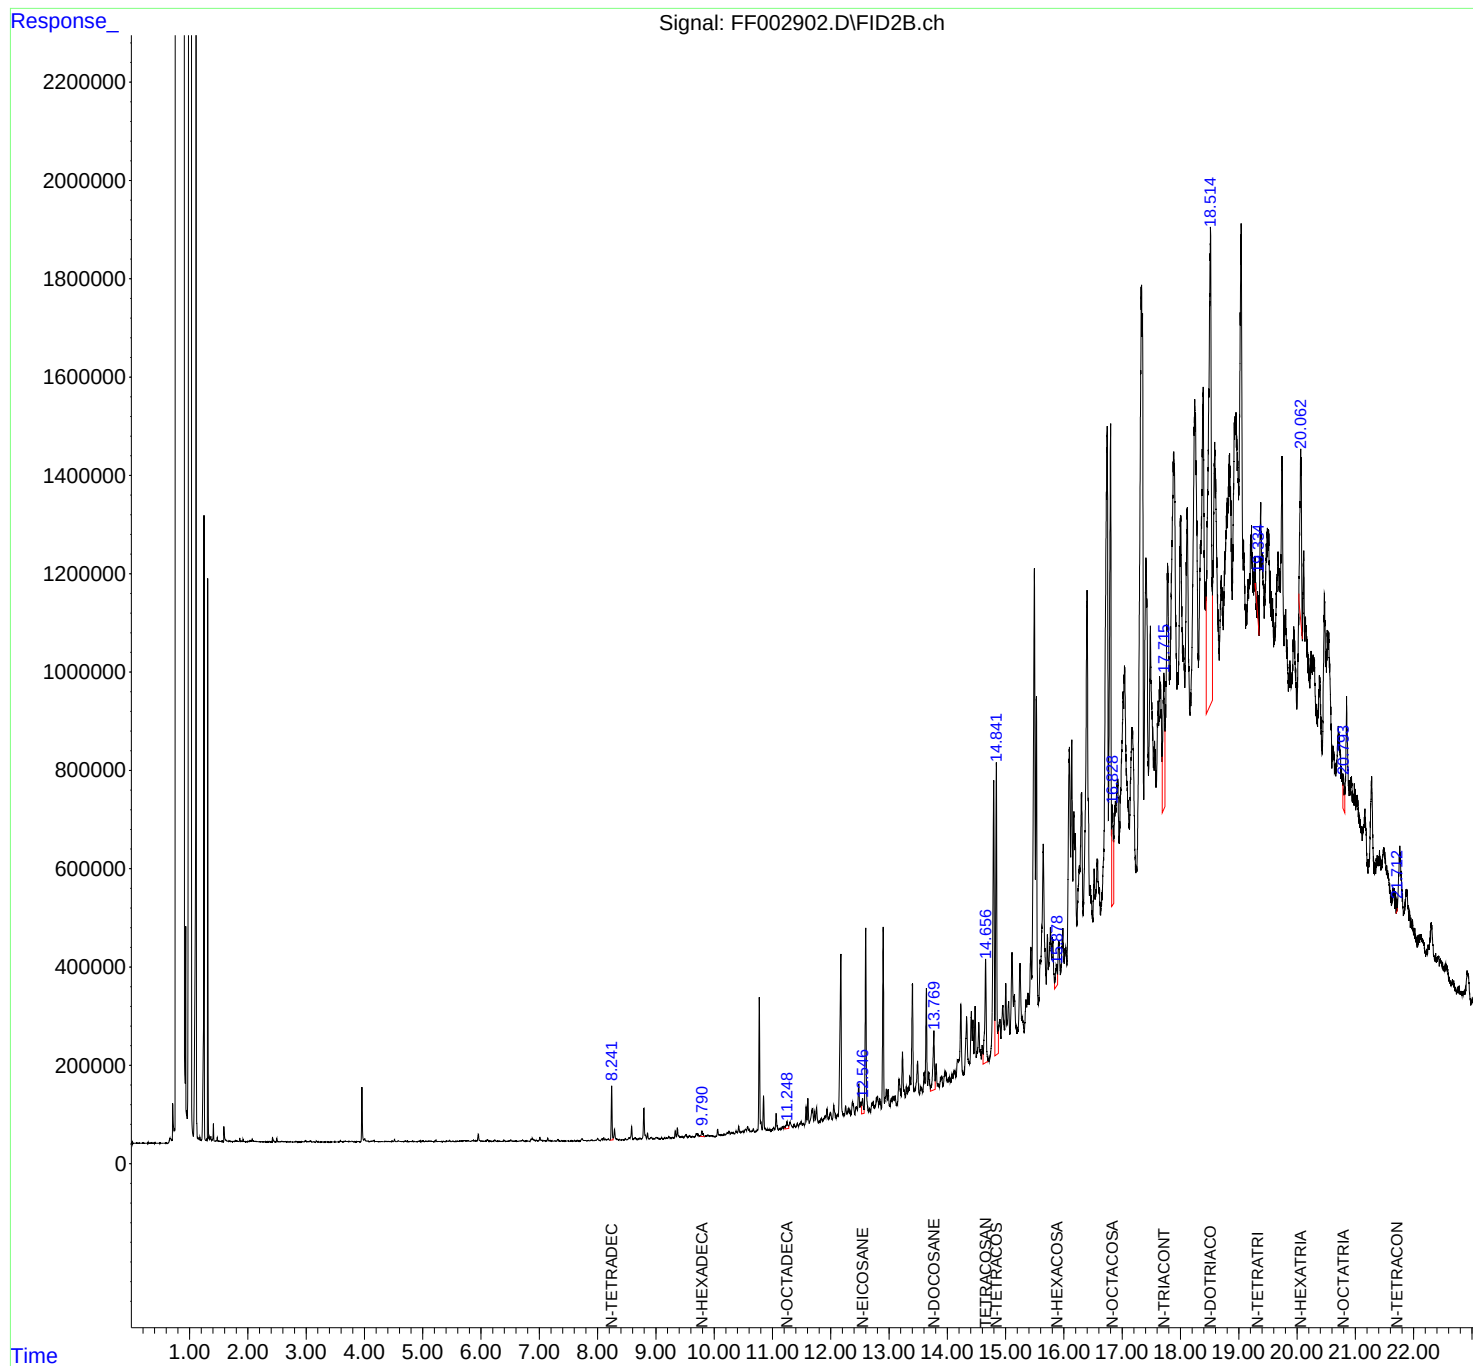


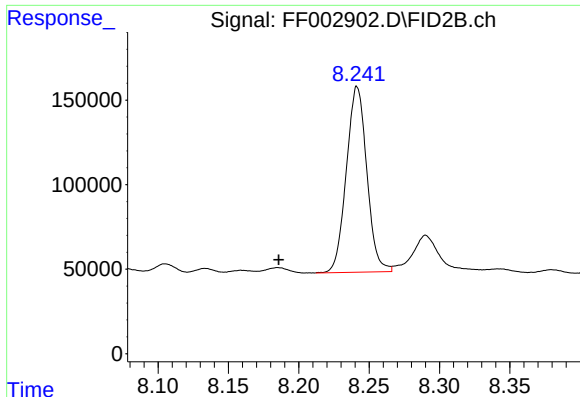

#4 N-TETRADECANE


R.T.: 8.242 min
Delta R.T.: 0.056 min
Response: 1113260
Conc: 6.95 ug/ml

Instrument :
FID_F
ClientSampleId :

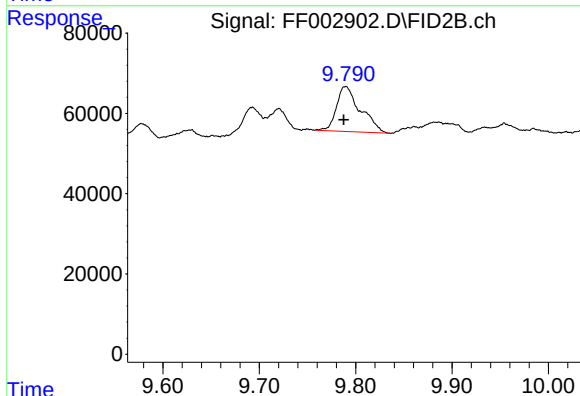


#5 N-HEXADECANE

R.T.: 9.790 min
Delta R.T.: 0.002 min
Response: 193423
Conc: 1.21 ug/ml

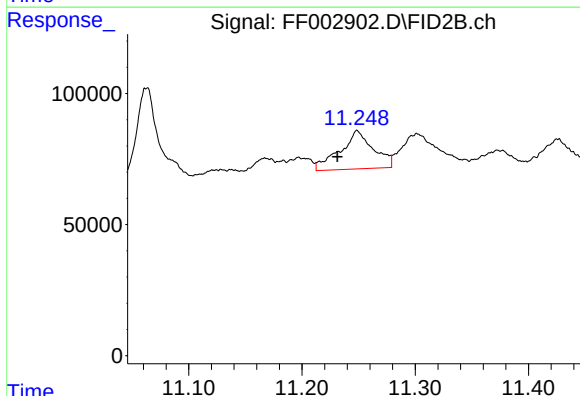


#6 N-OCTADECANE

R.T.: 11.249 min
Delta R.T.: 0.018 min
Response: 297857
Conc: 1.88 ug/ml

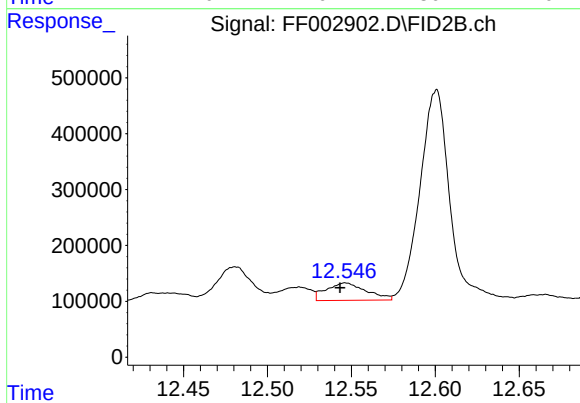

#7 N-EICOSANE


R.T.: 12.547 min
Delta R.T.: 0.003 min
Response: 519065
Conc: 3.37 ug/ml

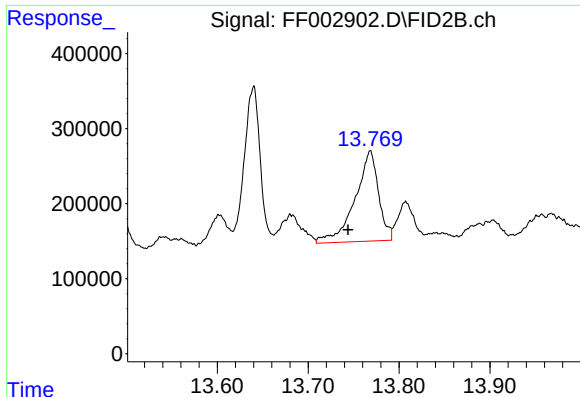

#8 N-DOCOSANE


R.T.: 13.768 min
Delta R.T.: 0.025 min
Response: 2160174
Conc: 14.45 ug/ml

Instrument :
FID_F
ClientSampleId :

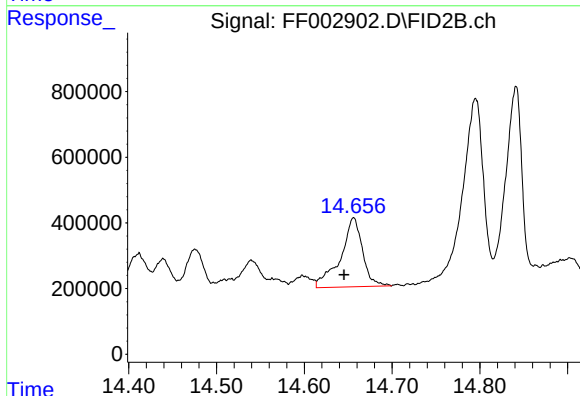


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: 0.011 min
Response: 3676195
Conc: 28.32 ug/ml

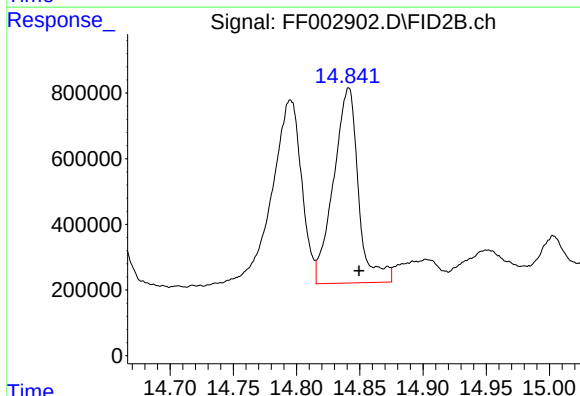


#10 N-TETRACOSANE

R.T.: 14.841 min
Delta R.T.: -0.008 min
Response: 8133335
Conc: 56.28 ug/ml

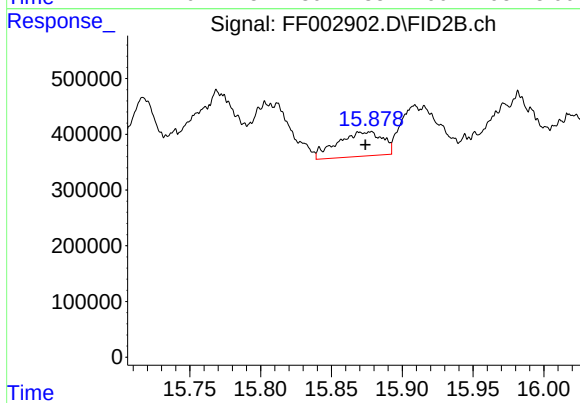

#11 N-HEXACOSANE


R.T.: 15.877 min
Delta R.T.: 0.003 min
Response: 975253
Conc: 6.99 ug/ml

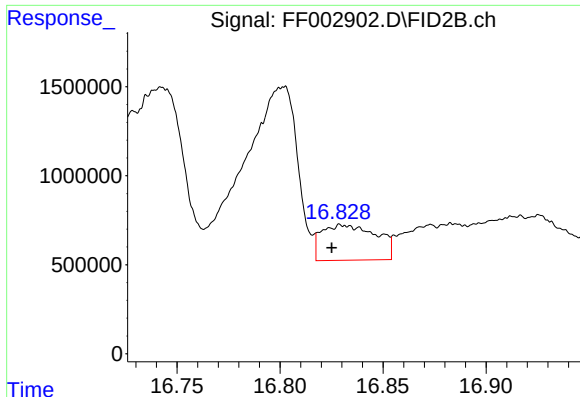

#12 N-OCTACOSANE


R.T.: 16.830 min
Delta R.T.: 0.005 min
Response: 3673061
Conc: 27.41 ug/ml

Instrument :
FID_F
ClientSampleId :

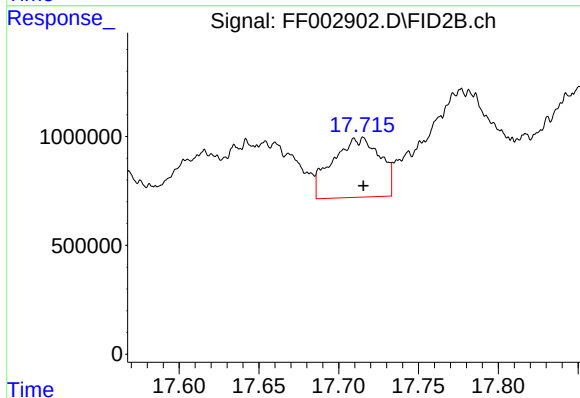


#13 N-TRIACONTANE

R.T.: 17.716 min
Delta R.T.: 0.000 min
Response: 5672896
Conc: 44.27 ug/ml

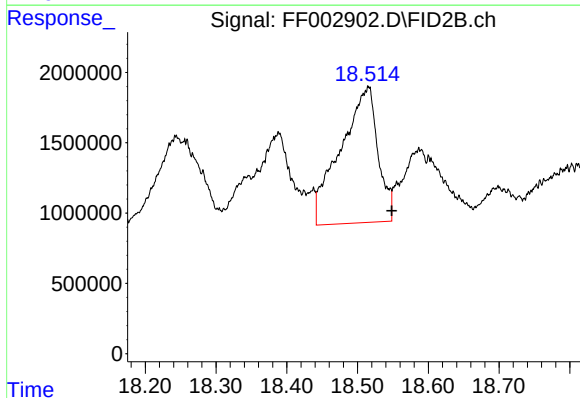


#14 N-DOTRIACONTANE

R.T.: 18.516 min
Delta R.T.: -0.033 min
Response: 35343406
Conc: 295.96 ug/ml

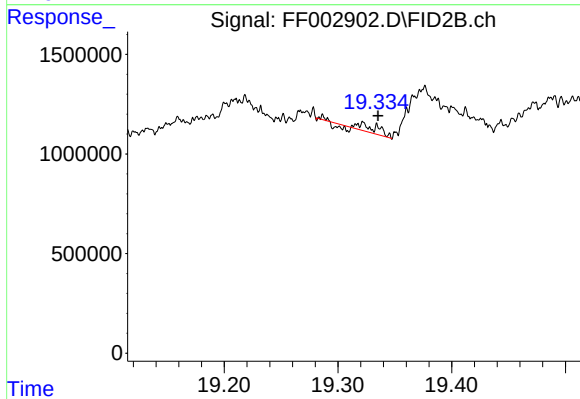

#15 N-TETRATRIACONTANE


R.T.: 19.322 min
Delta R.T.: -0.013 min
Response: 379806
Conc: 3.35 ug/ml

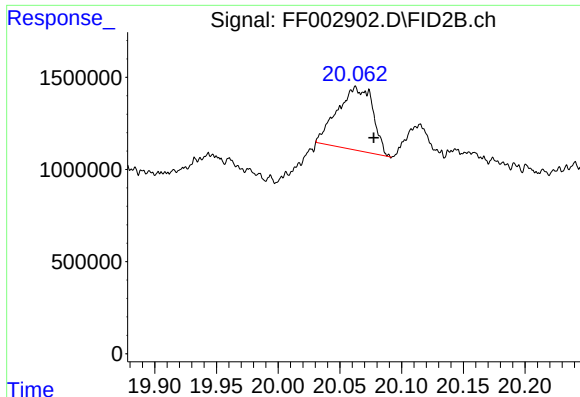

#16 N-HEXATRIACONTANE


R.T.: 20.063 min
Delta R.T.: -0.015 min
Response: 6855778
Conc: 63.54 ug/ml

Instrument :
FID_F
ClientSampleId :

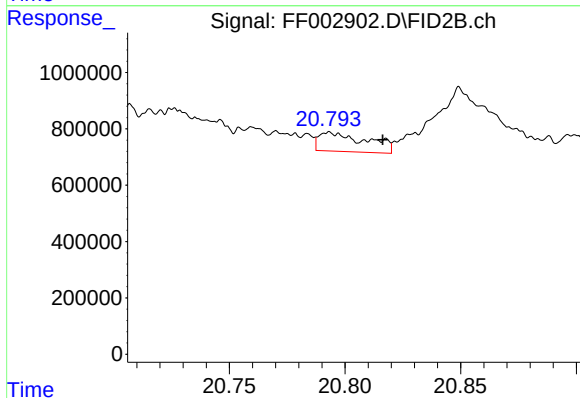

#17 N-OCTATRIACONTANE

R.T.: 20.794 min
Delta R.T.: -0.023 min
Response: 966173
Conc: 9.52 ug/ml

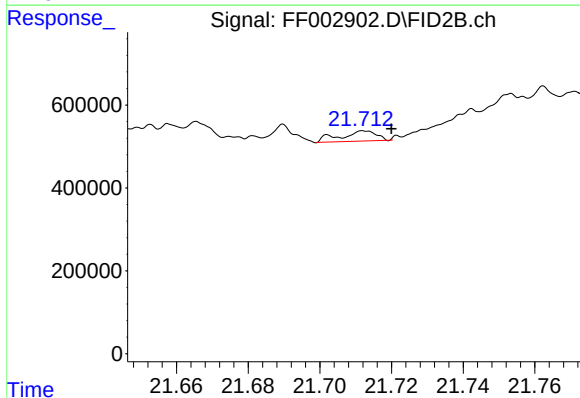

#18 N-TETRACONTANE

R.T.: 21.713 min
Delta R.T.: -0.007 min
Response: 170877
Conc: 1.63 ug/ml