

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002903.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 15:18
 Operator : AJ\SJ
 Sample : J6208-17
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:05:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.656	4048191	31.182 ug/ml
Target Compounds			
4) N-TETRADECANE	8.136	420955	2.626 ug/ml
5) N-HEXADECANE	9.795	1633138	10.198 ug/ml
6) N-OCTADECANE	11.209	232754	1.469 ug/ml
7) N-EICOSANE	12.532	1497700	9.711 ug/ml
8) N-DOCOSANE	13.775	3812818	25.499 ug/ml
10) N-TETRACOSANE	14.853	12520164	86.636 ug/ml
11) N-HEXACOSANE	15.897	837136	5.998 ug/ml
12) N-OCTACOSANE	16.851	3942203	29.422 ug/ml
13) N-TRIACONTANE	17.708	1659557	12.952 ug/ml
14) N-DOTRIACONTANE	18.515	4469266	37.424 ug/ml
15) N-TETRATRIACONTANE	19.301	67388	0.595 ug/ml
16) N-HEXATRIACONTANE	20.073	98913	0.917 ug/ml
17) N-OCTATRIACONTANE	20.768	1109578	10.932 ug/ml
18) N-TETRACONTANE	21.724	1290366	12.277 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002903.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 15:18
Operator : AJ\SJ
Sample : J6208-17
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:05:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

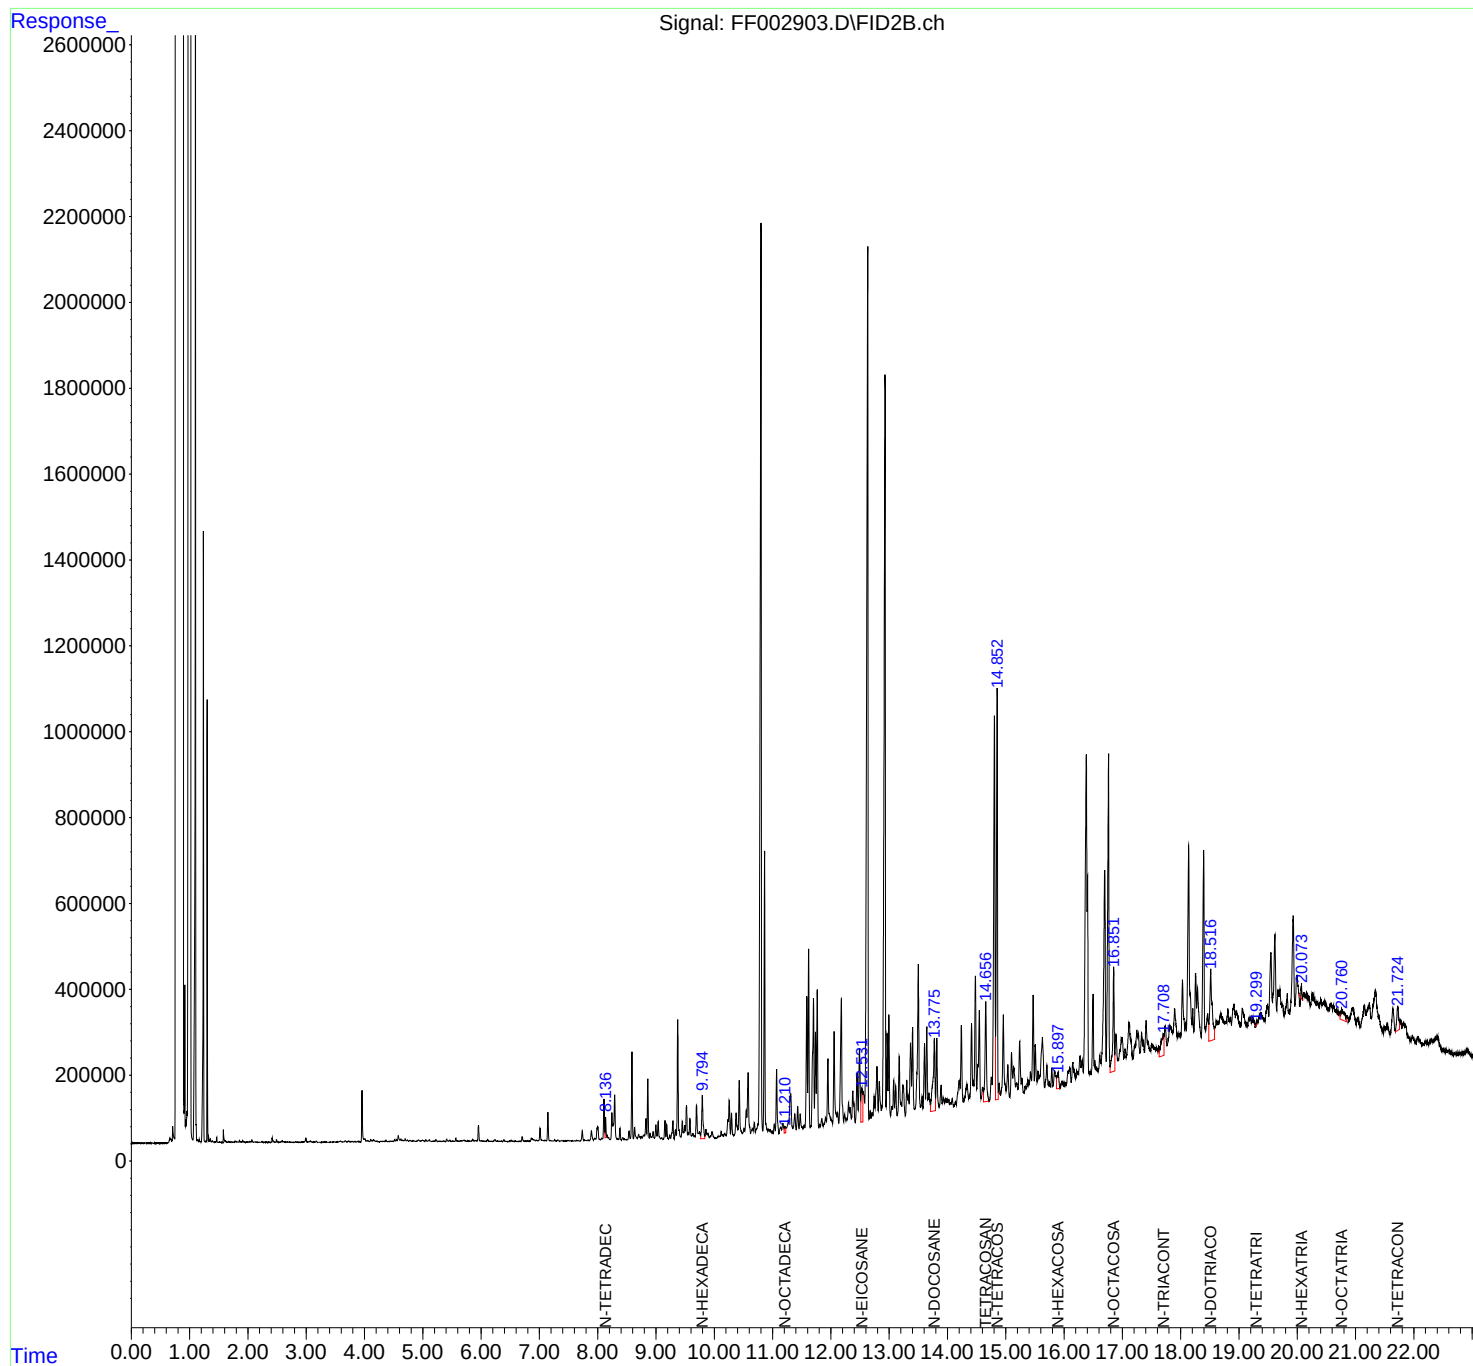


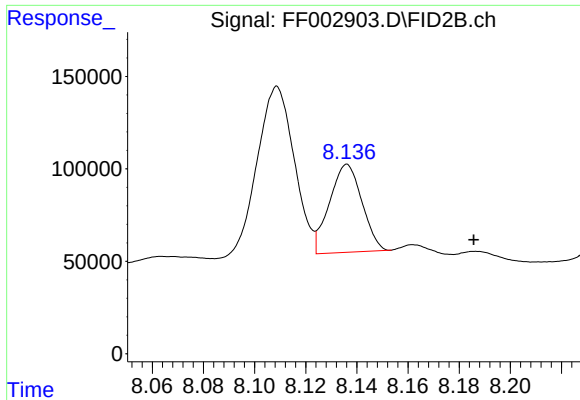

#4 N-TETRADECANE


R.T.: 8.136 min
Delta R.T.: -0.050 min
Response: 420955
Conc: 2.63 ug/ml

Instrument :
FID_F
ClientSampleId :

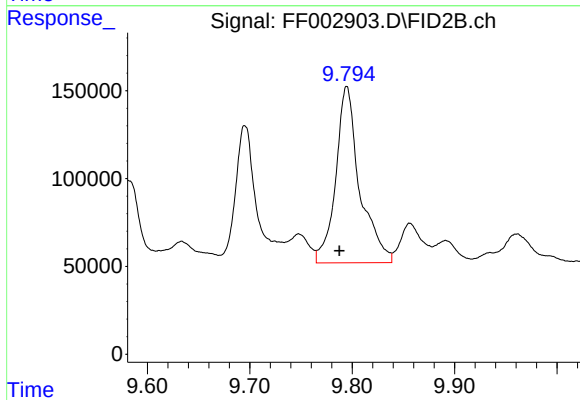


#5 N-HEXADECANE

R.T.: 9.795 min
Delta R.T.: 0.007 min
Response: 1633138
Conc: 10.20 ug/ml

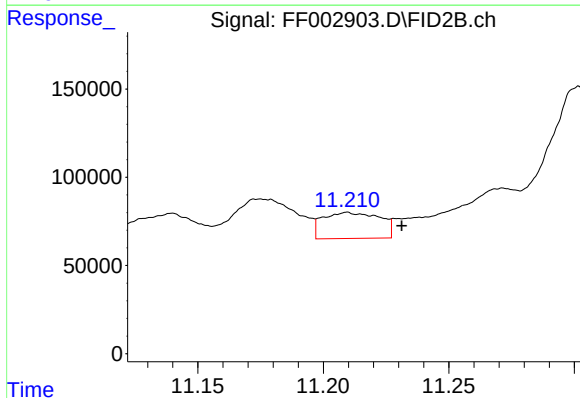


#6 N-OCTADECANE

R.T.: 11.209 min
Delta R.T.: -0.022 min
Response: 232754
Conc: 1.47 ug/ml

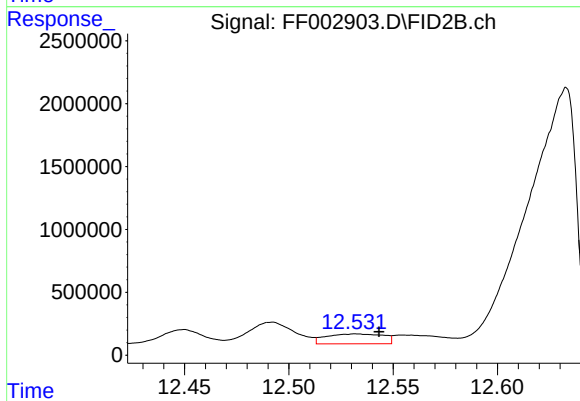

#7 N-EICOSANE


R.T.: 12.532 min
Delta R.T.: -0.011 min
Response: 1497700
Conc: 9.71 ug/ml

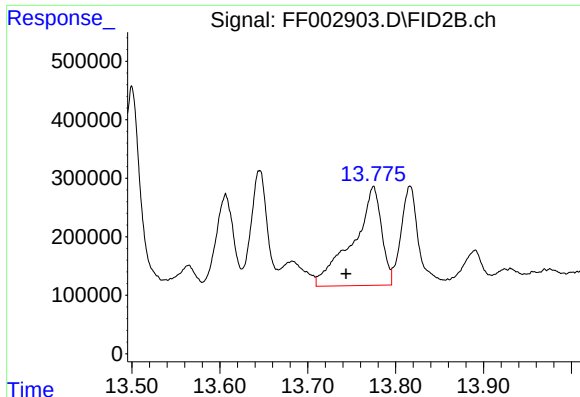

#8 N-DOCOSANE


R.T.: 13.775 min
Delta R.T.: 0.031 min
Response: 3812818
Conc: 25.50 ug/ml

Instrument :
FID_F
ClientSampleId :

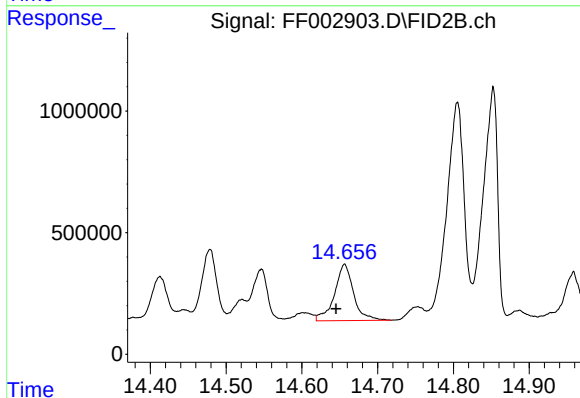


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: 0.011 min
Response: 4048191
Conc: 31.18 ug/ml

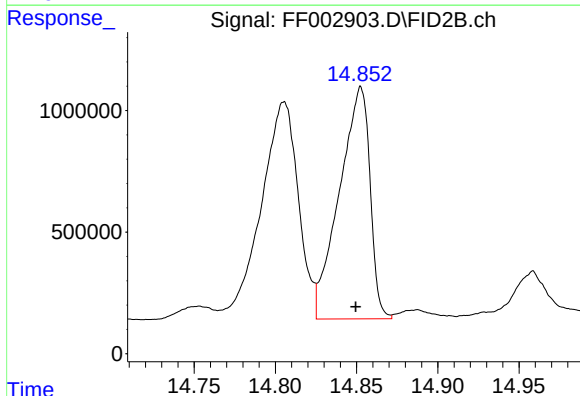


#10 N-TETRACOSANE

R.T.: 14.853 min
Delta R.T.: 0.003 min
Response: 12520164
Conc: 86.64 ug/ml

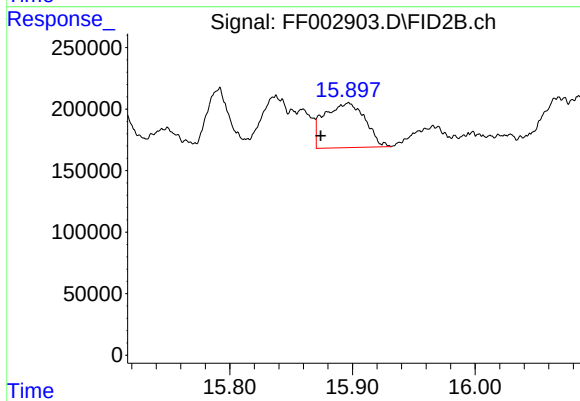

#11 N-HEXACOSANE


R.T.: 15.897 min
Delta R.T.: 0.023 min
Response: 837136
Conc: 6.00 ug/ml

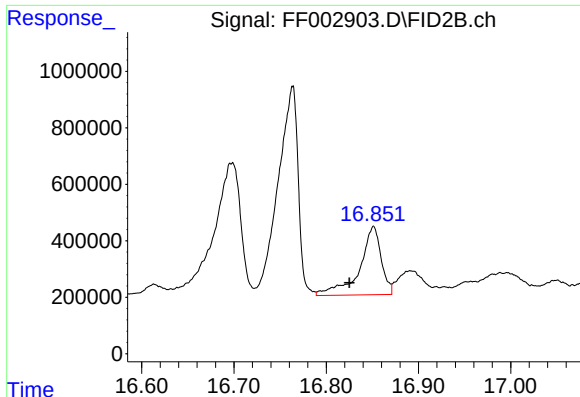

#12 N-OCTACOSANE


R.T.: 16.851 min
Delta R.T.: 0.026 min
Response: 3942203
Conc: 29.42 ug/ml

Instrument :
FID_F
ClientSampleId :

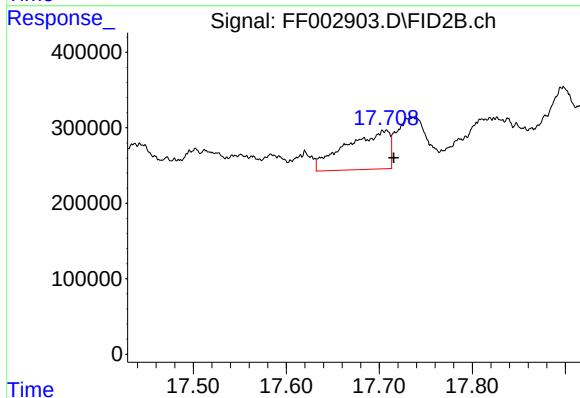


#13 N-TRIACONTANE

R.T.: 17.708 min
Delta R.T.: -0.007 min
Response: 1659557
Conc: 12.95 ug/ml

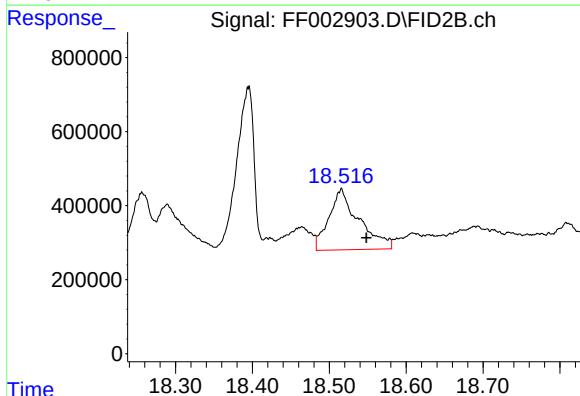


#14 N-DOTRIACONTANE

R.T.: 18.515 min
Delta R.T.: -0.033 min
Response: 4469266
Conc: 37.42 ug/ml

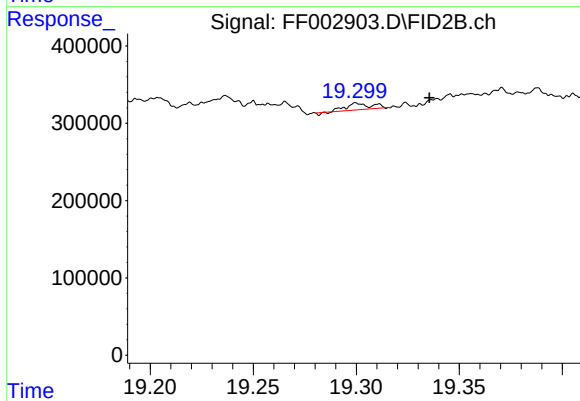

#15 N-TETRATRIACONTANE


R.T.: 19.301 min
Delta R.T.: -0.034 min
Response: 67388
Conc: 0.59 ug/ml

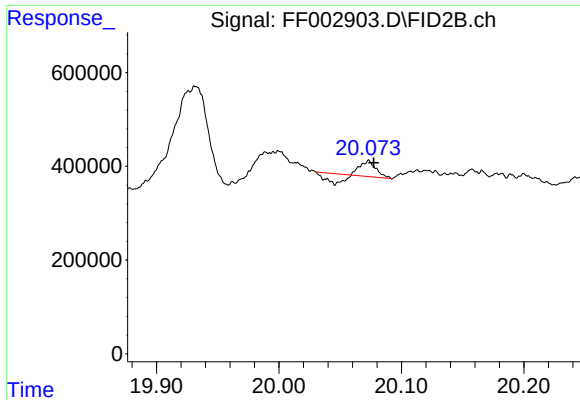

#16 N-HEXATRIACONTANE


R.T.: 20.073 min
Delta R.T.: -0.005 min
Response: 98913
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :

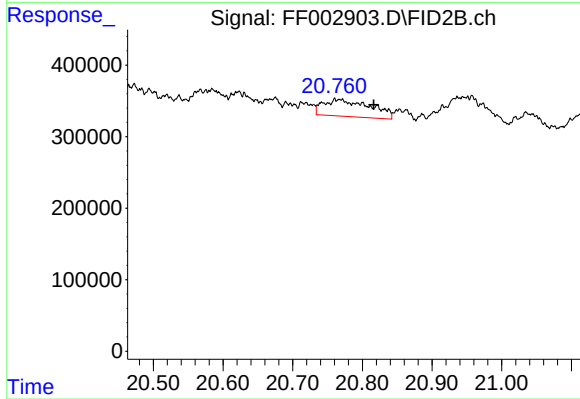

#17 N-OCTATRIACONTANE

R.T.: 20.768 min
Delta R.T.: -0.048 min
Response: 1109578
Conc: 10.93 ug/ml

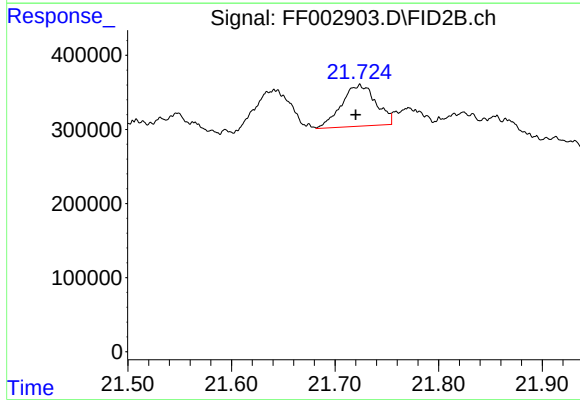

#18 N-TETRACONTANE

R.T.: 21.724 min
Delta R.T.: 0.004 min
Response: 1290366
Conc: 12.28 ug/ml