

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002904.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 15:49
 Operator : AJ\SJ
 Sample : J6210-09
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:05:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	1867201	14.382 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	1467756	9.157 ug/ml
12) N-OCTACOSANE	16.876f	100859	0.753 ug/ml
13) N-TRIACONTANE	17.721	315936	2.466 ug/ml
14) N-DOTRIACONTANE	18.547	301149	2.522 ug/ml
15) N-TETRATRIACONTANE	19.342	102329	0.903 ug/ml
16) N-HEXATRIACONTANE	20.069	35536	0.329 ug/ml
18) N-TETRACONTANE	21.724	52015	0.495 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002904.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 15:49
Operator : AJ\SJ
Sample : J6210-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:05:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

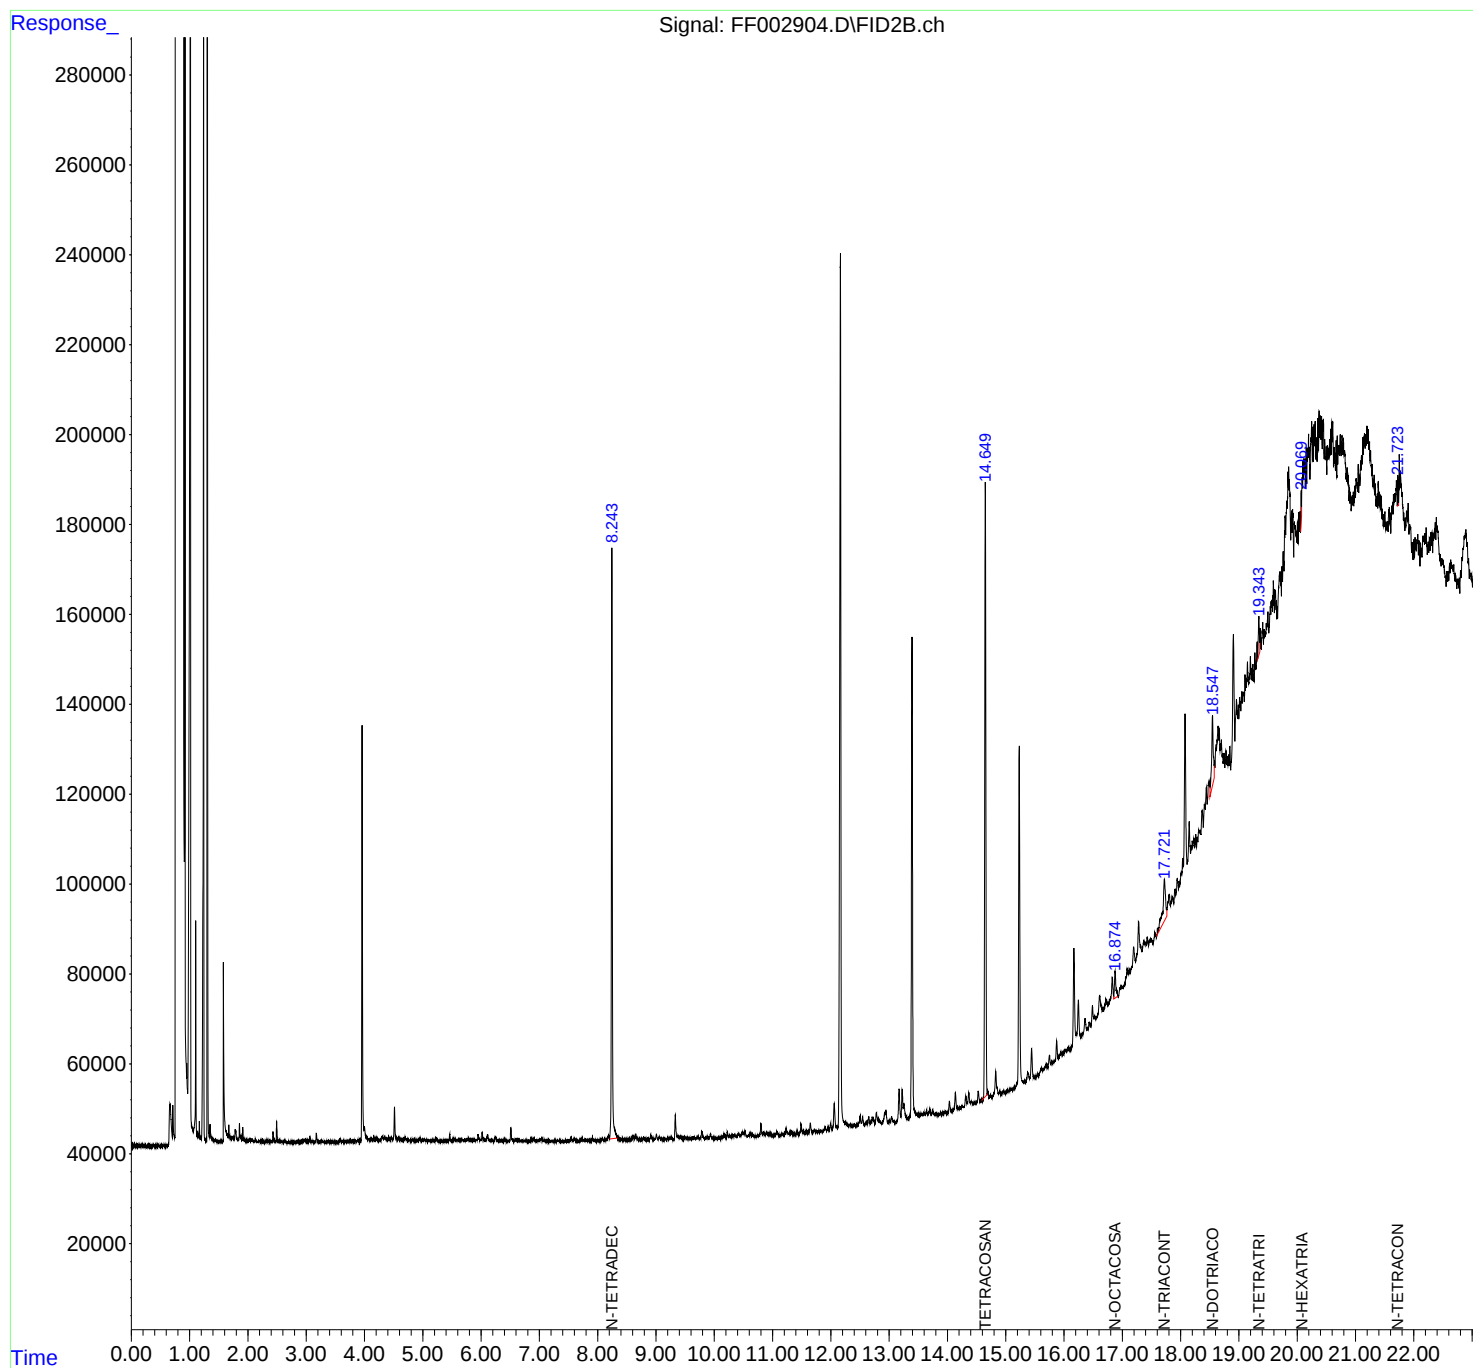


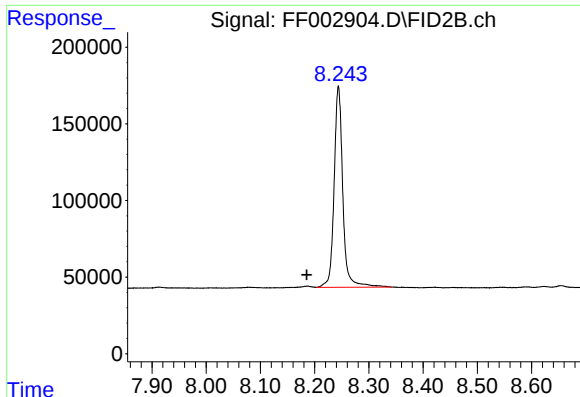

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.058 min
Response: 1467756
Conc: 9.16 ug/ml

Instrument :
FID_F
ClientSampleId :

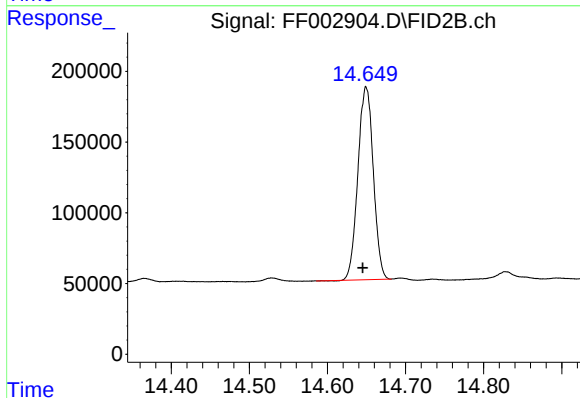


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.004 min
Response: 1867201
Conc: 14.38 ug/ml

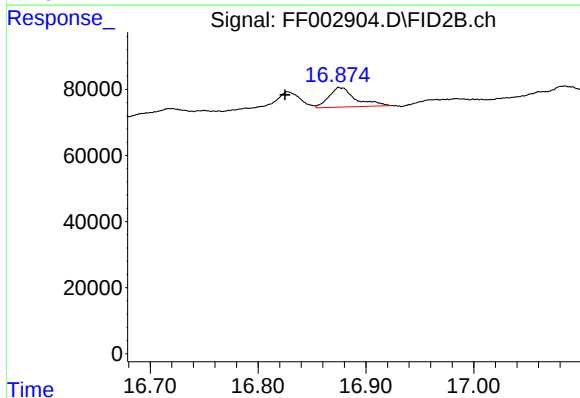


#12 N-OCTACOSANE

R.T.: 16.876 min
Delta R.T.: 0.050 min
Response: 100859
Conc: 0.75 ug/ml

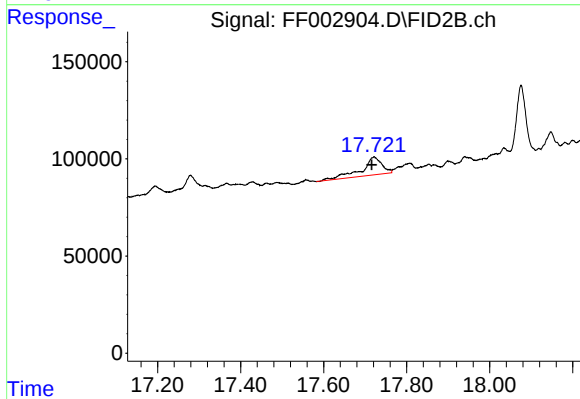

#13 N-TRIACONTANE


R.T.: 17.721 min
Delta R.T.: 0.006 min
Response: 315936
Conc: 2.47 ug/ml

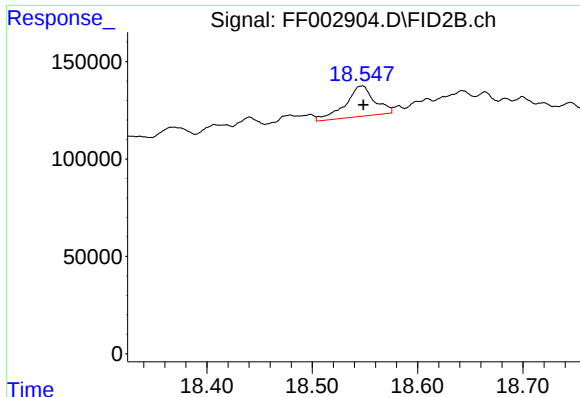

#14 N-DOTRIACONTANE


R.T.: 18.547 min
Delta R.T.: -0.001 min
Response: 301149
Conc: 2.52 ug/ml

Instrument :
FID_F
ClientSampleId :

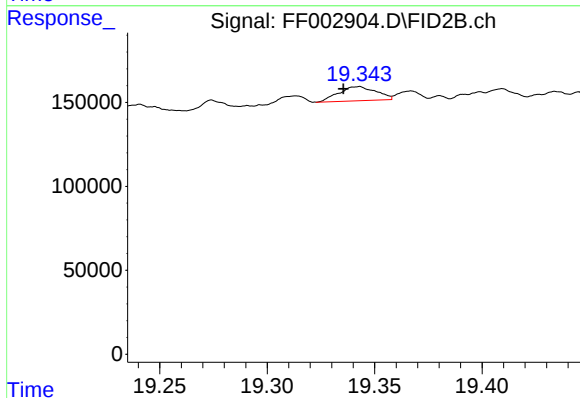


#15 N-TETRATRIACONTANE

R.T.: 19.342 min
Delta R.T.: 0.007 min
Response: 102329
Conc: 0.90 ug/ml

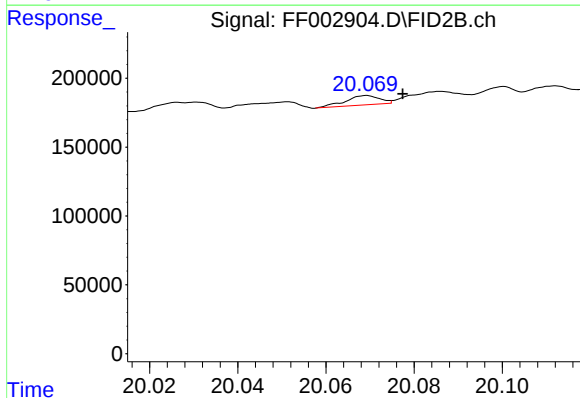

#16 N-HEXATRIACONTANE

R.T.: 20.069 min
Delta R.T.: -0.008 min
Response: 35536
Conc: 0.33 ug/ml

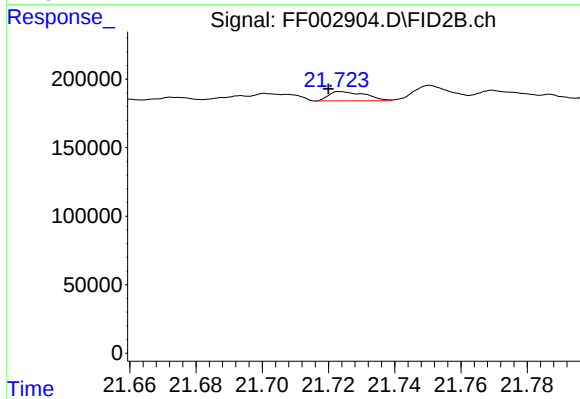

#18 N-TETRACONTANE

R.T.: 21.724 min
Delta R.T.: 0.004 min
Response: 52015
Conc: 0.49 ug/ml