

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002905.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 16:19
 Operator : AJ\SJ
 Sample : J6208-13
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:05:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	2129598	16.404 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	359721	2.244 ug/ml
5) N-HEXADECANE	9.793	141349	0.883 ug/ml
7) N-EICOSANE	12.547	211343	1.370 ug/ml
8) N-DOCOSANE	13.765	499090	3.338 ug/ml
10) N-TETRACOSANE	14.824	2156766	14.924 ug/ml
11) N-HEXACOSANE	15.878	268867	1.926 ug/ml
12) N-OCTACOSANE	16.827	524126	3.912 ug/ml
13) N-TRIACONTANE	17.722	378956	2.957 ug/ml
14) N-DOTRIACONTANE	18.547	170588	1.428 ug/ml
15) N-TETRATRIACONTANE	19.373	45612	0.402 ug/ml
18) N-TETRACONTANE	21.749	561556	5.343 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002905.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 16:19
Operator : AJ\SJ
Sample : J6208-13
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:05:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

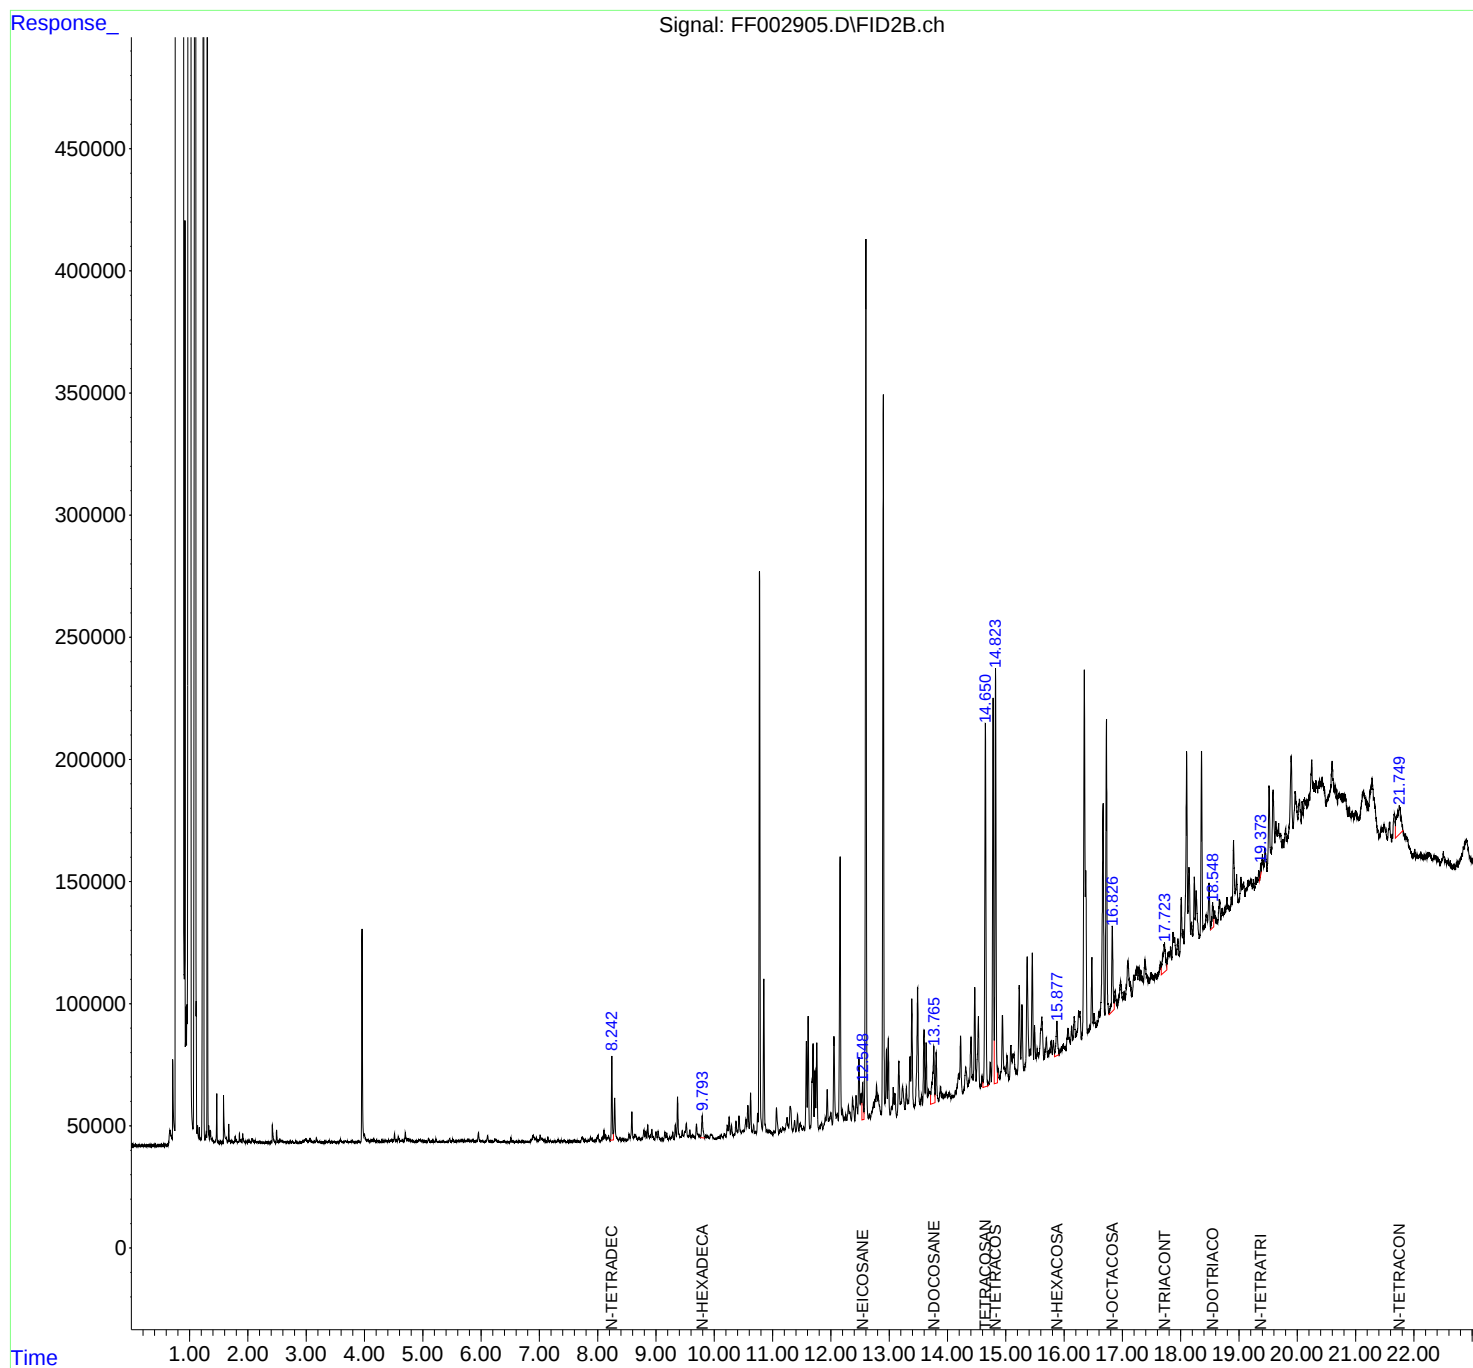


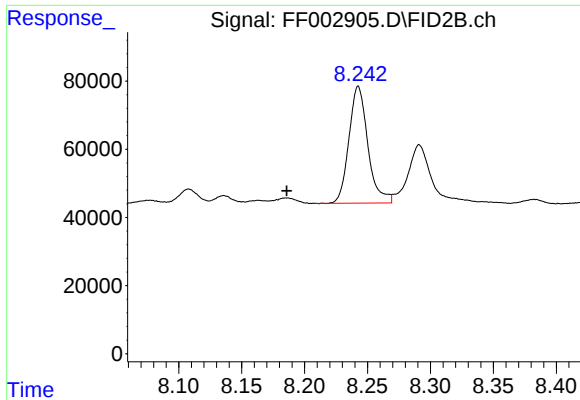

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: 0.057 min
Response: 359721
Conc: 2.24 ug/ml

Instrument :
FID_F
ClientSampleId :

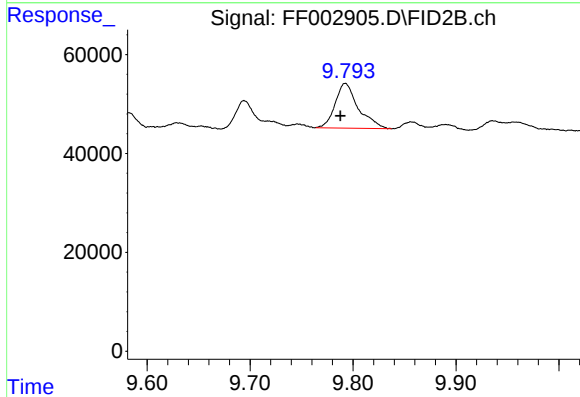


#5 N-HEXADECANE

R.T.: 9.793 min
Delta R.T.: 0.005 min
Response: 141349
Conc: 0.88 ug/ml

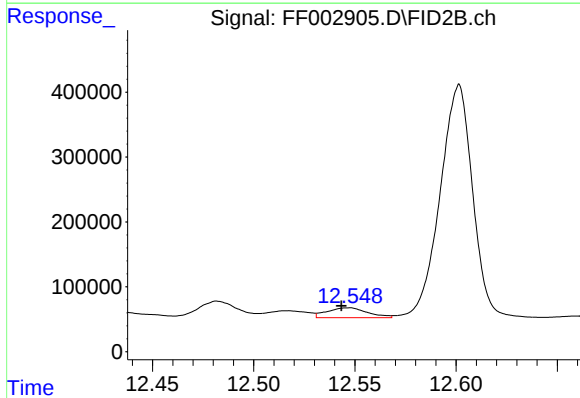


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: 0.004 min
Response: 211343
Conc: 1.37 ug/ml

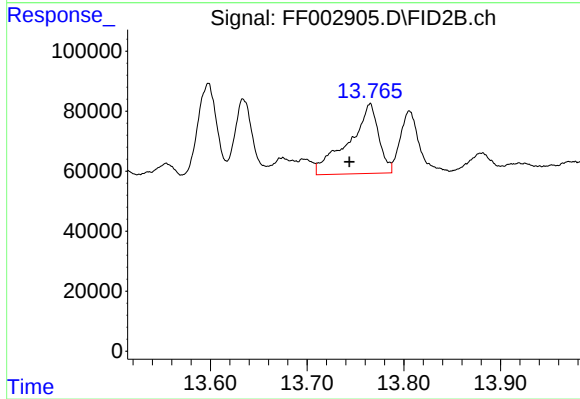

#8 N-DOCOSANE


R.T.: 13.765 min
Delta R.T.: 0.021 min
Response: 499090
Conc: 3.34 ug/ml

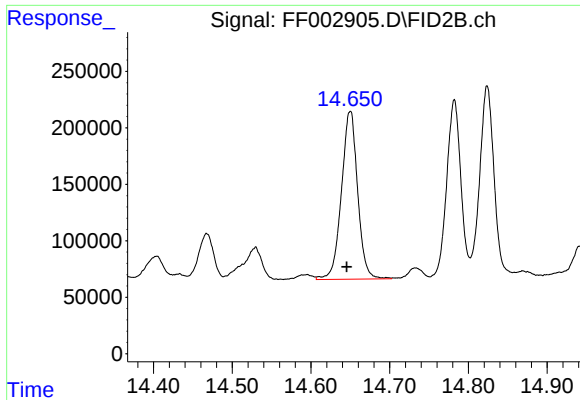

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.650 min
Delta R.T.: 0.005 min
Response: 2129598
Conc: 16.40 ug/ml

Instrument :
FID_F
ClientSampleId :

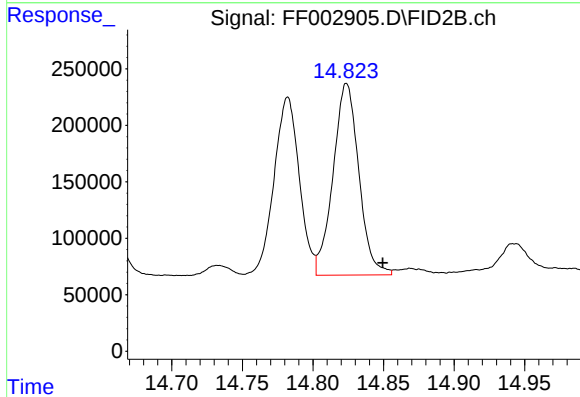


#10 N-TETRACOSANE

R.T.: 14.824 min
Delta R.T.: -0.026 min
Response: 2156766
Conc: 14.92 ug/ml

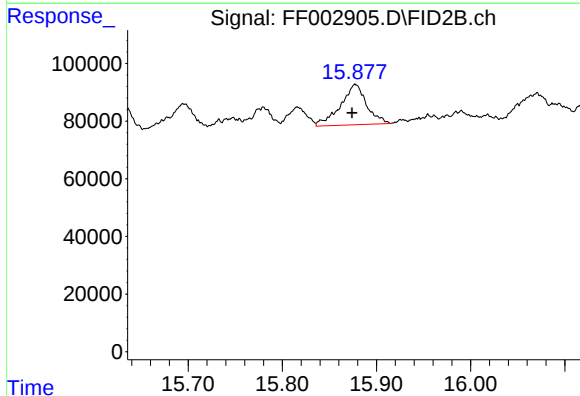


#11 N-HEXACOSANE

R.T.: 15.878 min
Delta R.T.: 0.004 min
Response: 268867
Conc: 1.93 ug/ml

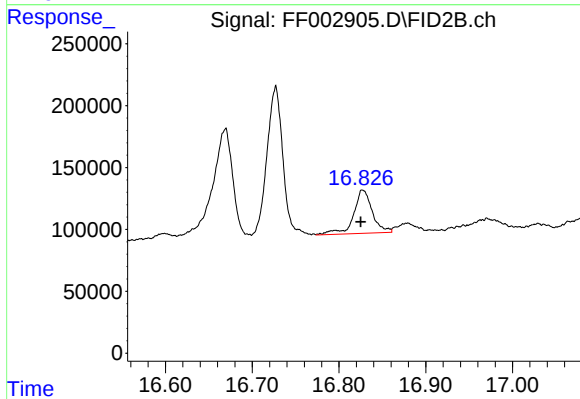

#12 N-OCTACOSANE


R.T.: 16.827 min
Delta R.T.: 0.002 min
Response: 524126
Conc: 3.91 ug/ml

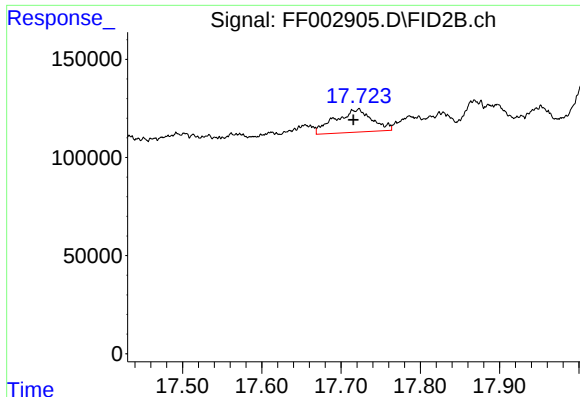

#13 N-TRIACONTANE


R.T.: 17.722 min
Delta R.T.: 0.007 min
Response: 378956
Conc: 2.96 ug/ml

Instrument :
FID_F
ClientSampleId :

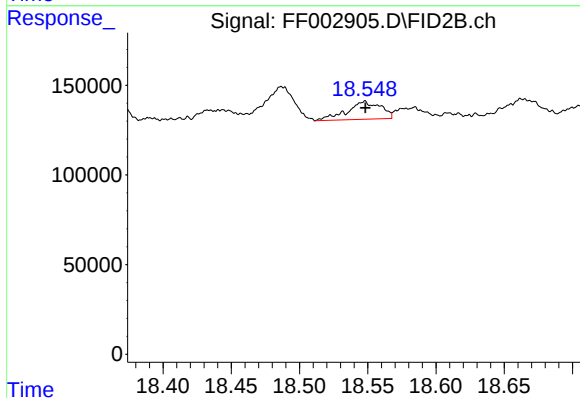


#14 N-DOTRIACONTANE

R.T.: 18.547 min
Delta R.T.: -0.001 min
Response: 170588
Conc: 1.43 ug/ml

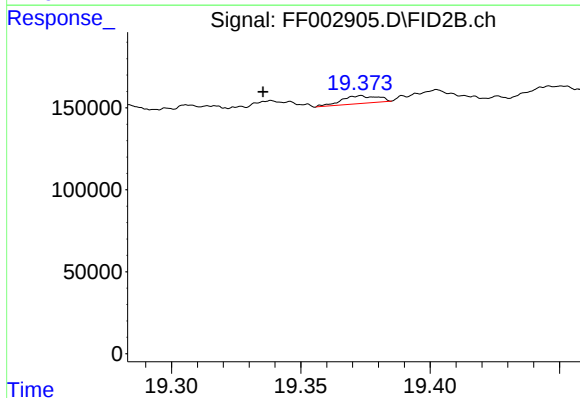

#15 N-TETRATRIACONTANE

R.T.: 19.373 min
Delta R.T.: 0.037 min
Response: 45612
Conc: 0.40 ug/ml

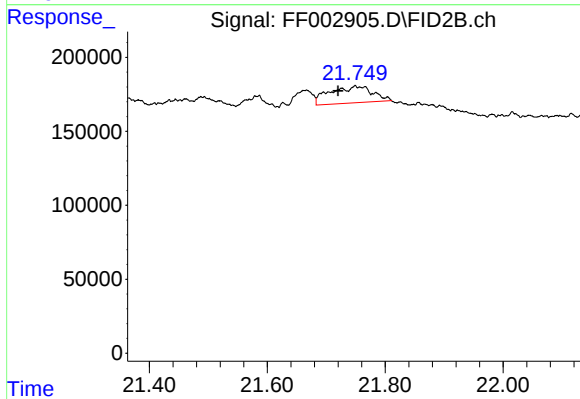

#18 N-TETRACONTANE

R.T.: 21.749 min
Delta R.T.: 0.029 min
Response: 561556
Conc: 5.34 ug/ml