

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002906.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 16:50
 Operator : AJ\SJ
 Sample : J6208-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:06:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.653	2922570	22.512 ug/ml
Target Compounds			
2) N-DECANE	4.409	54596	0.348 ug/ml
4) N-TETRADECANE	8.243f	598197	3.732 ug/ml
5) N-HEXADECANE	9.790	203774	1.272 ug/ml
6) N-OCTADECANE	11.250	225622	1.424 ug/ml
7) N-EICOSANE	12.547	181607	1.178 ug/ml
8) N-DOCOSANE	13.767	569617	3.809 ug/ml
10) N-TETRACOSANE	14.828	2640114	18.269 ug/ml
11) N-HEXACOSANE	15.886	1383441	9.912 ug/ml
12) N-OCTACOSANE	16.836	3438206	25.661 ug/ml
13) N-TRIACONTANE	17.727	3693404	28.825 ug/ml
14) N-DOTRIACONTANE	18.554	1234598	10.338 ug/ml
16) N-HEXATRIACONTANE	20.051	101955	0.945 ug/ml
18) N-TETRACONTANE	21.729	245645	2.337 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002906.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 16:50
Operator : AJ\SJ
Sample : J6208-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:06:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

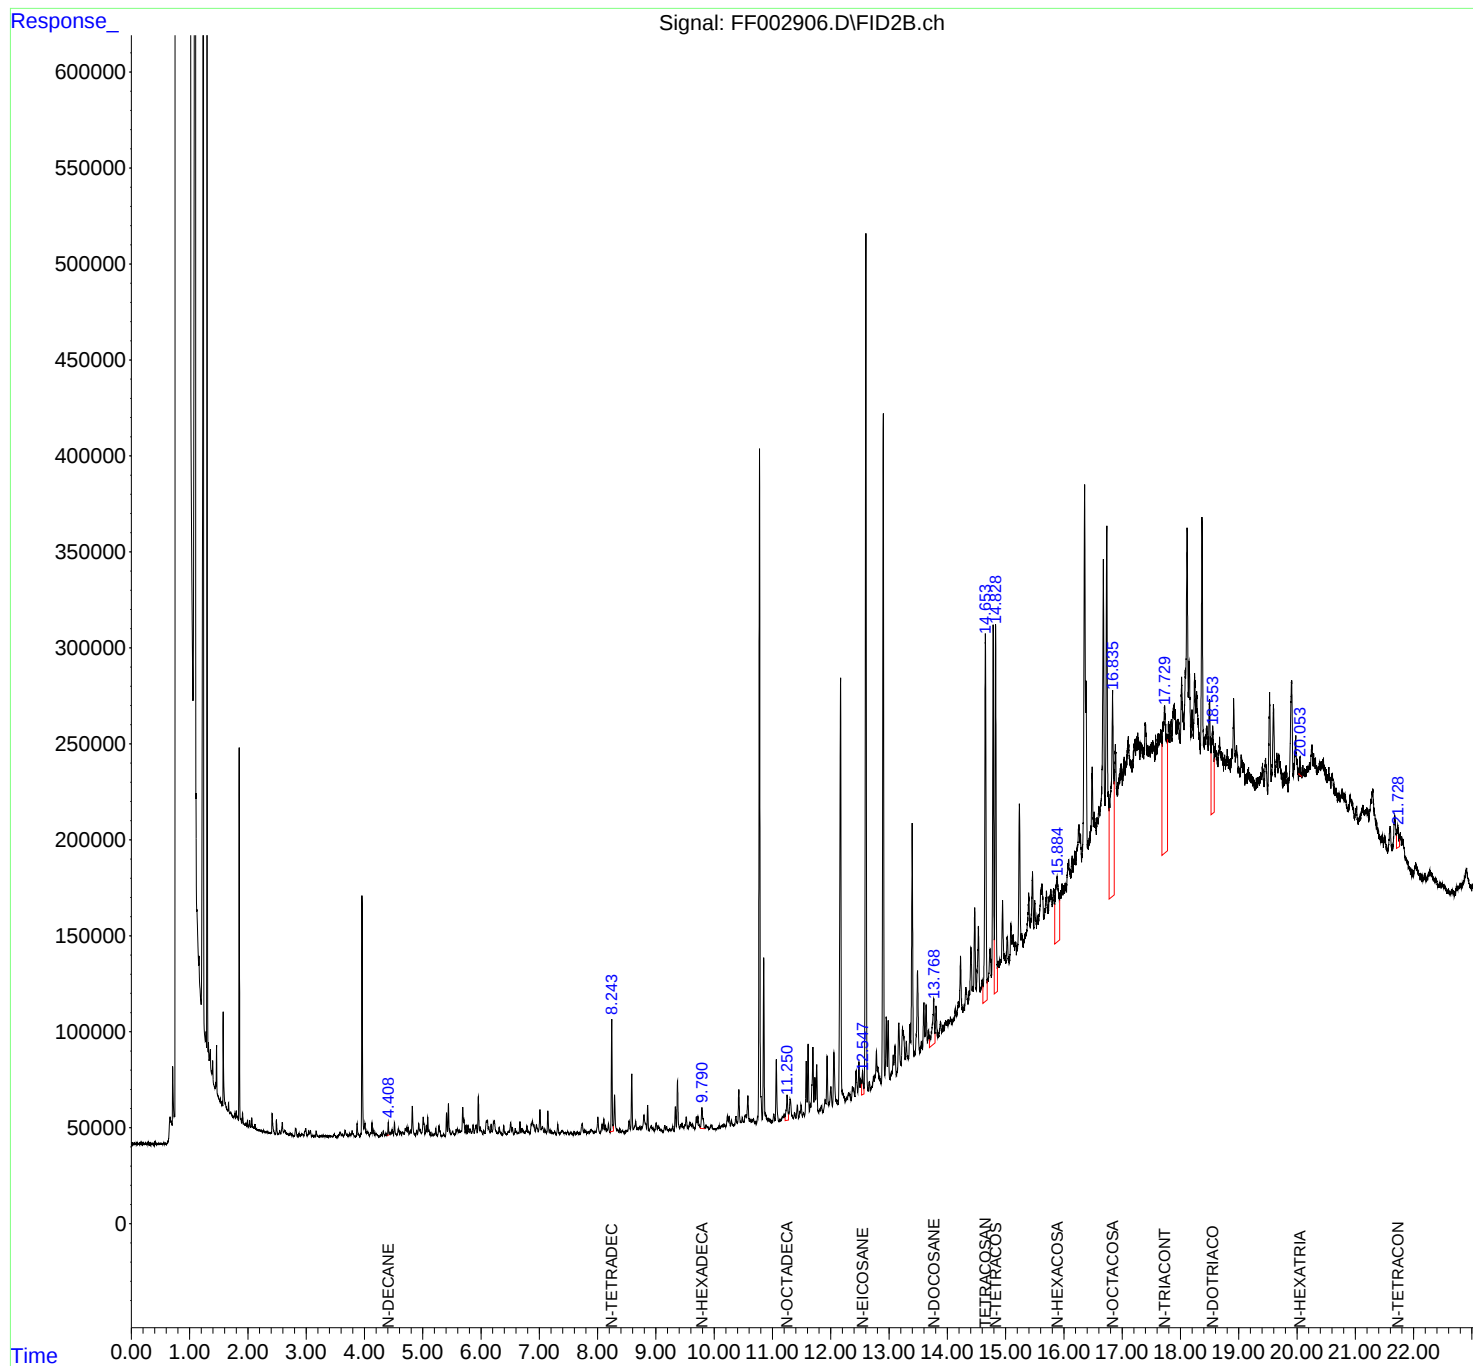


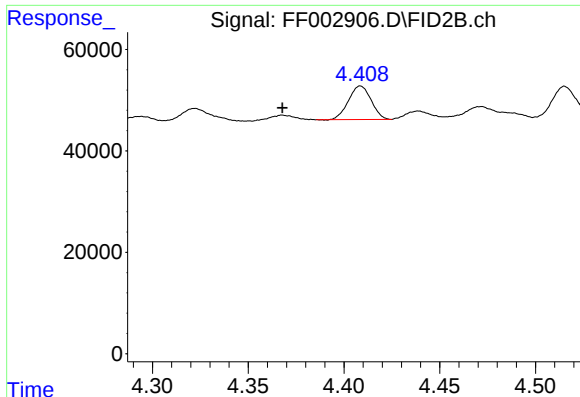

#2 N-DECANE


R.T.: 4.409 min
Delta R.T.: 0.041 min
Response: 54596
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

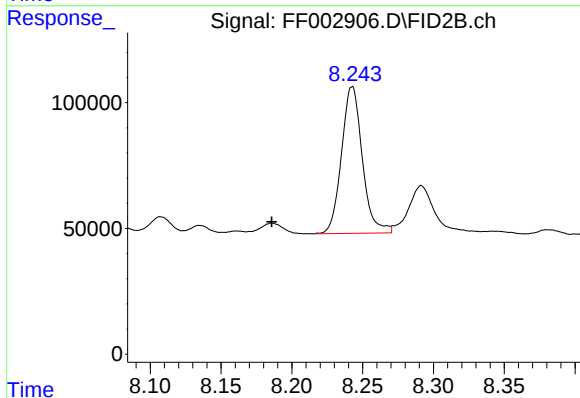


#4 N-TETRADECANE

R.T.: 8.243 min
Delta R.T.: 0.057 min
Response: 598197
Conc: 3.73 ug/ml

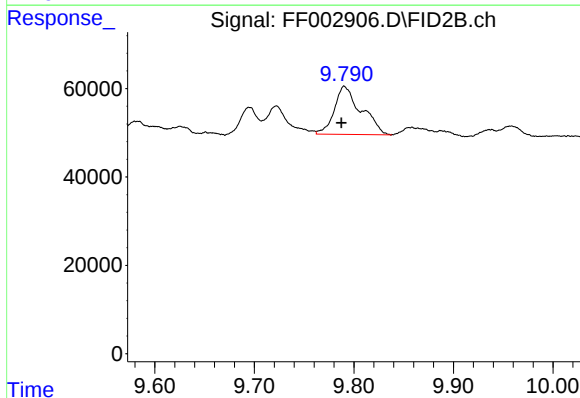


#5 N-HEXADECANE

R.T.: 9.790 min
Delta R.T.: 0.003 min
Response: 203774
Conc: 1.27 ug/ml

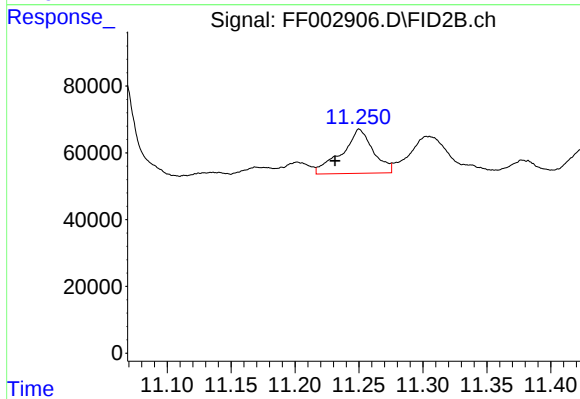

#6 N-OCTADECANE


R.T.: 11.250 min
Delta R.T.: 0.019 min
Response: 225622
Conc: 1.42 ug/ml

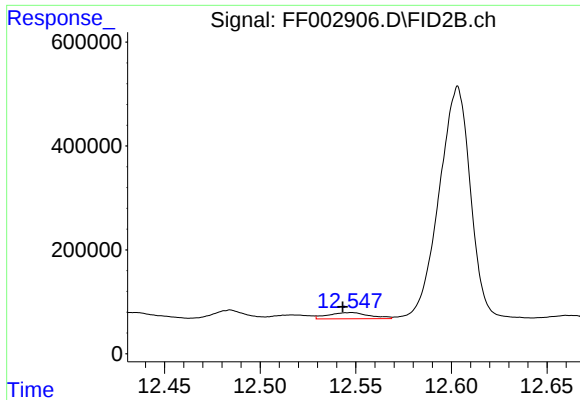

#7 N-EICOSANE


R.T.: 12.547 min
Delta R.T.: 0.004 min
Response: 181607
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :

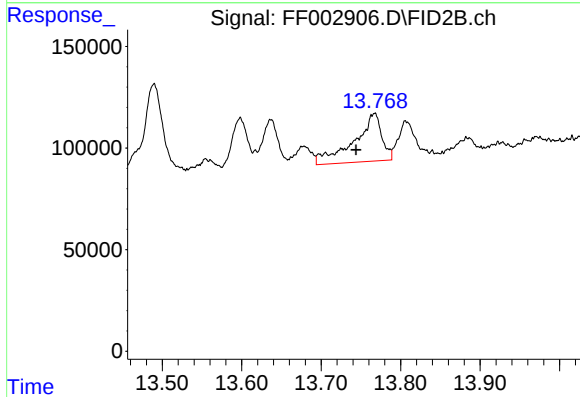


#8 N-DOCOSANE

R.T.: 13.767 min
Delta R.T.: 0.023 min
Response: 569617
Conc: 3.81 ug/ml

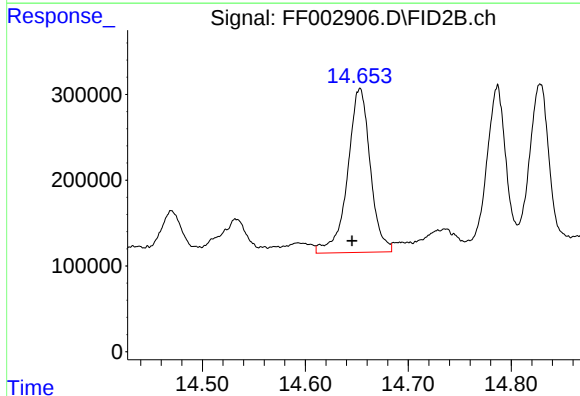


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.653 min
Delta R.T.: 0.008 min
Response: 2922570
Conc: 22.51 ug/ml

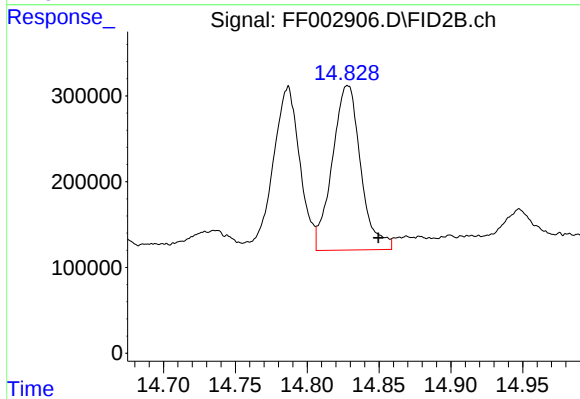

#10 N-TETRACOSANE


R.T.: 14.828 min
Delta R.T.: -0.022 min
Response: 2640114
Conc: 18.27 ug/ml

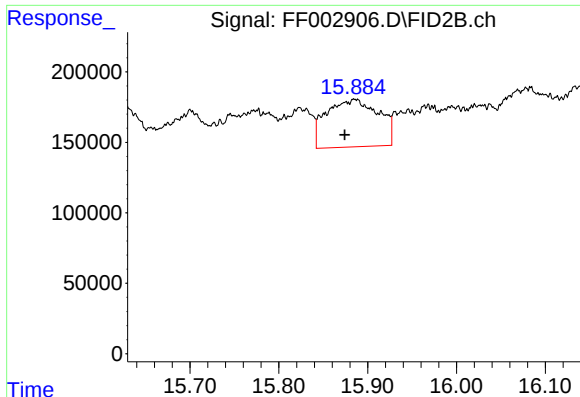

#11 N-HEXACOSANE


R.T.: 15.886 min
Delta R.T.: 0.012 min
Response: 1383441
Conc: 9.91 ug/ml

Instrument :
FID_F
ClientSampleId :

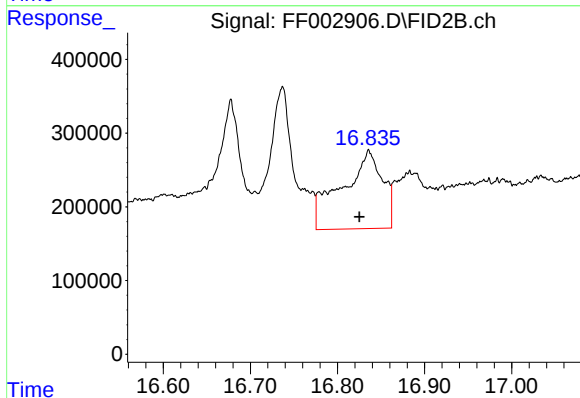


#12 N-OCTACOSANE

R.T.: 16.836 min
Delta R.T.: 0.011 min
Response: 3438206
Conc: 25.66 ug/ml

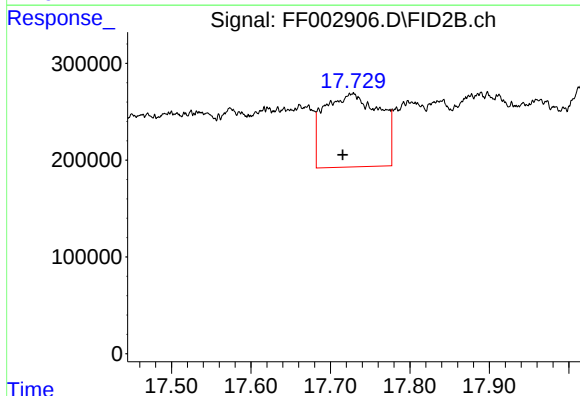


#13 N-TRIACONTANE

R.T.: 17.727 min
Delta R.T.: 0.012 min
Response: 3693404
Conc: 28.82 ug/ml

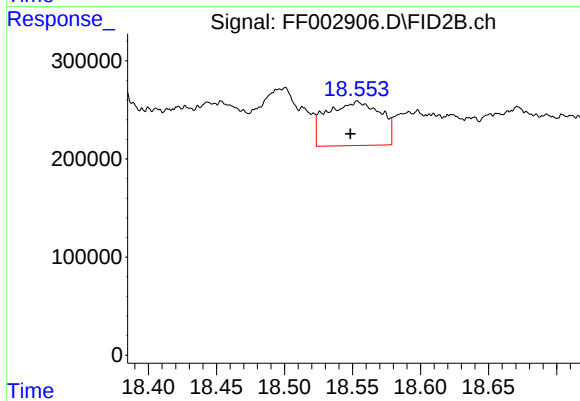

#14 N-DOTRIACONTANE


R.T.: 18.554 min
Delta R.T.: 0.005 min
Response: 1234598
Conc: 10.34 ug/ml

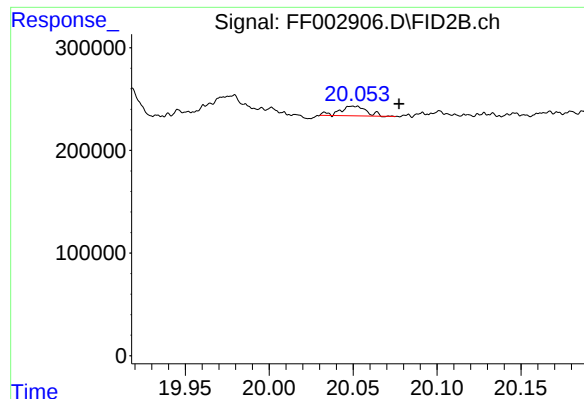

#16 N-HEXATRIACONTANE

R.T.: 20.051 min
Delta R.T.: -0.027 min
Response: 101955
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

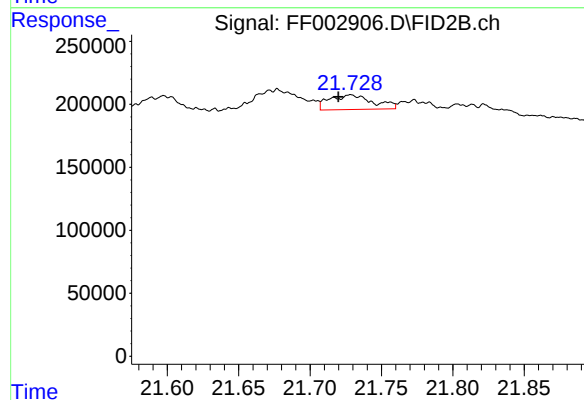

#18 N-TETRACONTANE

R.T.: 21.729 min
Delta R.T.: 0.009 min
Response: 245645
Conc: 2.34 ug/ml