

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002907.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 17:20
 Operator : AJ\SJ
 Sample : J6208-09
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:06:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	2564400	19.753 ug/ml
Target Compounds			
4) N-TETRADECANE	8.136	127108	0.793 ug/ml
5) N-HEXADECANE	9.794	317599	1.983 ug/ml
6) N-OCTADECANE	11.171f	129024	0.814 ug/ml
7) N-EICOSANE	12.550	522964	3.391 ug/ml
8) N-DOCOSANE	13.768	1257828	8.412 ug/ml
10) N-TETRACOSANE	14.831	3557145	24.614 ug/ml
11) N-HEXACOSANE	15.887	331134	2.372 ug/ml
12) N-OCTACOSANE	16.833	1023516	7.639 ug/ml
13) N-TRIACONTANE	17.719	948855	7.405 ug/ml
14) N-DOTRIACONTANE	18.557	435895	3.650 ug/ml
15) N-TETRATRIACONTANE	19.380	55861	0.493 ug/ml
16) N-HEXATRIACONTANE	20.092	66458	0.616 ug/ml
18) N-TETRACONTANE	21.725	106589	1.014 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002907.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 17:20
Operator : AJ\SJ
Sample : J6208-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:06:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

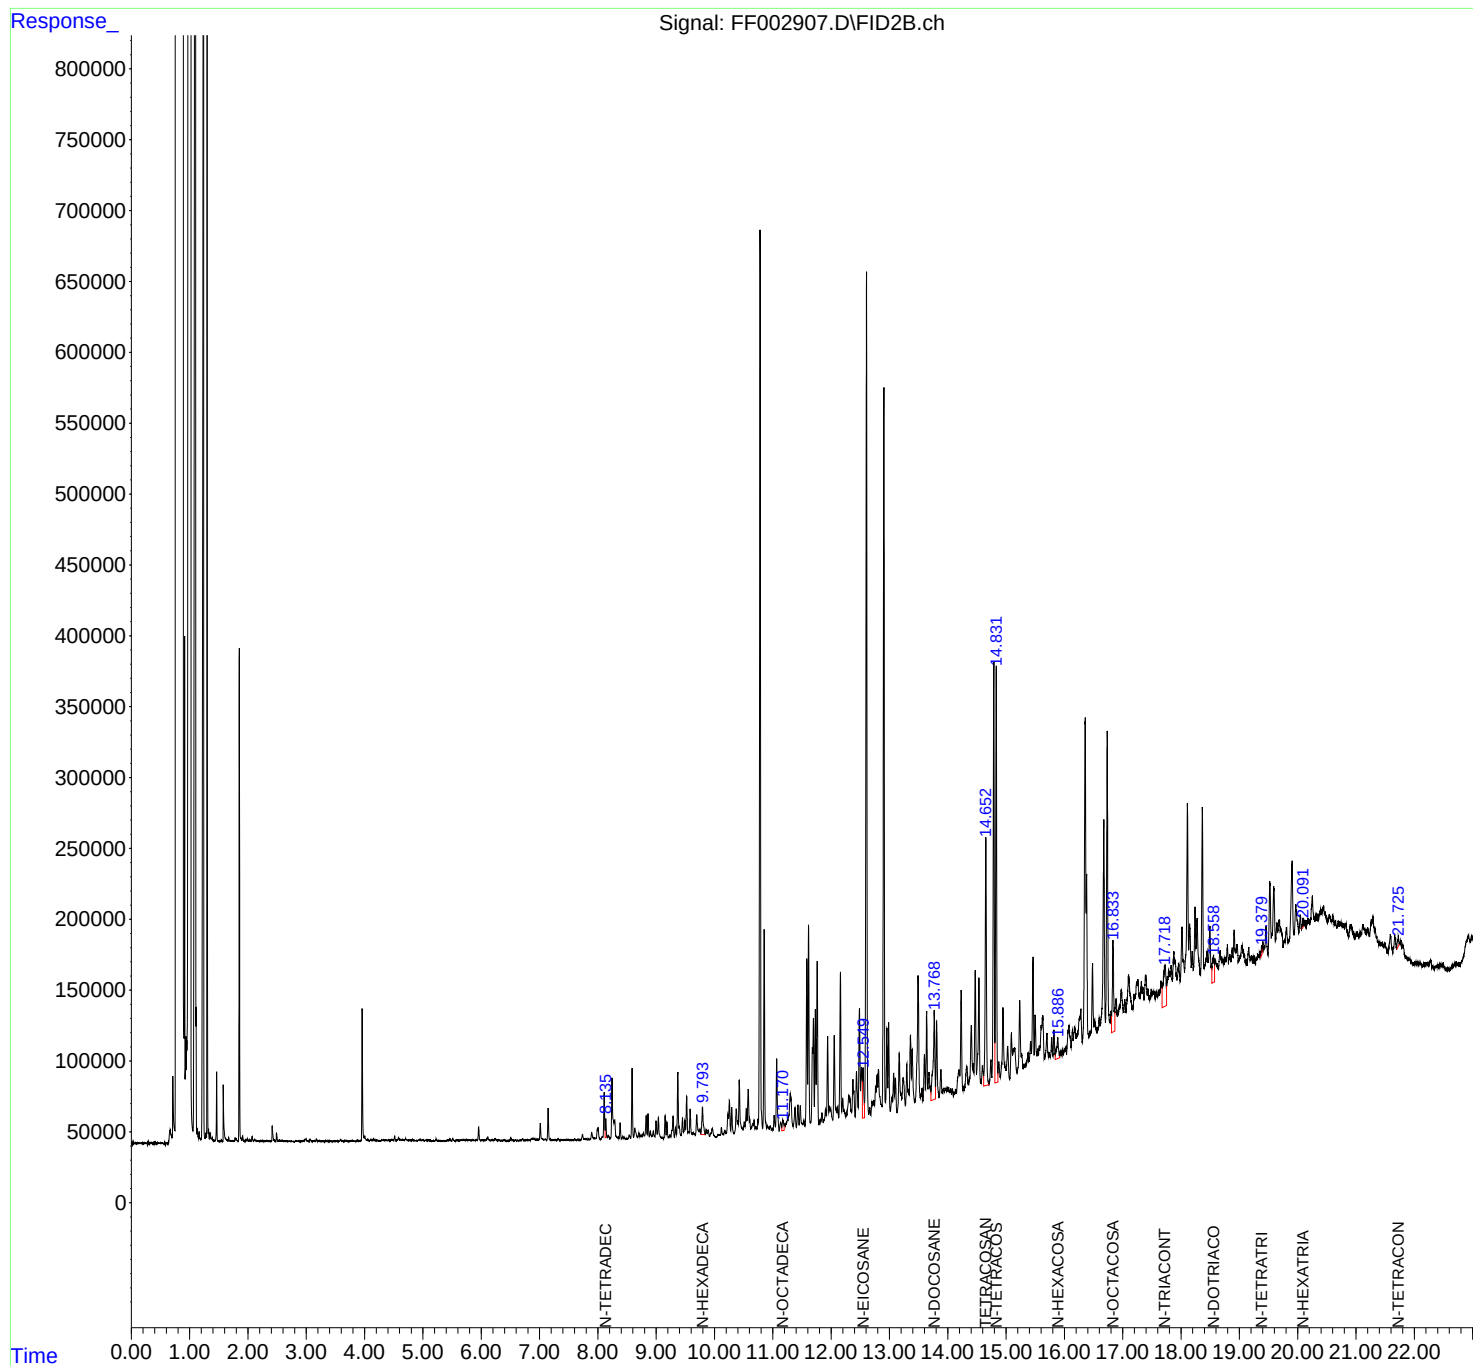


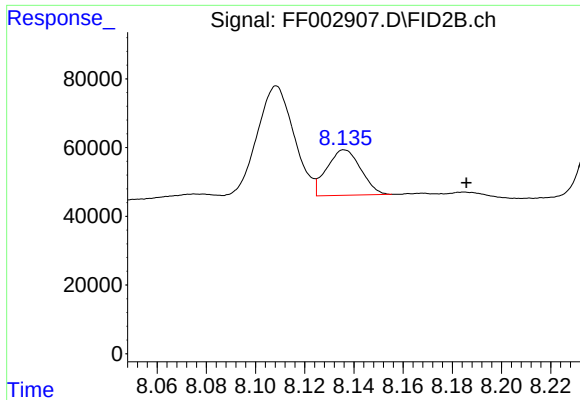

#4 N-TETRADECANE


R.T.: 8.136 min
Delta R.T.: -0.049 min
Response: 127108
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :

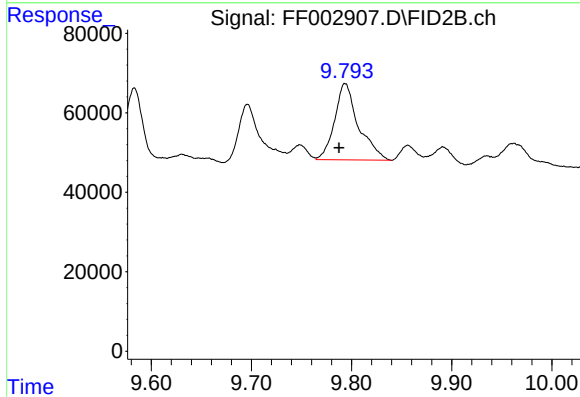


#5 N-HEXADECANE

R.T.: 9.794 min
Delta R.T.: 0.006 min
Response: 317599
Conc: 1.98 ug/ml

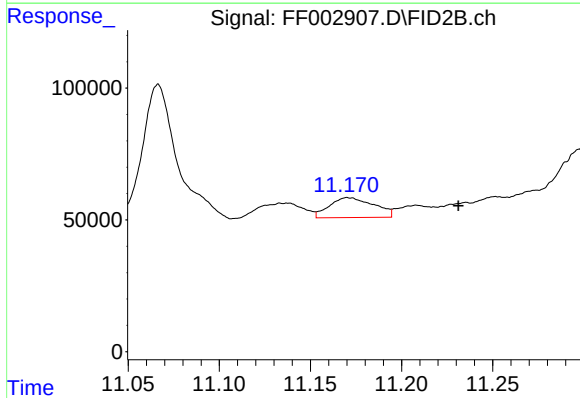


#6 N-OCTADECANE

R.T.: 11.171 min
Delta R.T.: -0.061 min
Response: 129024
Conc: 0.81 ug/ml

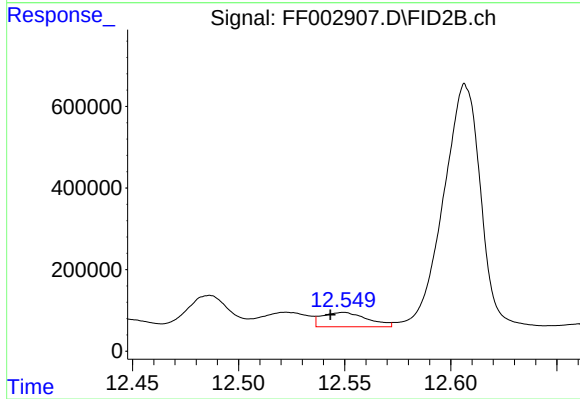

#7 N-EICOSANE


R.T.: 12.550 min
Delta R.T.: 0.006 min
Response: 522964
Conc: 3.39 ug/ml

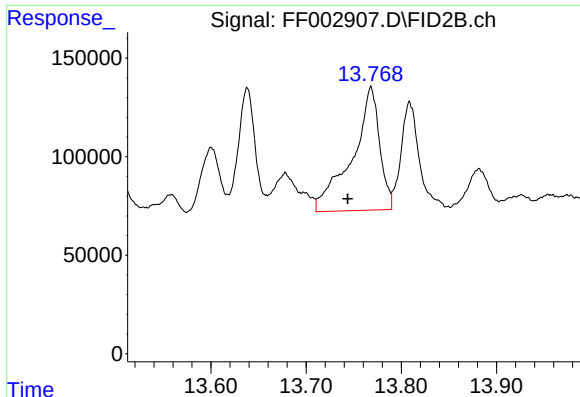

#8 N-DOCOSANE


R.T.: 13.768 min
Delta R.T.: 0.024 min
Response: 1257828
Conc: 8.41 ug/ml

Instrument :
FID_F
ClientSampleId :

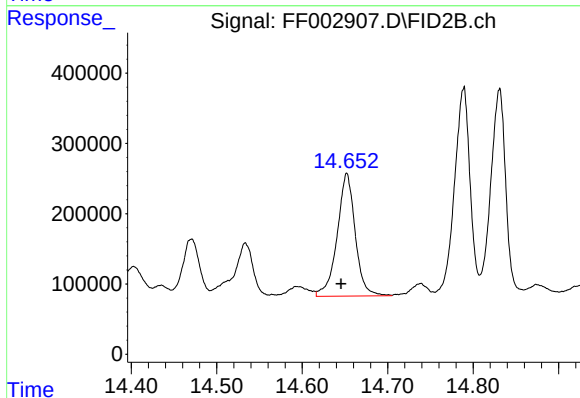


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.652 min
Delta R.T.: 0.007 min
Response: 2564400
Conc: 19.75 ug/ml

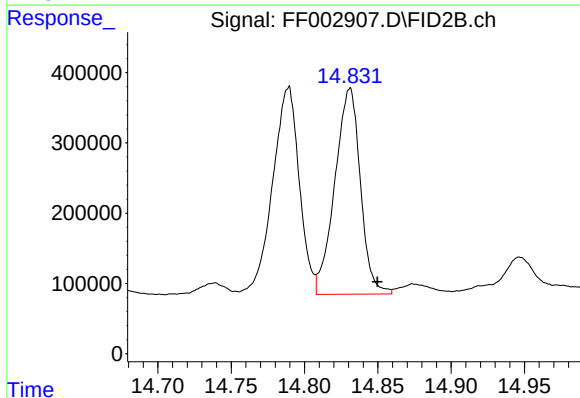


#10 N-TETRACOSANE

R.T.: 14.831 min
Delta R.T.: -0.019 min
Response: 3557145
Conc: 24.61 ug/ml

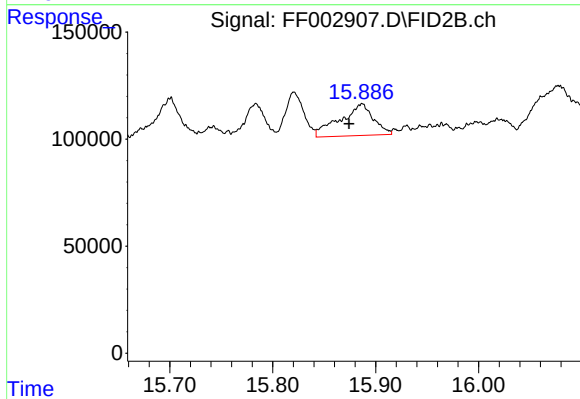

#11 N-HEXACOSANE


R.T.: 15.887 min
Delta R.T.: 0.013 min
Response: 331134
Conc: 2.37 ug/ml

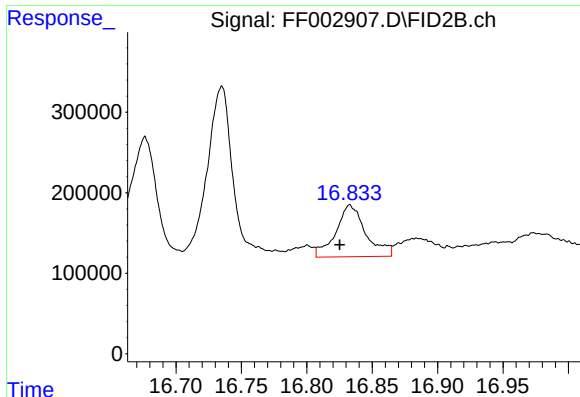

#12 N-OCTACOSANE


R.T.: 16.833 min
Delta R.T.: 0.008 min
Response: 1023516
Conc: 7.64 ug/ml

Instrument :
FID_F
ClientSampleId :

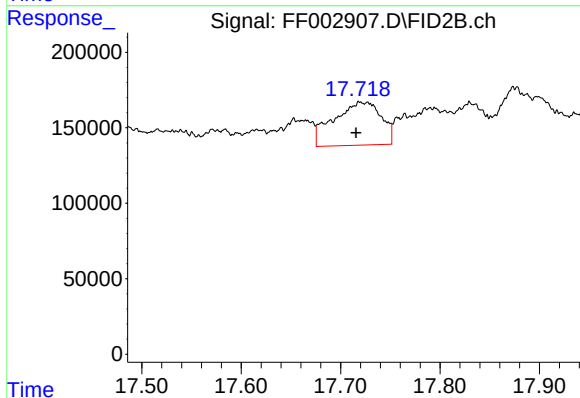


#13 N-TRIACONTANE

R.T.: 17.719 min
Delta R.T.: 0.004 min
Response: 948855
Conc: 7.41 ug/ml

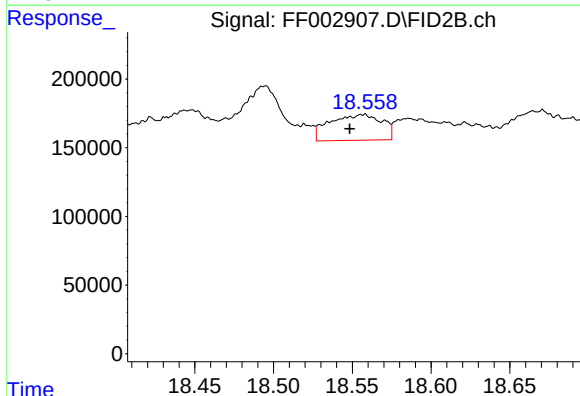


#14 N-DOTRIACONTANE

R.T.: 18.557 min
Delta R.T.: 0.008 min
Response: 435895
Conc: 3.65 ug/ml

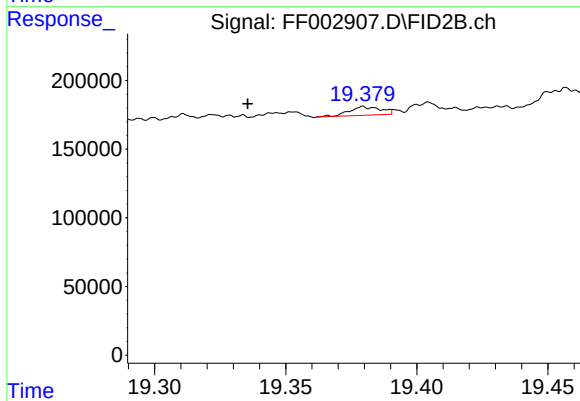

#15 N-TETRATRIACONTANE


R.T.: 19.380 min
Delta R.T.: 0.044 min
Response: 55861
Conc: 0.49 ug/ml

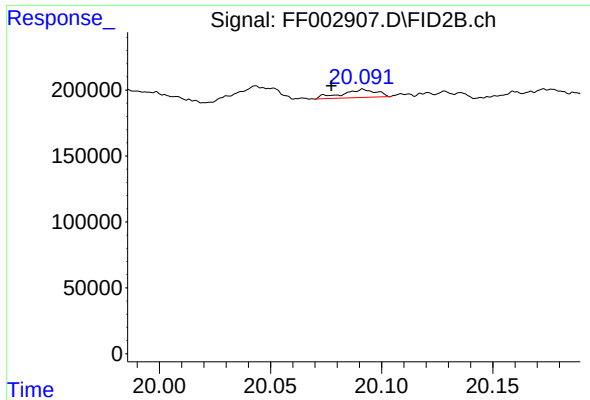

#16 N-HEXATRIACONTANE

R.T.: 20.092 min
Delta R.T.: 0.015 min
Response: 66458
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

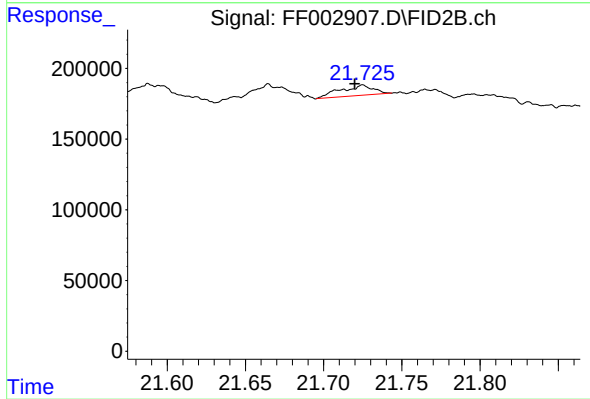

#18 N-TETRACONTANE

R.T.: 21.725 min
Delta R.T.: 0.005 min
Response: 106589
Conc: 1.01 ug/ml