

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002908.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 17:51
 Operator : AJ\SJ
 Sample : J6208-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:06:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	1763276	13.582 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	385266	2.404 ug/ml
7) N-EICOSANE	12.598f	1182293	7.666 ug/ml
10) N-TETRACOSANE	14.820	691665	4.786 ug/ml
12) N-OCTACOSANE	16.825	228583	1.706 ug/ml
13) N-TRIACONTANE	17.720	207042	1.616 ug/ml
14) N-DOTRIACONTANE	18.549	400266	3.352 ug/ml
16) N-HEXATRIACONTANE	20.084	33396	0.310 ug/ml
18) N-TETRACONTANE	21.766	969358	9.223 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002908.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 17:51
Operator : AJ\SJ
Sample : J6208-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:06:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

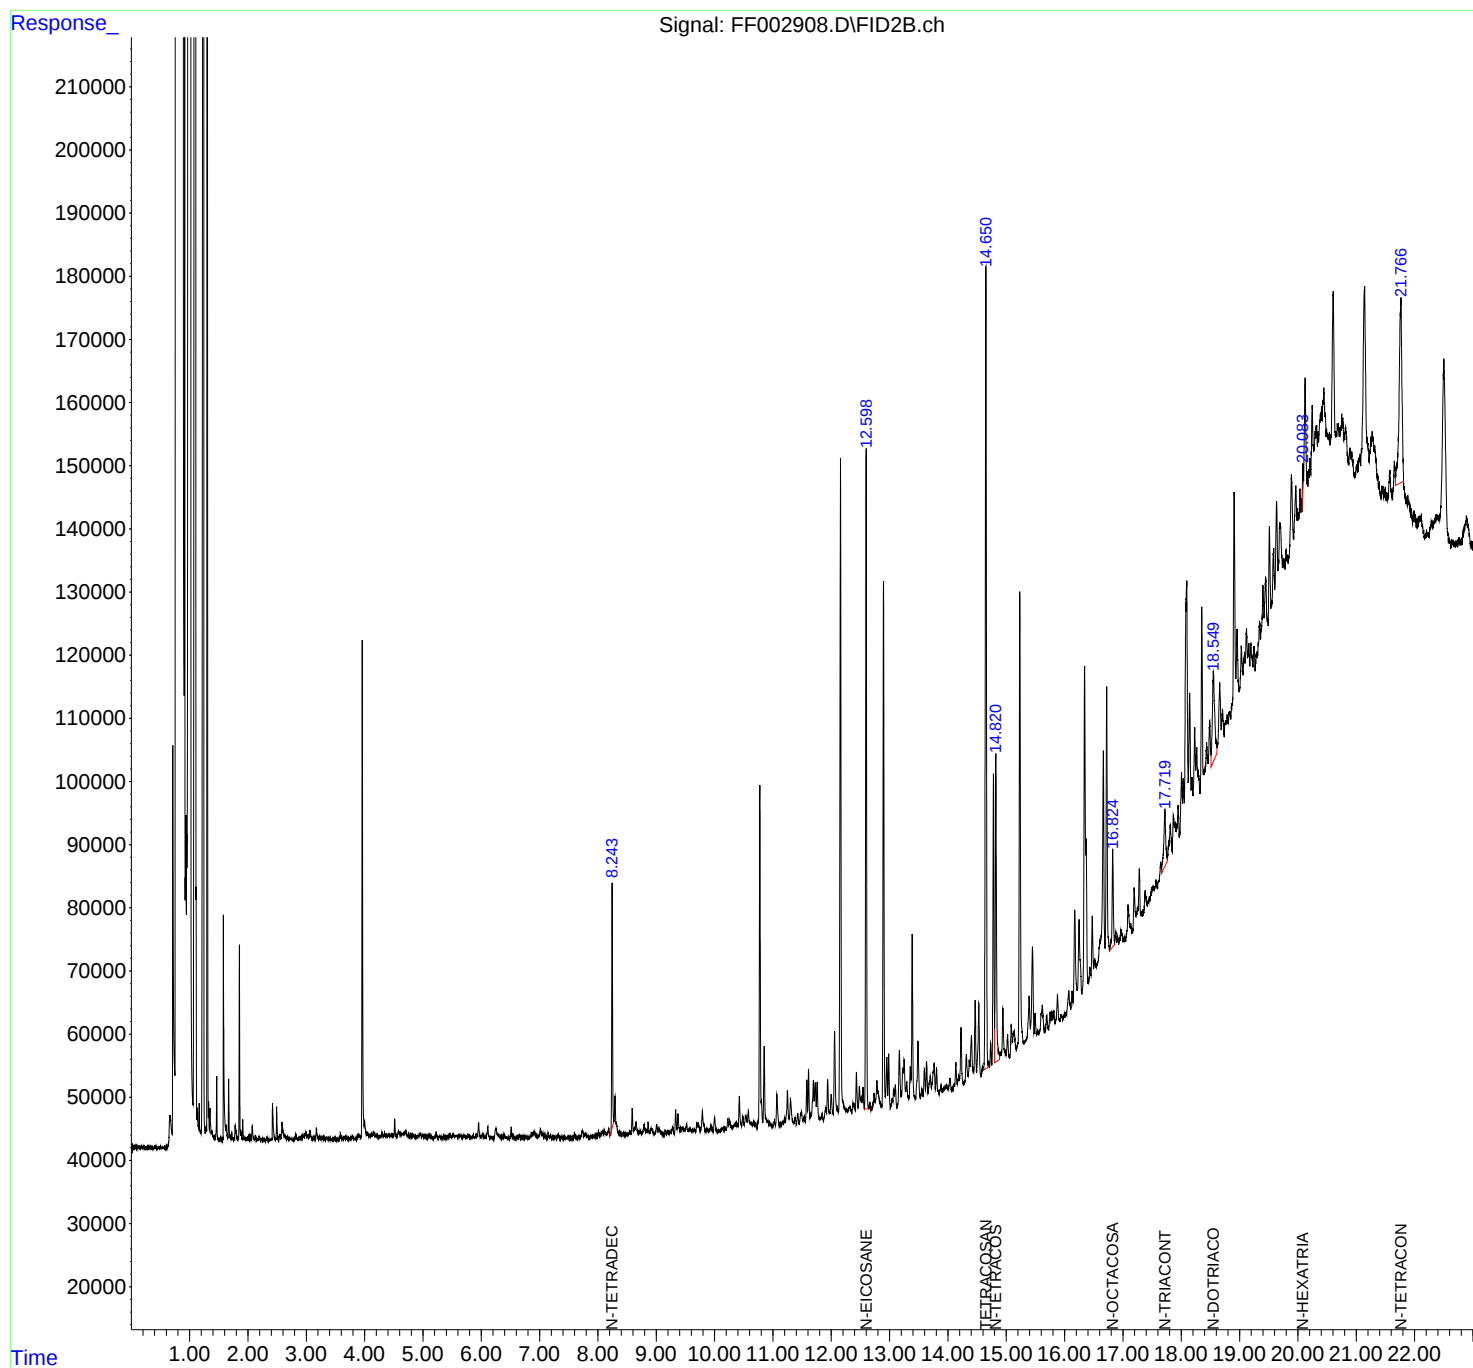


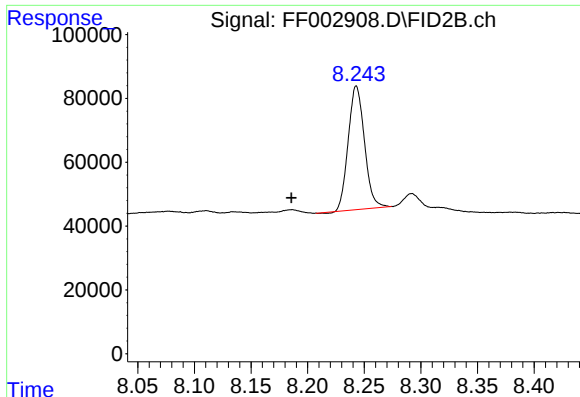

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: 0.057 min
Response: 385266
Conc: 2.40 ug/ml

Instrument :
FID_F
ClientSampleId :

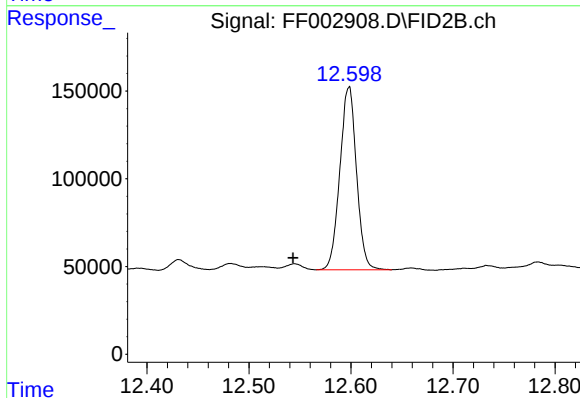


#7 N-EICOSANE

R.T.: 12.598 min
Delta R.T.: 0.055 min
Response: 1182293
Conc: 7.67 ug/ml

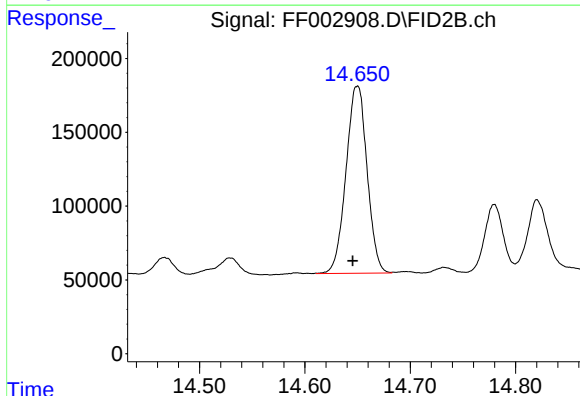


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.004 min
Response: 1763276
Conc: 13.58 ug/ml

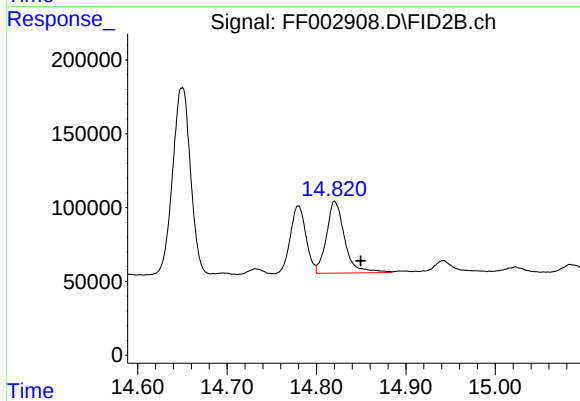

#10 N-TETRACOSANE


R.T.: 14.820 min
Delta R.T.: -0.029 min
Response: 691665
Conc: 4.79 ug/ml

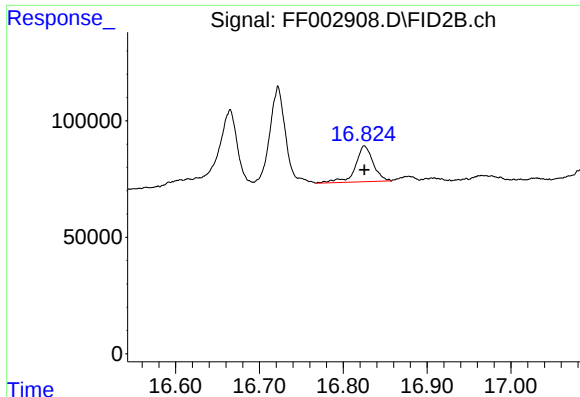

#12 N-OCTACOSANE


R.T.: 16.825 min
Delta R.T.: 0.000 min
Response: 228583
Conc: 1.71 ug/ml

Instrument :
FID_F
ClientSampleId :

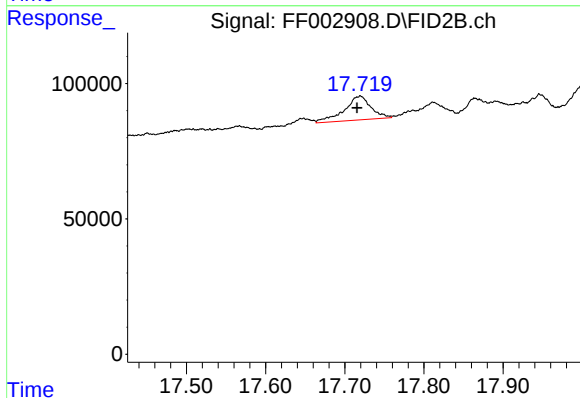


#13 N-TRIACONTANE

R.T.: 17.720 min
Delta R.T.: 0.004 min
Response: 207042
Conc: 1.62 ug/ml

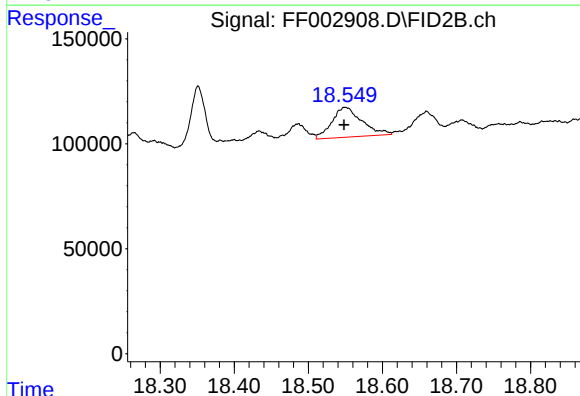


#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: 0.000 min
Response: 400266
Conc: 3.35 ug/ml

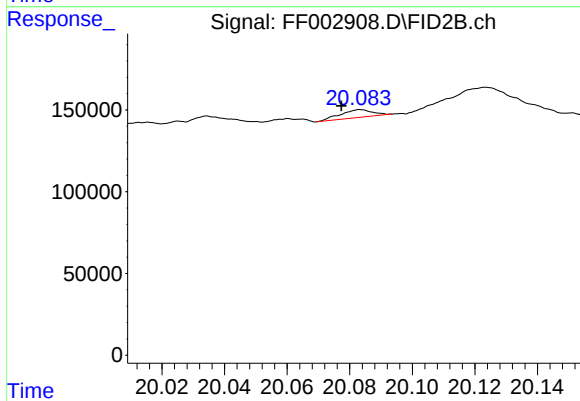

#16 N-HEXATRIACONTANE

R.T.: 20.084 min
Delta R.T.: 0.006 min
Response: 33396
Conc: 0.31 ug/ml

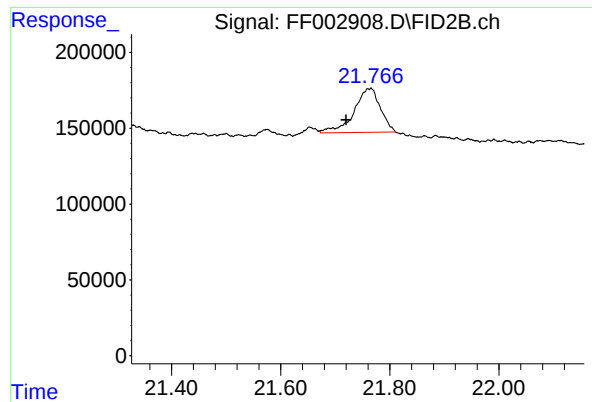

#18 N-TETRACONTANE

R.T.: 21.766 min
Delta R.T.: 0.046 min
Response: 969358
Conc: 9.22 ug/ml

Instrument :
FID_F
ClientSampleId :