

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002911.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 19:23
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:06:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	2215947	17.069 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.829	102701	0.711 ug/ml
13) N-TRIACONTANE	17.718	109901	0.858 ug/ml
14) N-DOTRIACONTANE	18.553	147895	1.238 ug/ml
15) N-TETRATRIACONTANE	19.340	85664	0.756 ug/ml
18) N-TETRACONTANE	21.723	281348	2.677 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002911.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 19:23
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:06:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

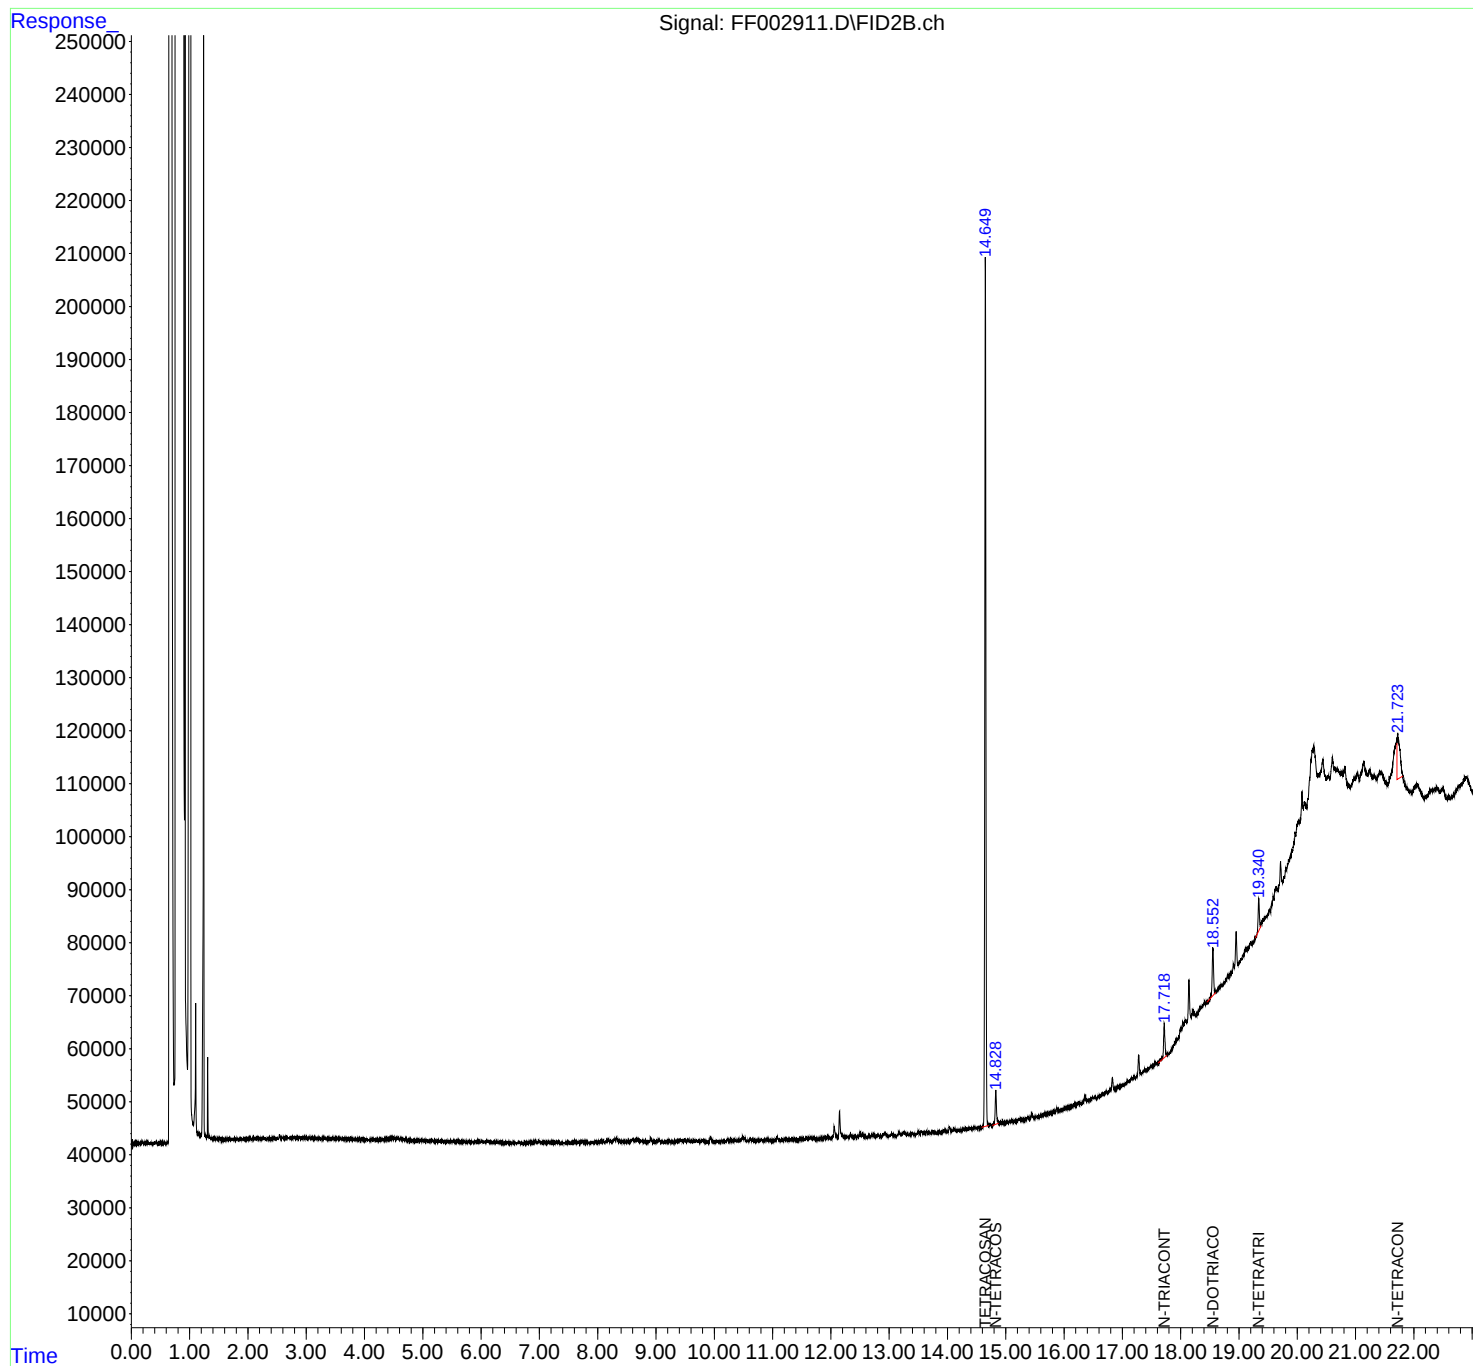


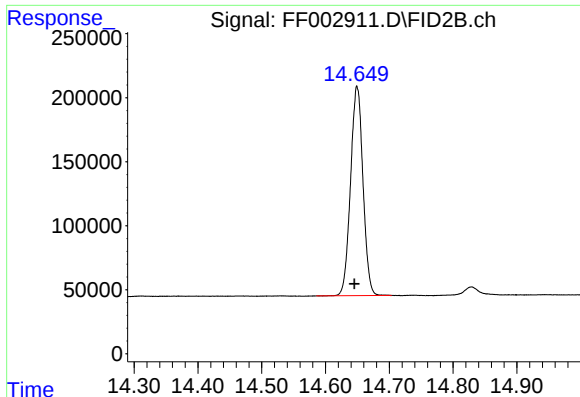

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.650 min
Delta R.T.: 0.004 min
Response: 2215947
Conc: 17.07 ug/ml

Instrument :
FID_F
ClientSampleId :

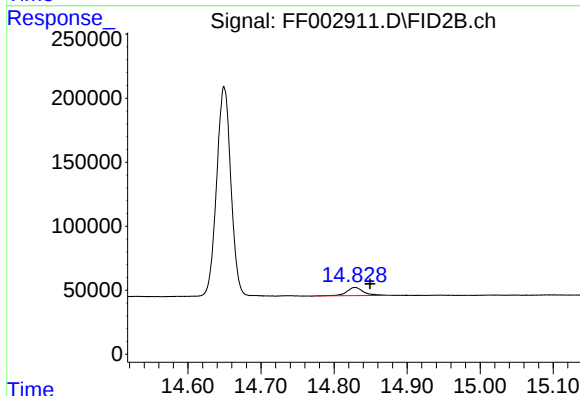


#10 N-TETRACOSANE

R.T.: 14.829 min
Delta R.T.: -0.021 min
Response: 102701
Conc: 0.71 ug/ml

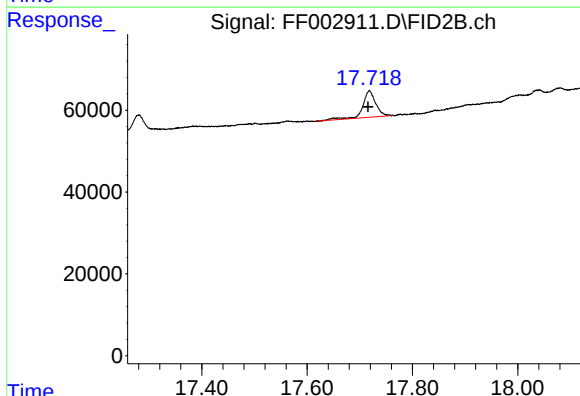


#13 N-TRIACONTANE

R.T.: 17.718 min
Delta R.T.: 0.003 min
Response: 109901
Conc: 0.86 ug/ml

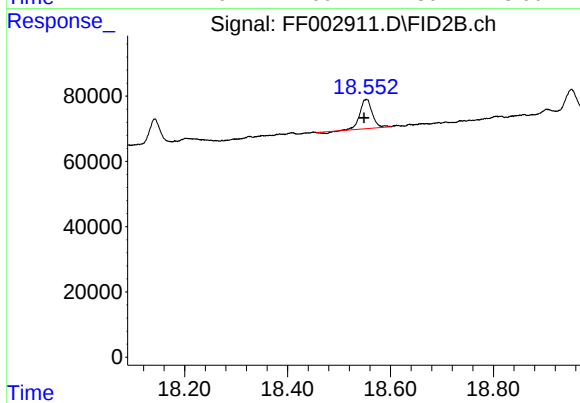

#14 N-DOTRIACONTANE


R.T.: 18.553 min
Delta R.T.: 0.005 min
Response: 147895
Conc: 1.24 ug/ml

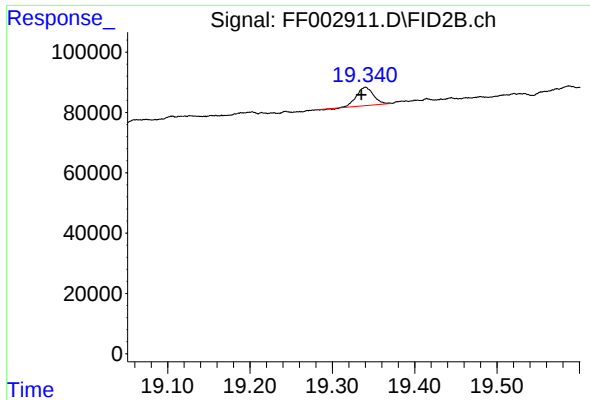

#15 N-TETRATRIACONTANE

R.T.: 19.340 min
Delta R.T.: 0.005 min
Response: 85664
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

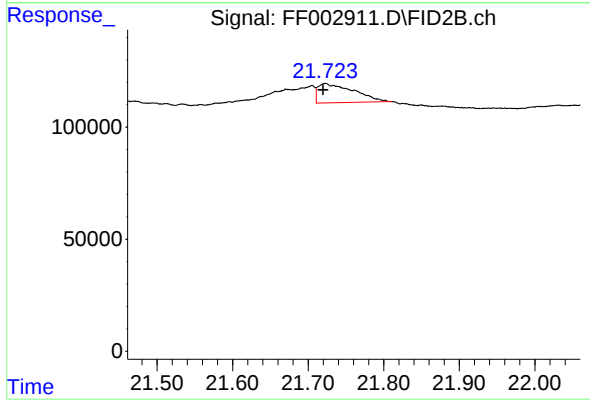

#18 N-TETRACONTANE

R.T.: 21.723 min
Delta R.T.: 0.003 min
Response: 281348
Conc: 2.68 ug/ml