

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002913.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 20:23
 Operator : AJ\SJ
 Sample : J6210-07
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:07:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	1635408	12.597 ug/ml
Target Compounds			
1) N-OCTANE	2.243	303748	1.964 ug/ml
4) N-TETRADECANE	8.243f	839193	5.236 ug/ml
7) N-EICOSANE	12.595f	752765	4.881 ug/ml
8) N-DOCOSANE	13.763	129812	0.868 ug/ml
10) N-TETRACOSANE	14.820	744332	5.151 ug/ml
12) N-OCTACOSANE	16.824	278525	2.079 ug/ml
13) N-TRIACONTANE	17.719	384045	2.997 ug/ml
14) N-DOTRIACONTANE	18.548	429891	3.600 ug/ml
15) N-TETRATRIACONTANE	19.340	117899	1.040 ug/ml
18) N-TETRACONTANE	21.757	477310	4.541 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002913.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 20:23
Operator : AJ\SJ
Sample : J6210-07
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:07:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

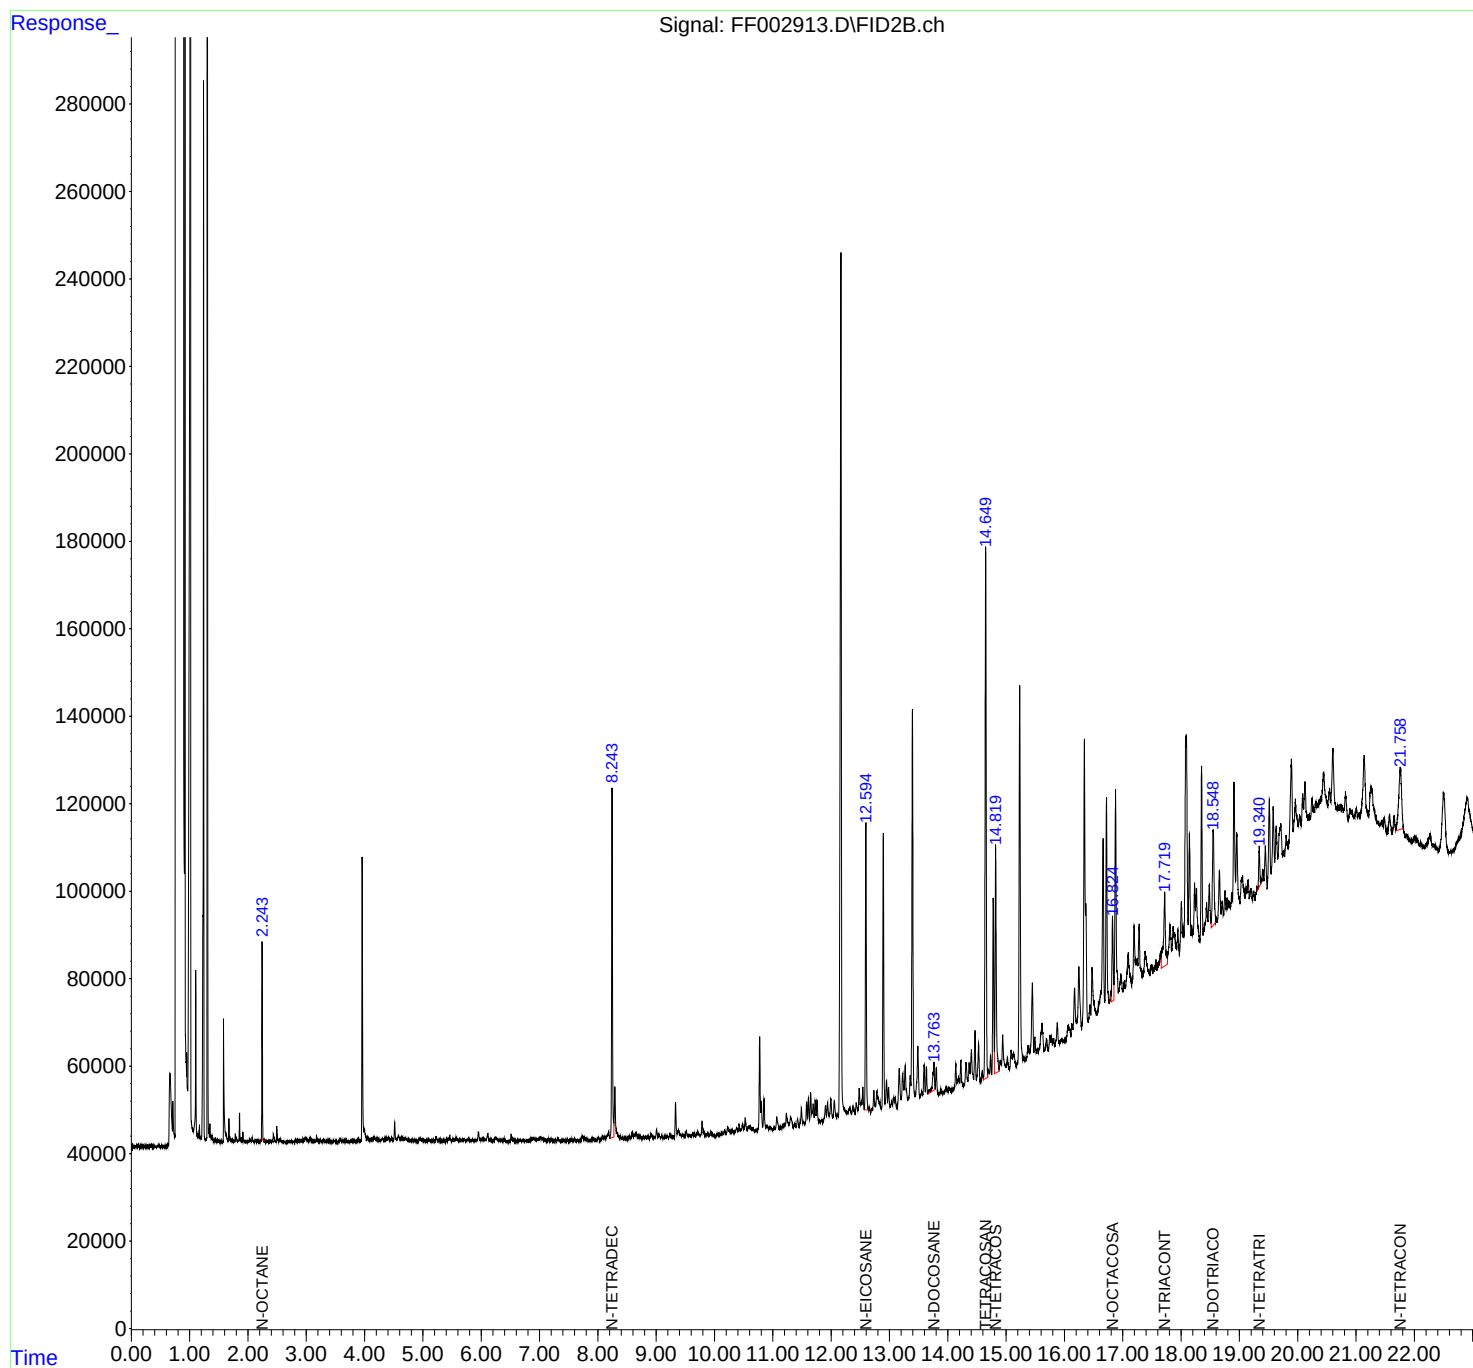


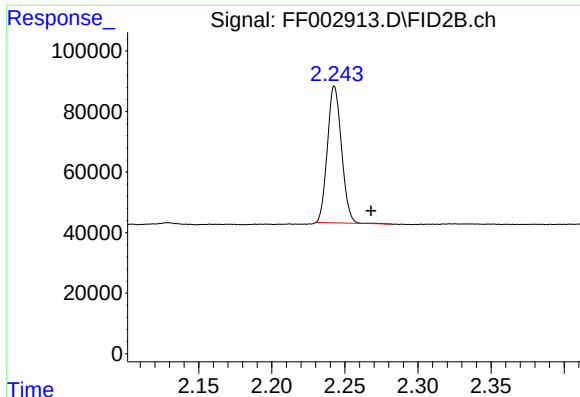

#1 N-OCTANE


R.T.: 2.243 min
Delta R.T.: -0.025 min
Response: 303748
Conc: 1.96 ug/ml

Instrument :
FID_F
ClientSampleId :

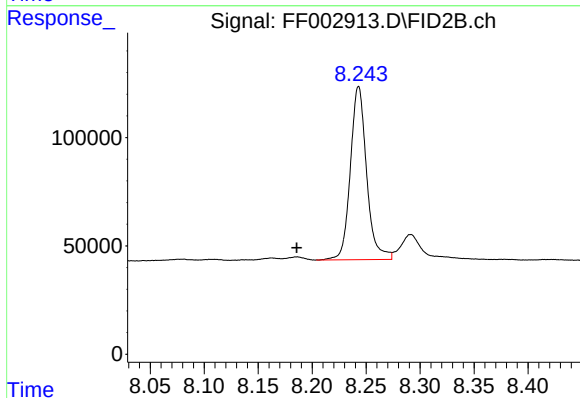


#4 N-TETRADECANE

R.T.: 8.243 min
Delta R.T.: 0.057 min
Response: 839193
Conc: 5.24 ug/ml

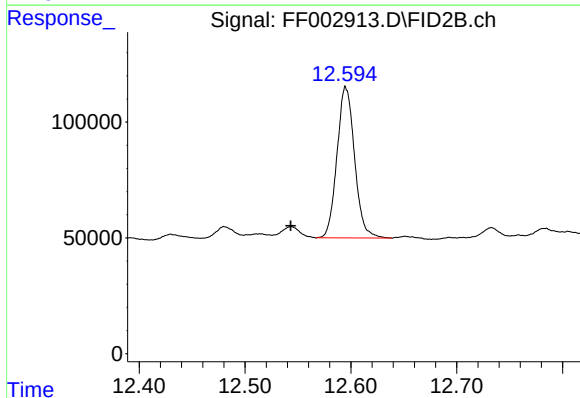


#7 N-EICOSANE

R.T.: 12.595 min
Delta R.T.: 0.052 min
Response: 752765
Conc: 4.88 ug/ml

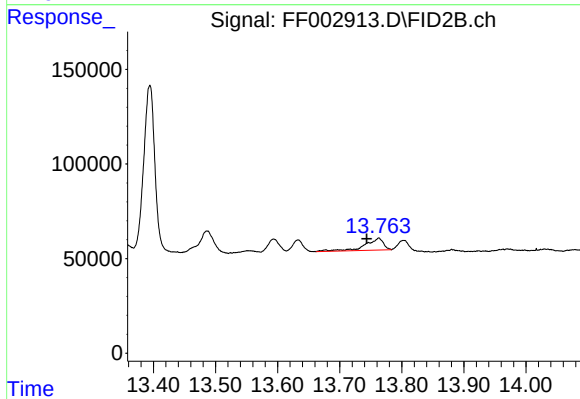

#8 N-DOCOSANE


R.T.: 13.763 min
Delta R.T.: 0.019 min
Response: 129812
Conc: 0.87 ug/ml

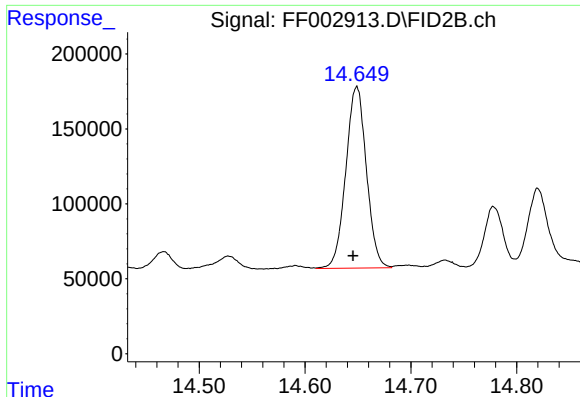

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.649 min
Delta R.T.: 0.004 min
Response: 1635408
Conc: 12.60 ug/ml

Instrument :
FID_F
ClientSampleId :

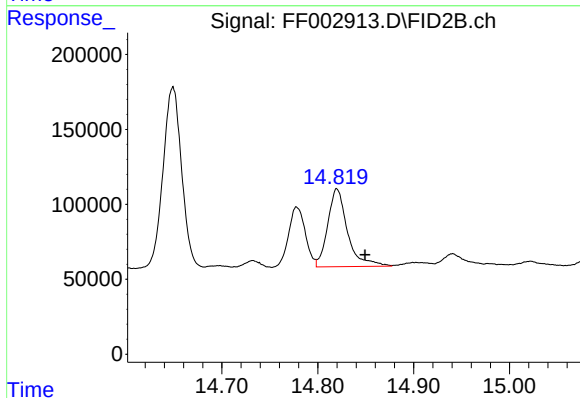


#10 N-TETRACOSANE

R.T.: 14.820 min
Delta R.T.: -0.030 min
Response: 744332
Conc: 5.15 ug/ml

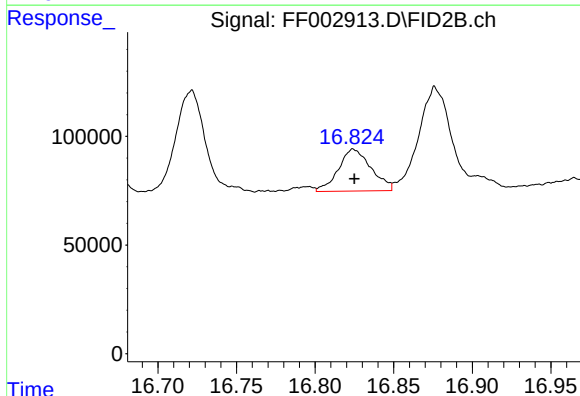


#12 N-OCTACOSANE

R.T.: 16.824 min
Delta R.T.: 0.000 min
Response: 278525
Conc: 2.08 ug/ml

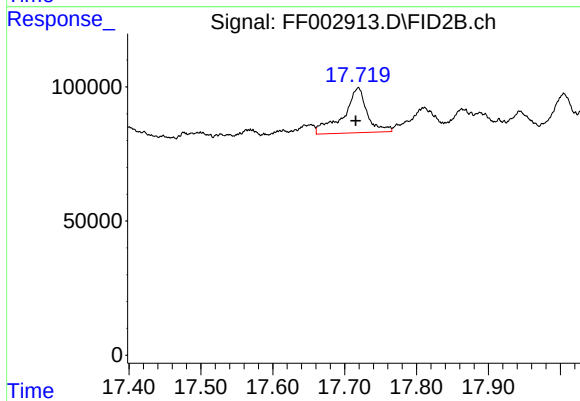

#13 N-TRIACONTANE


R.T.: 17.719 min
Delta R.T.: 0.004 min
Response: 384045
Conc: 3.00 ug/ml

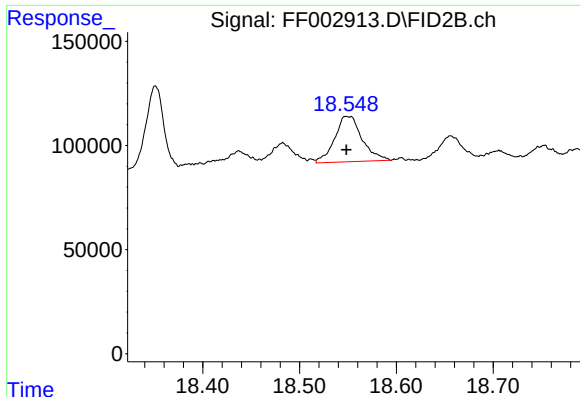

#14 N-DOTRIACONTANE


R.T.: 18.548 min
Delta R.T.: 0.000 min
Response: 429891
Conc: 3.60 ug/ml

Instrument :
FID_F
ClientSampleId :

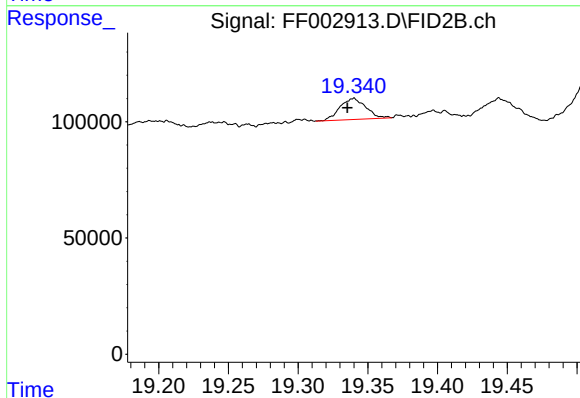

#15 N-TETRATRIACONTANE

R.T.: 19.340 min
Delta R.T.: 0.004 min
Response: 117899
Conc: 1.04 ug/ml

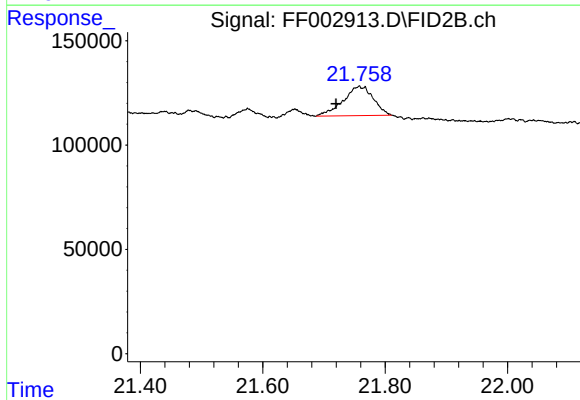

#18 N-TETRACONTANE

R.T.: 21.757 min
Delta R.T.: 0.038 min
Response: 477310
Conc: 4.54 ug/ml