

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120518\  
 Data File : FF002916.D  
 Signal(s) : FID2B.ch  
 Acq On : 05 Dec 2018 21:55  
 Operator : AJ\SJ  
 Sample : J6208-17 10X  
 Misc :  
 ALS Vial : 70 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Dec 06 03:07:20 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120418.M  
 Quant Title :  
 QLast Update : Tue Dec 04 16:40:56 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.648  | 326926   | 2.518 ug/ml |
| Target Compounds              |         |          |             |
| 5) N-HEXADECANE               | 9.793   | 113153   | 0.707 ug/ml |
| 7) N-EICOSANE                 | 12.514  | 114445   | 0.742 ug/ml |
| 8) N-DOCOSANE                 | 13.763  | 250797   | 1.677 ug/ml |
| 10) N-TETRACOSANE             | 14.820  | 1138113  | 7.875 ug/ml |
| 12) N-OCTACOSANE              | 16.822  | 278394   | 2.078 ug/ml |
| 13) N-TRIACONTANE             | 17.719  | 195333   | 1.524 ug/ml |
| 14) N-DOTRIACONTANE           | 18.480f | 163696   | 1.371 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120518\  
Data File : FF002916.D  
Signal(s) : FID2B.ch  
Acq On : 05 Dec 2018 21:55  
Operator : AJ\SJ  
Sample : J6208-17 10X  
Misc :  
ALS Vial : 70 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 06 03:07:20 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120418.M  
Quant Title :  
QLast Update : Tue Dec 04 16:40:56 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

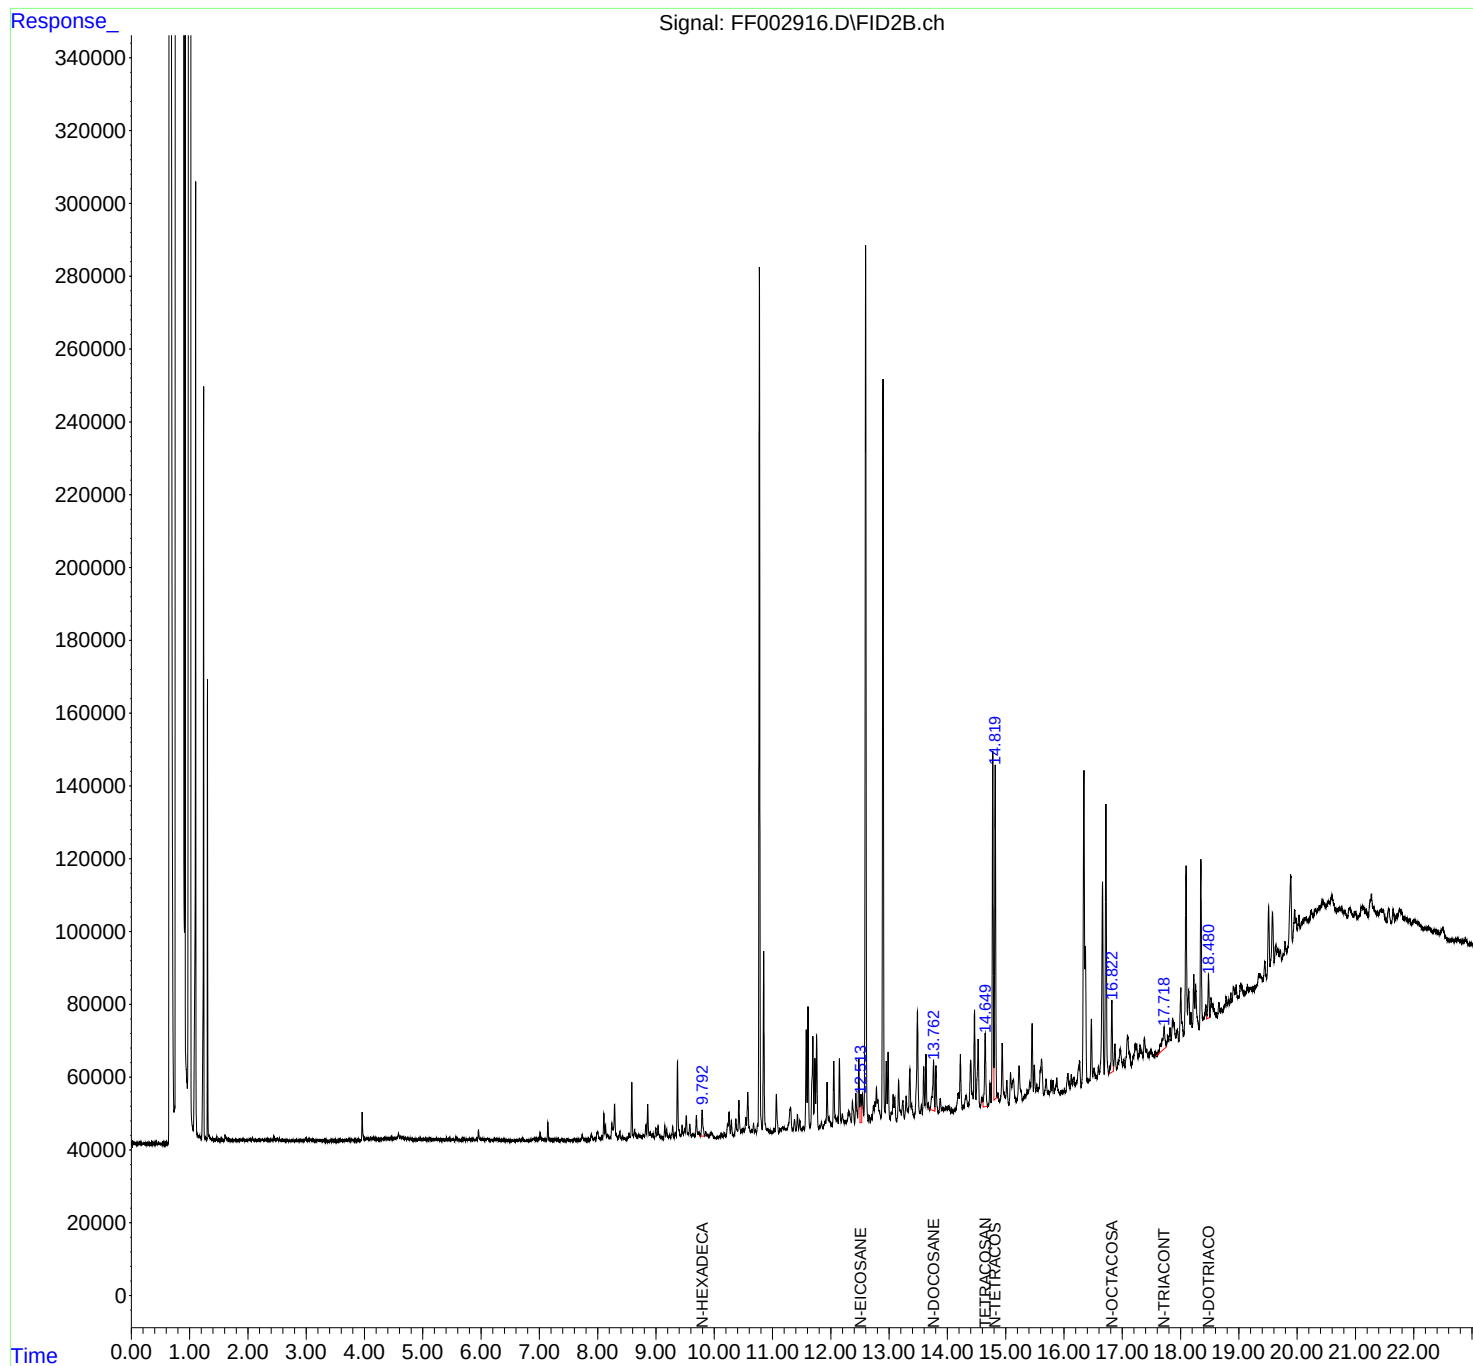


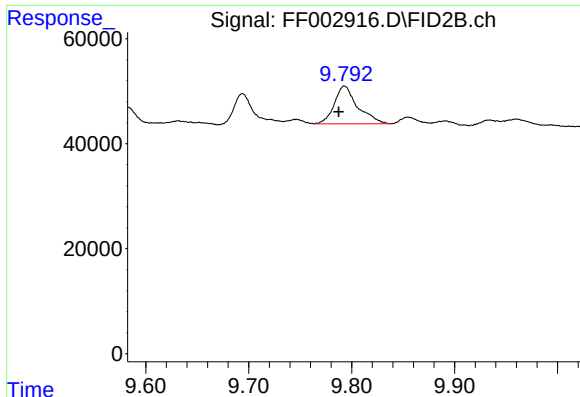

#5 N-HEXADECANE


R.T.: 9.793 min  
Delta R.T.: 0.006 min  
Response: 113153  
Conc: 0.71 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

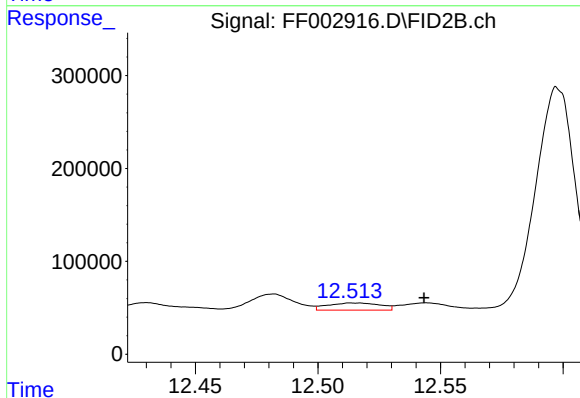


#7 N-EICOSANE

R.T.: 12.514 min  
Delta R.T.: -0.029 min  
Response: 114445  
Conc: 0.74 ug/ml

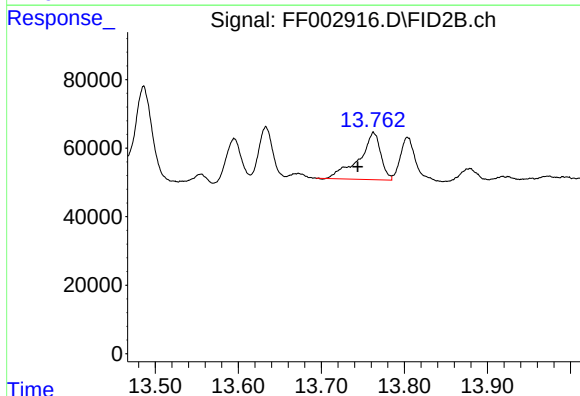


#8 N-DOCOSANE

R.T.: 13.763 min  
Delta R.T.: 0.019 min  
Response: 250797  
Conc: 1.68 ug/ml

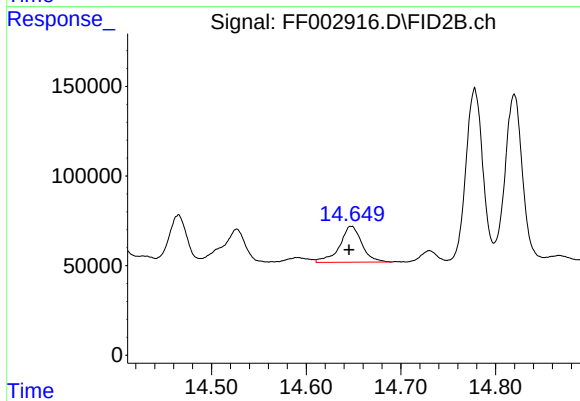

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.648 min  
Delta R.T.: 0.002 min  
Response: 326926  
Conc: 2.52 ug/ml

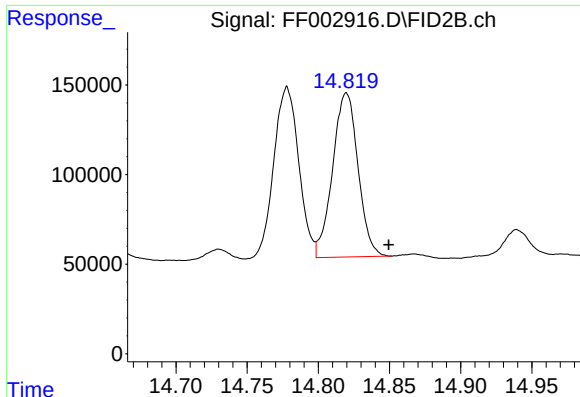

#10 N-TETRACOSANE


R.T.: 14.820 min  
Delta R.T.: -0.030 min  
Response: 1138113  
Conc: 7.88 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

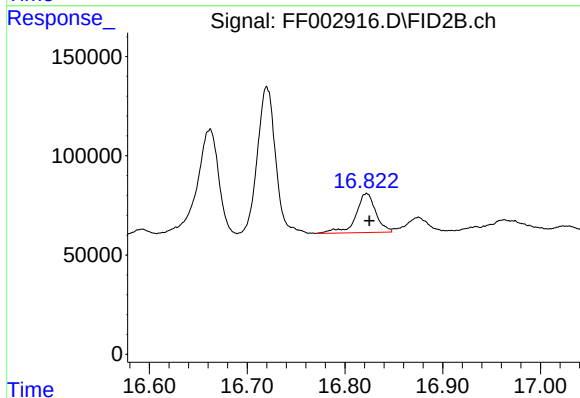


#12 N-OCTACOSANE

R.T.: 16.822 min  
Delta R.T.: -0.003 min  
Response: 278394  
Conc: 2.08 ug/ml

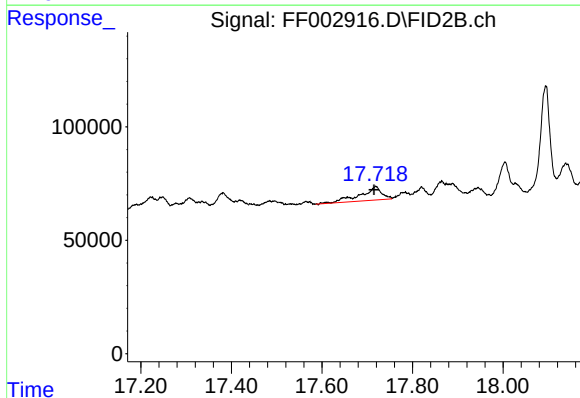

#13 N-TRIACONTANE

R.T.: 17.719 min  
Delta R.T.: 0.004 min  
Response: 195333  
Conc: 1.52 ug/ml

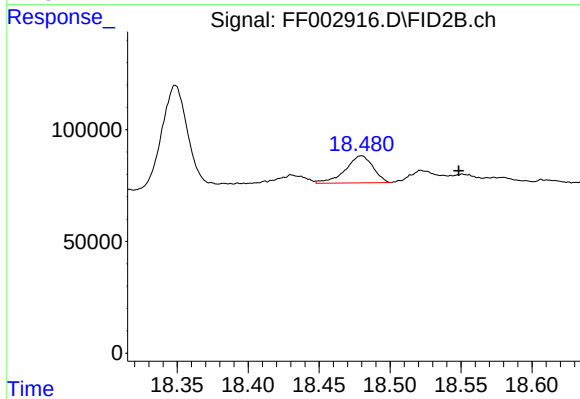

#14 N-DOTRIACONTANE

R.T.: 18.480 min  
Delta R.T.: -0.069 min  
Response: 163696  
Conc: 1.37 ug/ml