

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002917.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 22:25
 Operator : AJ\SJ
 Sample : J6148-01 10X
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:07:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	240801	1.855 ug/ml
Target Compounds			
7) N-EICOSANE	12.595f	650012	4.215 ug/ml
8) N-DOCOSANE	13.761	146068	0.977 ug/ml
10) N-TETRACOSANE	14.822	1000999	6.927 ug/ml
12) N-OCTACOSANE	16.821	232673	1.737 ug/ml
13) N-TRIACONTANE	17.689	484825	3.784 ug/ml
14) N-DOTRIACONTANE	18.555	51098	0.428 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002917.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 22:25
Operator : AJ\SJ
Sample : J6148-01 10X
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:07:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

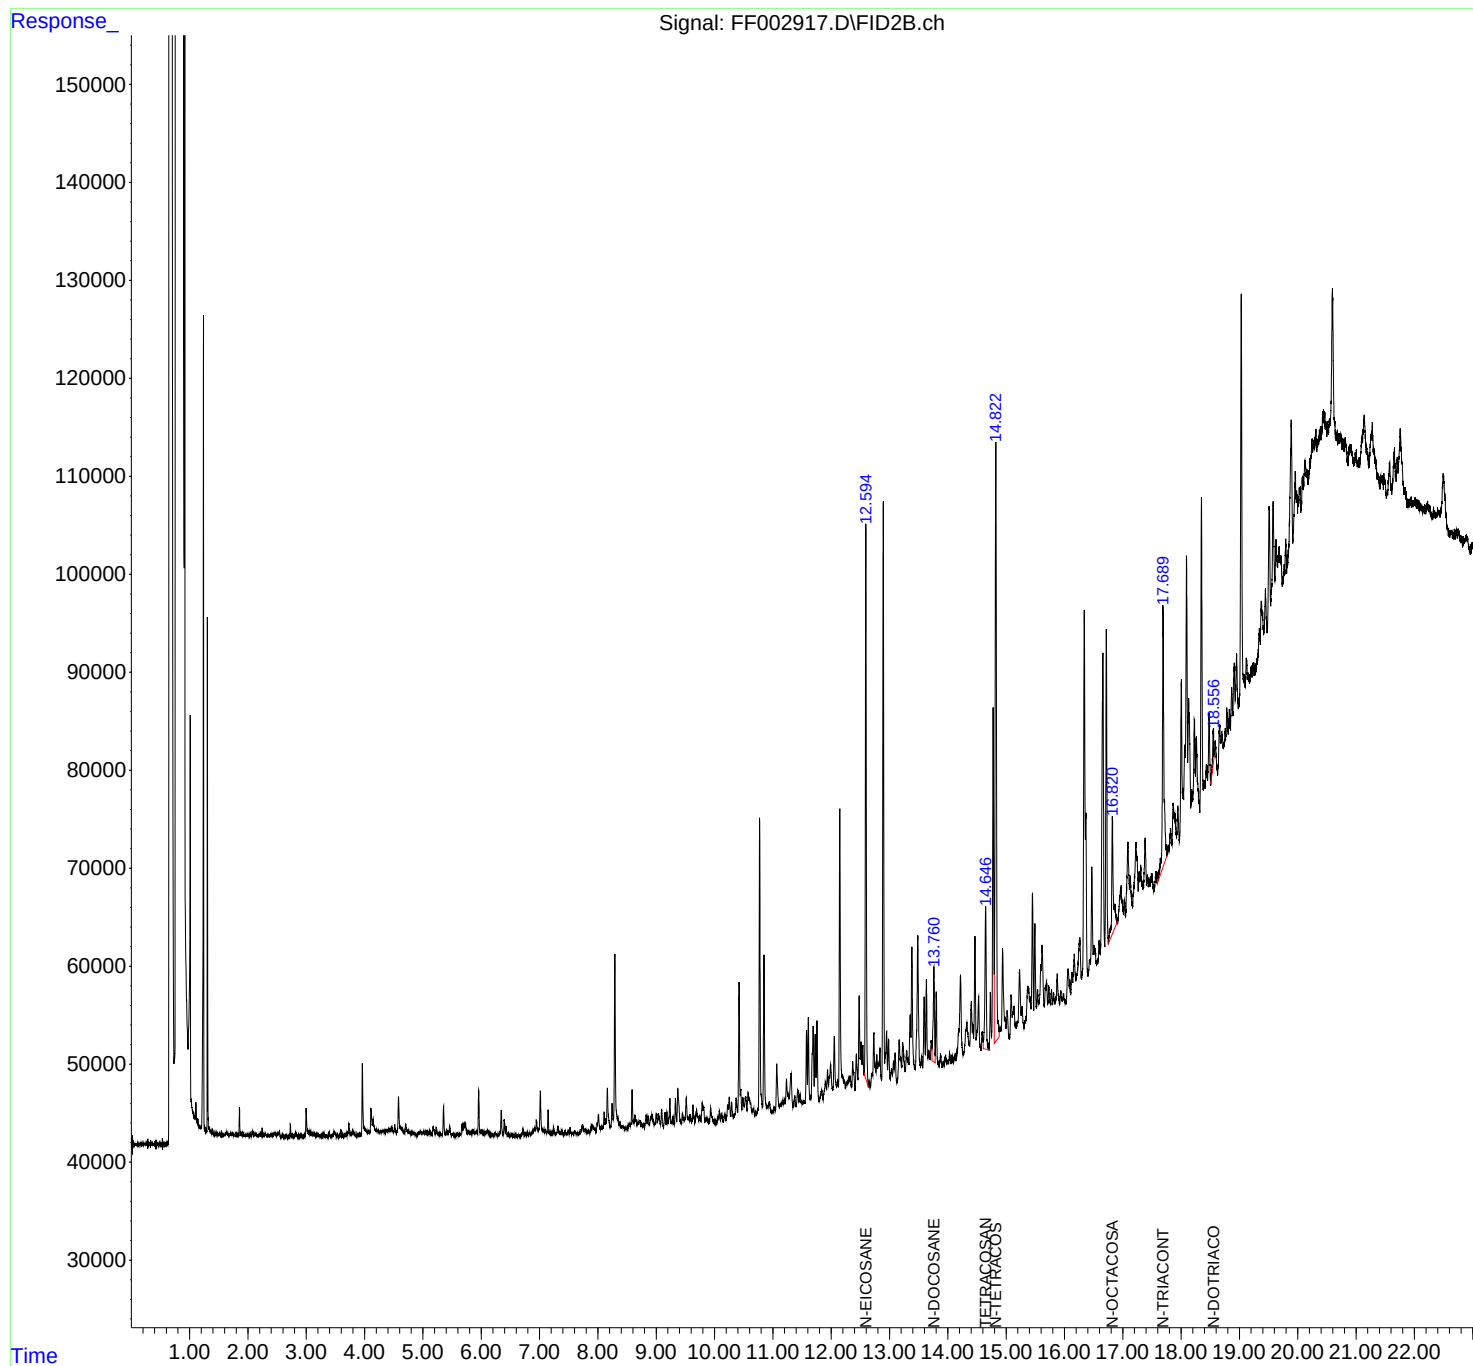


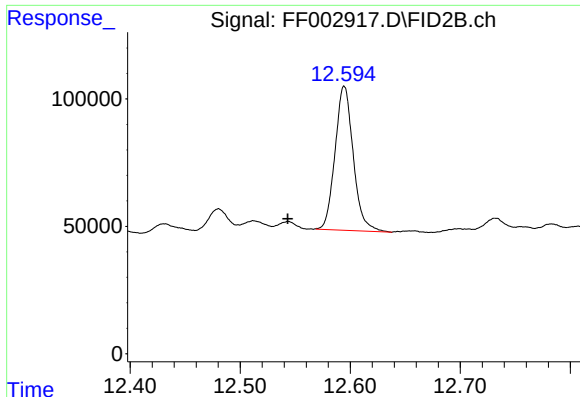

#7 N-EICOSANE


R.T.: 12.595 min
Delta R.T.: 0.051 min
Response: 650012
Conc: 4.21 ug/ml

Instrument :
FID_F
ClientSampleId :

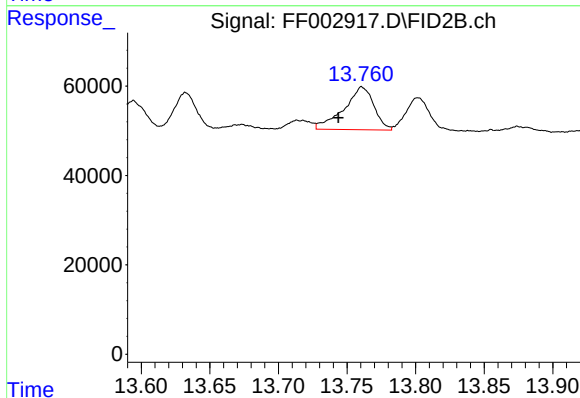


#8 N-DOCOSANE

R.T.: 13.761 min
Delta R.T.: 0.017 min
Response: 146068
Conc: 0.98 ug/ml

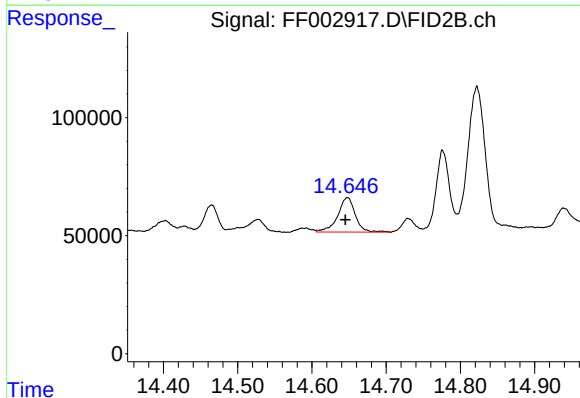


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min
Delta R.T.: 0.003 min
Response: 240801
Conc: 1.85 ug/ml

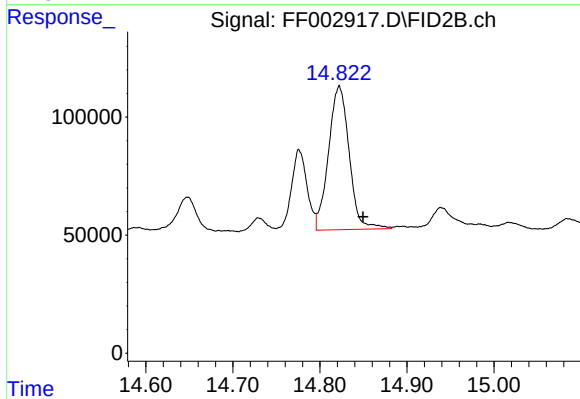

#10 N-TETRACOSANE


R.T.: 14.822 min
Delta R.T.: -0.027 min
Response: 1000999
Conc: 6.93 ug/ml

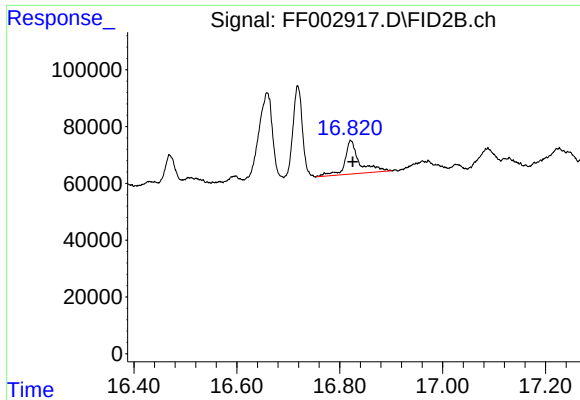

#12 N-OCTACOSANE


R.T.: 16.821 min
Delta R.T.: -0.004 min
Response: 232673
Conc: 1.74 ug/ml

Instrument :
FID_F
ClientSampleId :

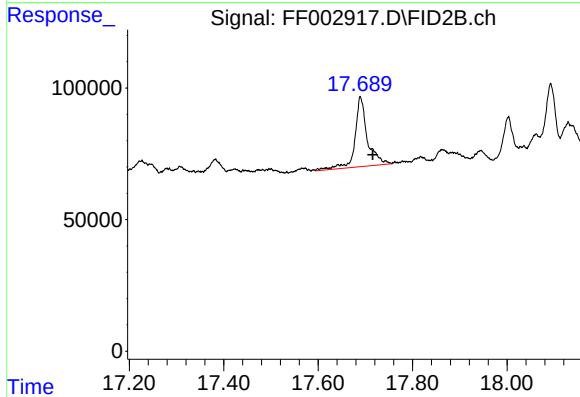

#13 N-TRIACONTANE

R.T.: 17.689 min
Delta R.T.: -0.026 min
Response: 484825
Conc: 3.78 ug/ml

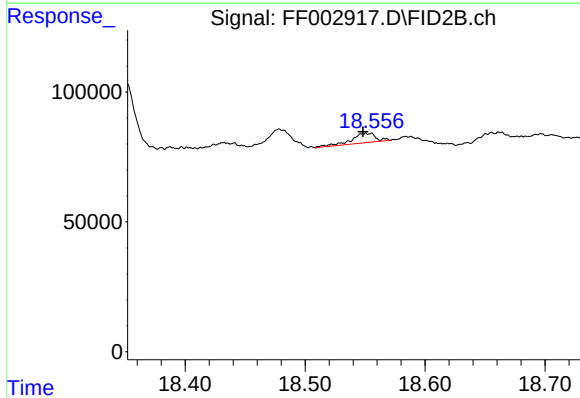

#14 N-DOTRIACONTANE

R.T.: 18.555 min
Delta R.T.: 0.006 min
Response: 51098
Conc: 0.43 ug/ml