

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002918.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 22:55
 Operator : AJ\SJ
 Sample : J6208-21 20X
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:07:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	129508	0.998 ug/ml
Target Compounds			
7) N-EICOSANE	12.595f	198371	1.286 ug/ml
10) N-TETRACOSANE	14.819	383449	2.653 ug/ml
12) N-OCTACOSANE	16.824	109227	0.815 ug/ml
13) N-TRIACONTANE	17.698	844408	6.590 ug/ml
14) N-DOTRIACONTANE	18.552	220012	1.842 ug/ml
15) N-TETRATRIACONTANE	19.342	340998	3.009 ug/ml
16) N-HEXATRIACONTANE	20.088	156315	1.449 ug/ml
17) N-OCTATRIACONTANE	20.824	247906	2.443 ug/ml
18) N-TETRACONTANE	21.753	389645	3.707 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002918.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 22:55
Operator : AJ\SJ
Sample : J6208-21 20X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:07:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

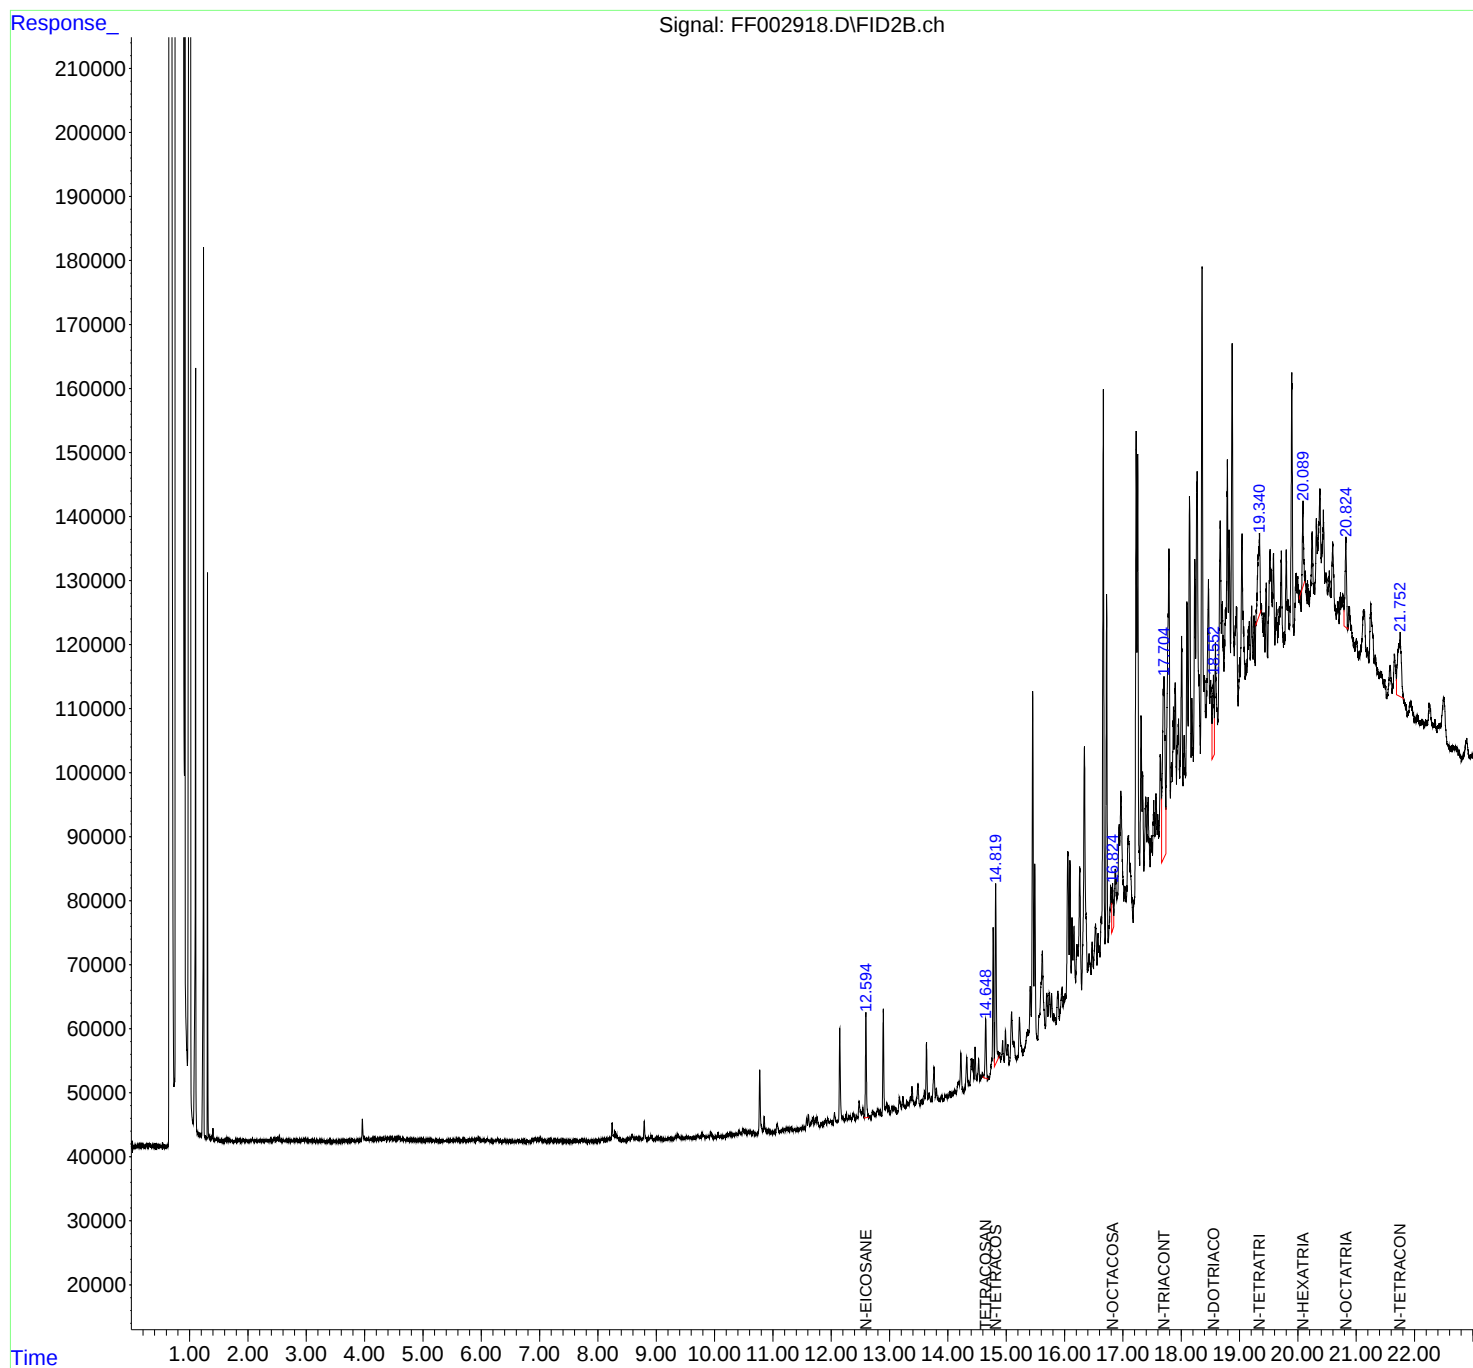


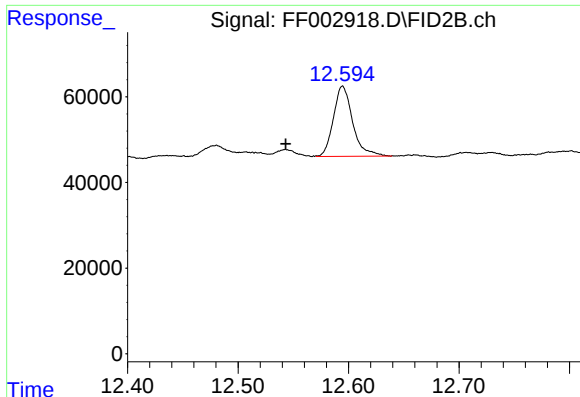

#7 N-EICOSANE


R.T.: 12.595 min
Delta R.T.: 0.051 min
Response: 198371
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :

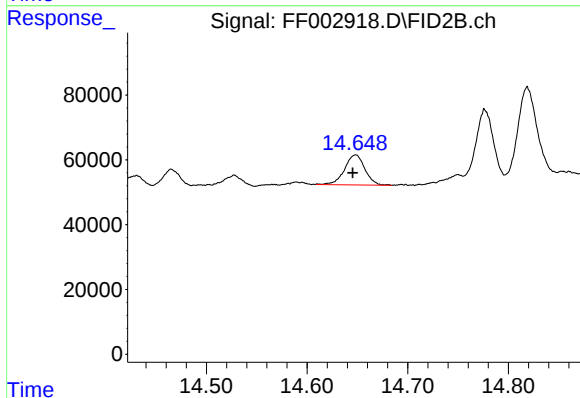


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min
Delta R.T.: 0.003 min
Response: 129508
Conc: 1.00 ug/ml

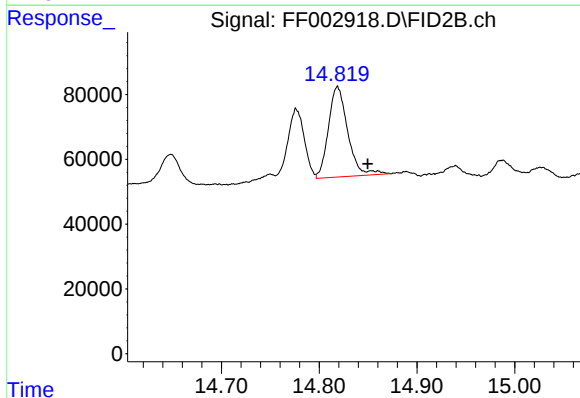


#10 N-TETRACOSANE

R.T.: 14.819 min
Delta R.T.: -0.031 min
Response: 383449
Conc: 2.65 ug/ml

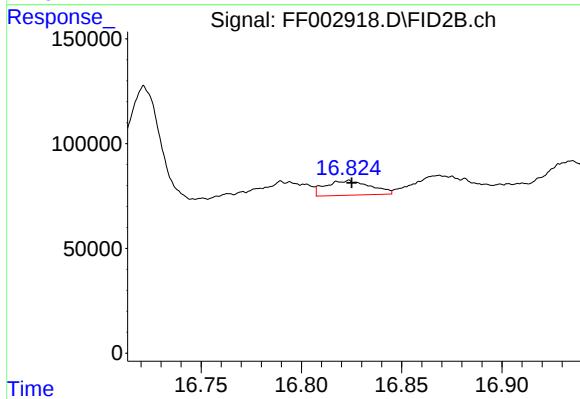

#12 N-OCTACOSANE


R.T.: 16.824 min
Delta R.T.: -0.001 min
Response: 109227
Conc: 0.82 ug/ml

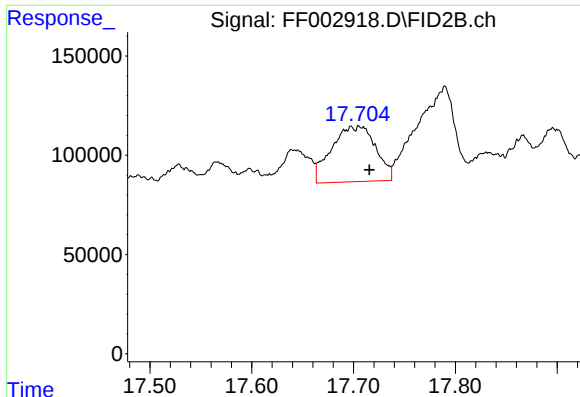

#13 N-TRIACONTANE


R.T.: 17.698 min
Delta R.T.: -0.018 min
Response: 844408
Conc: 6.59 ug/ml

Instrument :
FID_F
ClientSampleId :

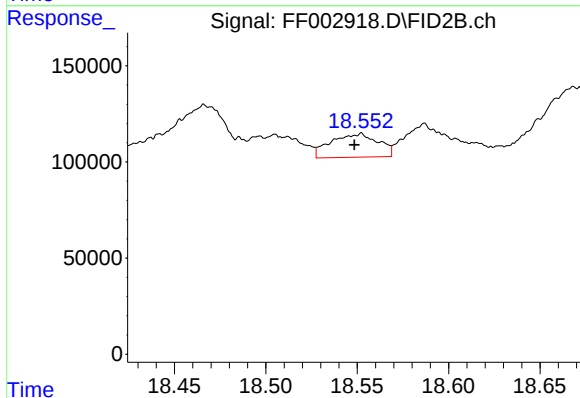


#14 N-DOTRIACONTANE

R.T.: 18.552 min
Delta R.T.: 0.004 min
Response: 220012
Conc: 1.84 ug/ml

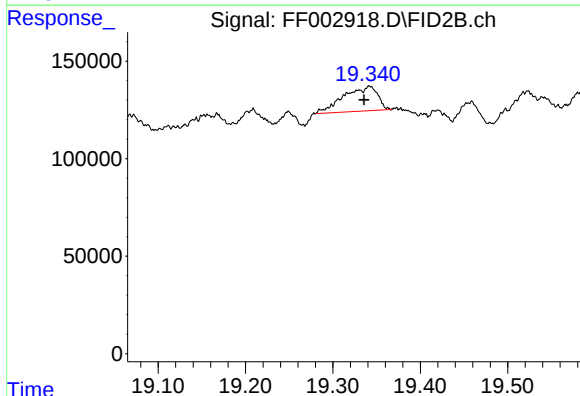


#15 N-TETRATRIACONTANE

R.T.: 19.342 min
Delta R.T.: 0.007 min
Response: 340998
Conc: 3.01 ug/ml

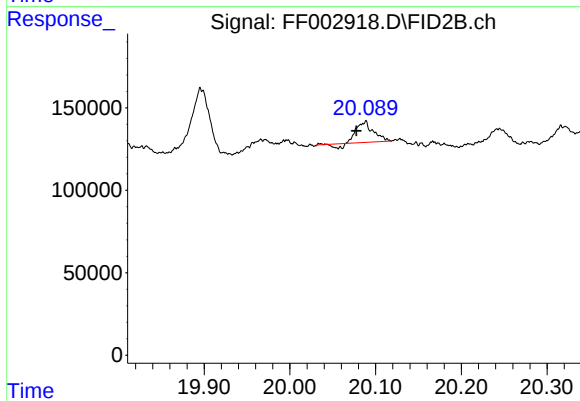

#16 N-HEXATRIACONTANE


R.T.: 20.088 min
Delta R.T.: 0.011 min
Response: 156315
Conc: 1.45 ug/ml

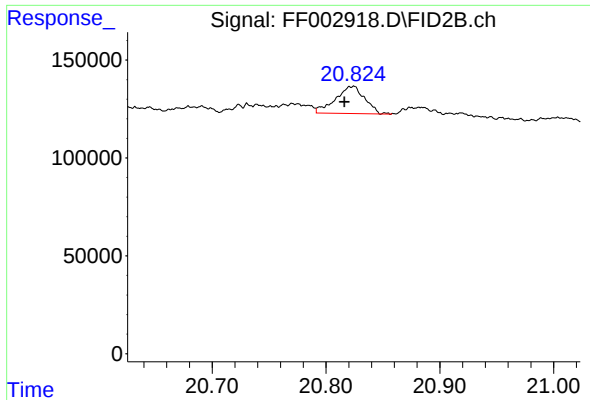

#17 N-OCTATRIACONTANE

R.T.: 20.824 min
Delta R.T.: 0.008 min
Response: 247906
Conc: 2.44 ug/ml

Instrument :
FID_F
ClientSampleId :

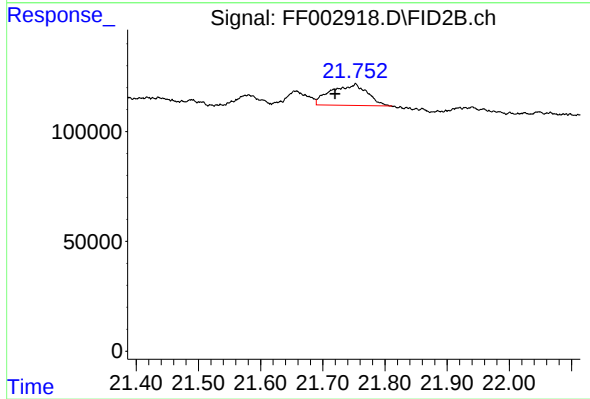

#18 N-TETRACONTANE

R.T.: 21.753 min
Delta R.T.: 0.033 min
Response: 389645
Conc: 3.71 ug/ml