

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002920.D
 Signal(s) : FID2B.ch
 Acq On : 05 Dec 2018 23:56
 Operator : AJ\SJ
 Sample : J6210-09 5X
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:07:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	346839	2.672 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	229755	1.433 ug/ml
10) N-TETRACOSANE	14.825	108199	0.749 ug/ml
14) N-DOTRIACONTANE	18.550	102709	0.860 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002920.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2018 23:56
Operator : AJ\SJ
Sample : J6210-09 5X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:07:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

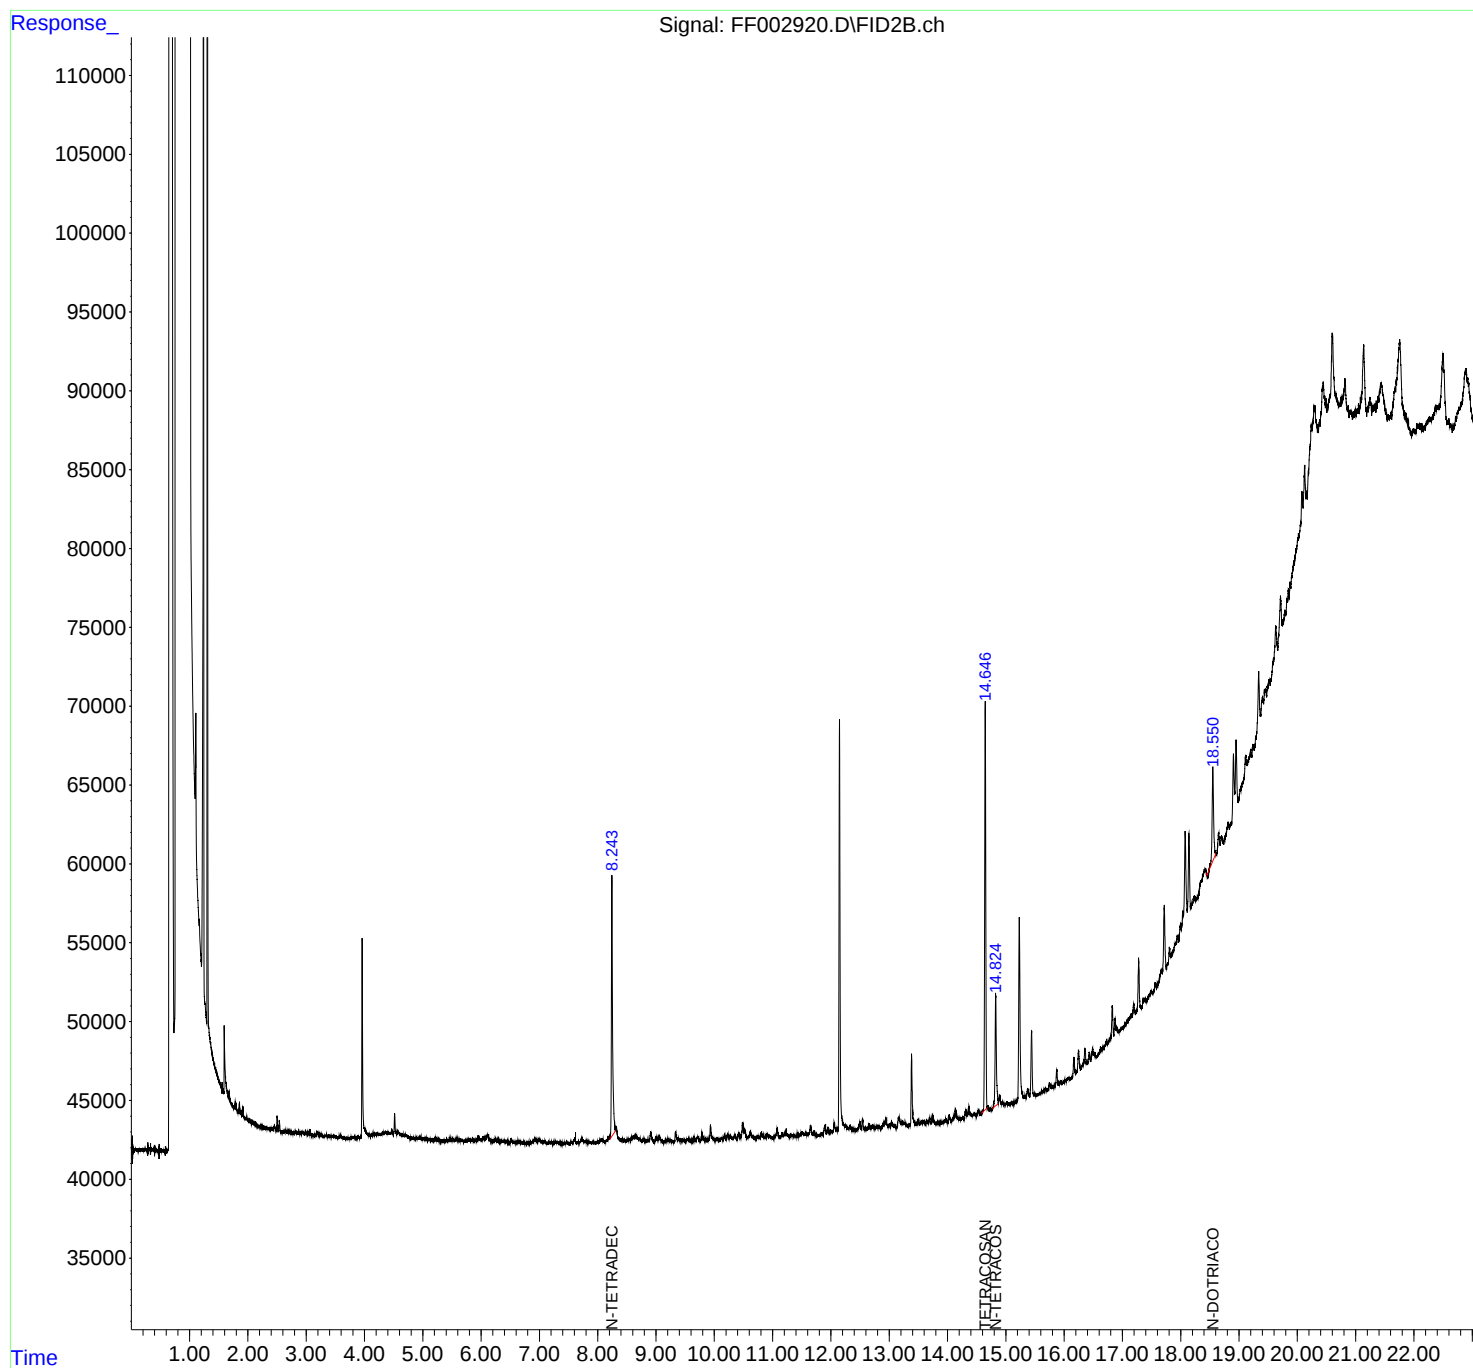


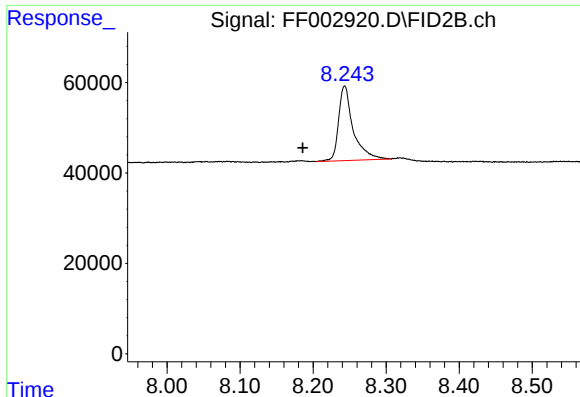

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: 0.058 min
Response: 229755
Conc: 1.43 ug/ml

Instrument :
FID_F
ClientSampleId :

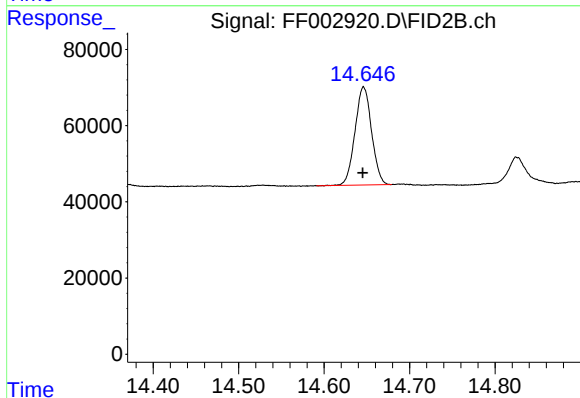


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.646 min
Delta R.T.: 0.000 min
Response: 346839
Conc: 2.67 ug/ml

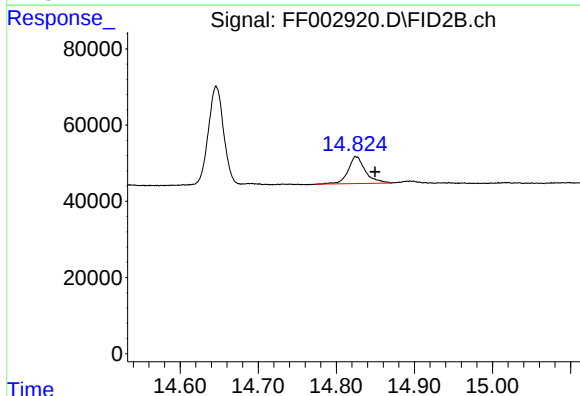

#10 N-TETRACOSANE

R.T.: 14.825 min
Delta R.T.: -0.024 min
Response: 108199
Conc: 0.75 ug/ml

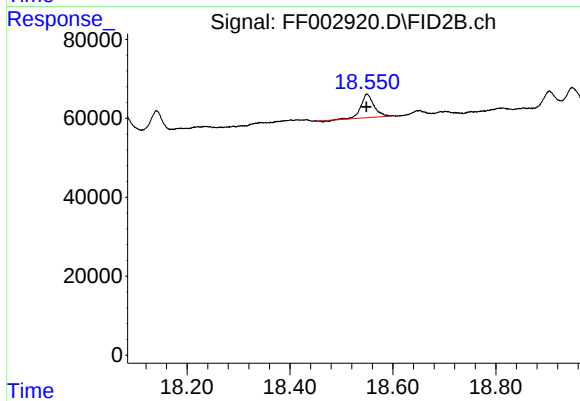

#14 N-DOTRIACONTANE

R.T.: 18.550 min
Delta R.T.: 0.001 min
Response: 102709
Conc: 0.86 ug/ml