

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002921.D
 Signal(s) : FID2B.ch
 Acq On : 06 Dec 2018 00:26
 Operator : AJ\SJ
 Sample : J6208-09 5X
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:07:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	450723	3.472 ug/ml
Target Compounds			
7) N-EICOSANE	12.595f	1344610	8.718 ug/ml
8) N-DOCOSANE	13.761	193865	1.296 ug/ml
10) N-TETRACOSANE	14.817	726001	5.024 ug/ml
12) N-OCTACOSANE	16.820	152649	1.139 ug/ml
13) N-TRIACONTANE	17.714	140153	1.094 ug/ml
14) N-DOTRIACONTANE	18.550	174940	1.465 ug/ml
15) N-TETRATRIACONTANE	19.335	82225	0.726 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002921.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2018 00:26
Operator : AJ\SJ
Sample : J6208-09 5X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Dec 06 03:07:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

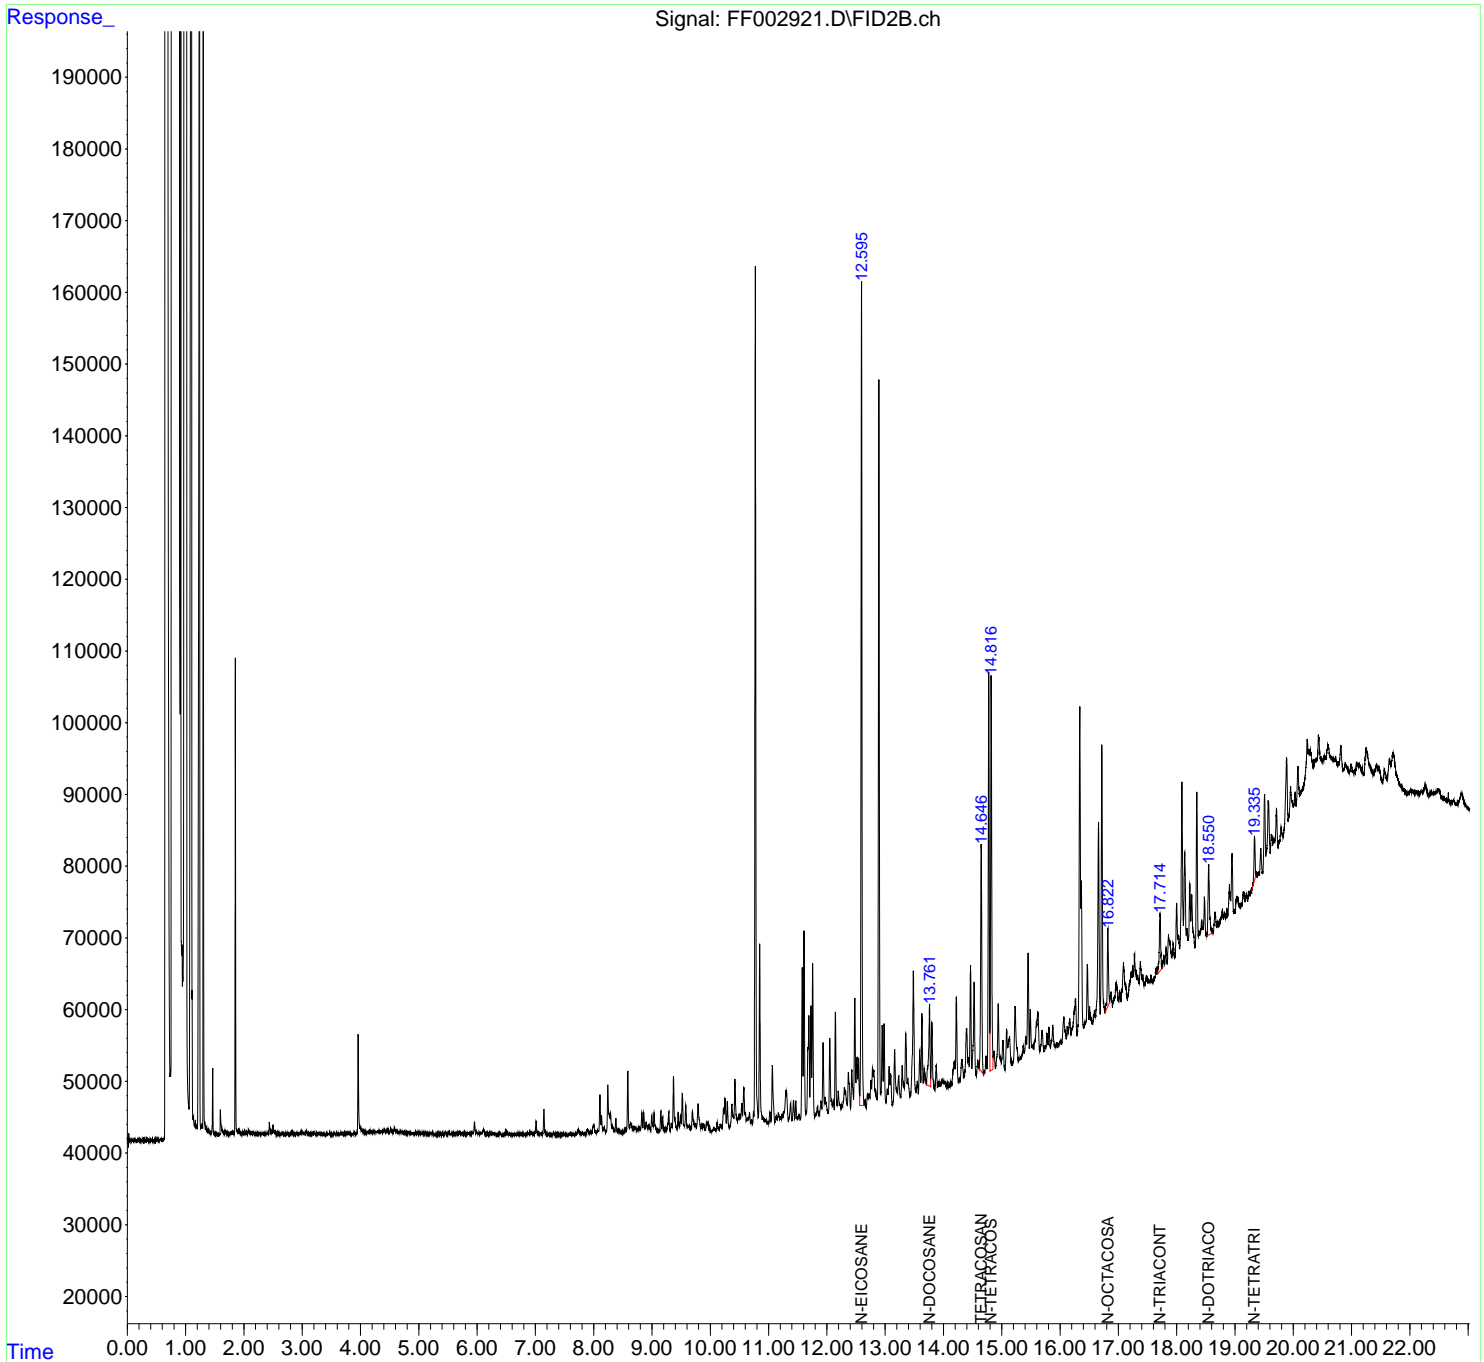

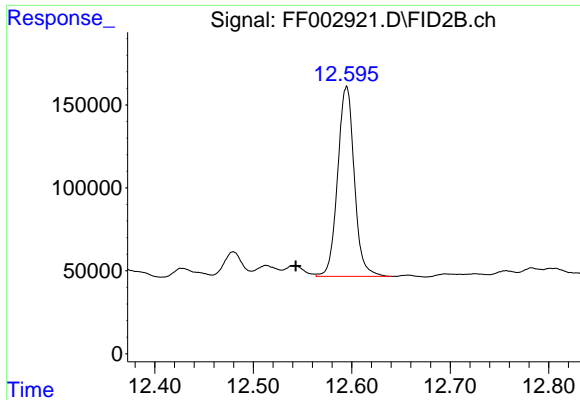


#7 N-EICOSANE
 R.T.: 12.595 min
 Delta R.T.: 0.052 min
 Response: 1344610
 Conc: 8.72 ug/ml


Instrument :
 FID_F
 ClientSampleId :

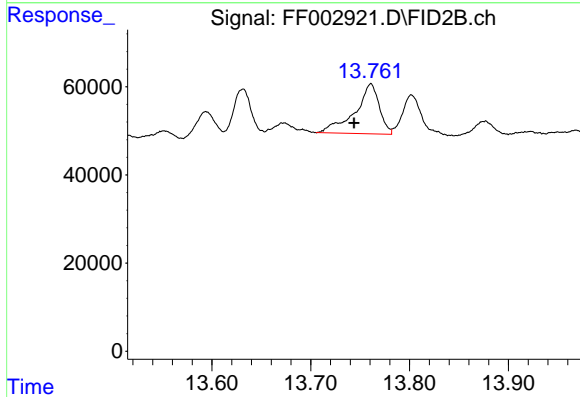


#8 N-DOCOSANE
 R.T.: 13.761 min
 Delta R.T.: 0.017 min
 Response: 193865
 Conc: 1.30 ug/ml

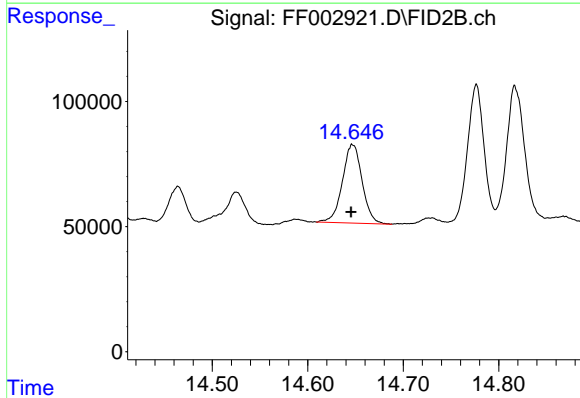

#9 TETRACOSANE-d50 (SURROGATE)
 R.T.: 14.647 min
 Delta R.T.: 0.002 min
 Response: 450723
 Conc: 3.47 ug/ml

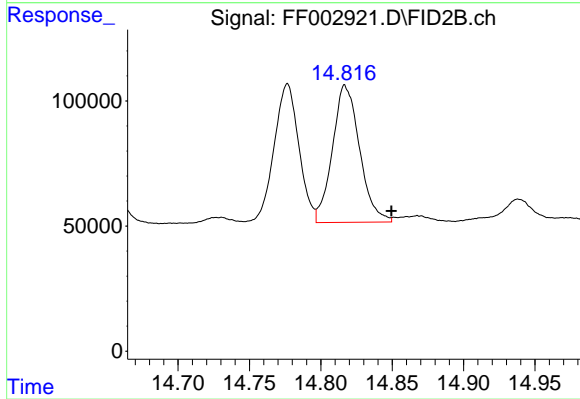


#10 N-TETRACOSANE
 R.T.: 14.817 min
 Delta R.T.: -0.033 min
 Response: 726001
 Conc: 5.02 ug/ml

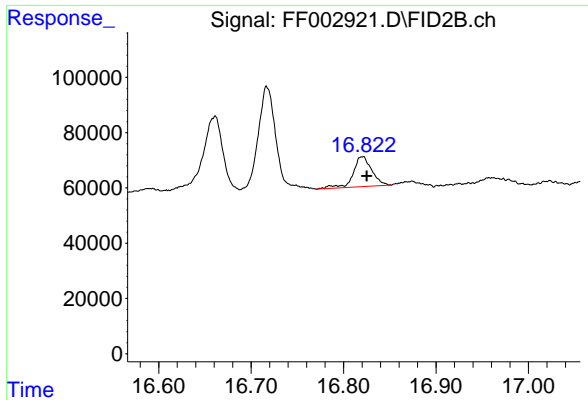


#12 N-OCTACOSANE
R.T.: 16.820 min
Delta R.T.: -0.005 min
Response: 152649
Conc: 1.14 ug/ml


Instrument :
FID_F
ClientSampleId :

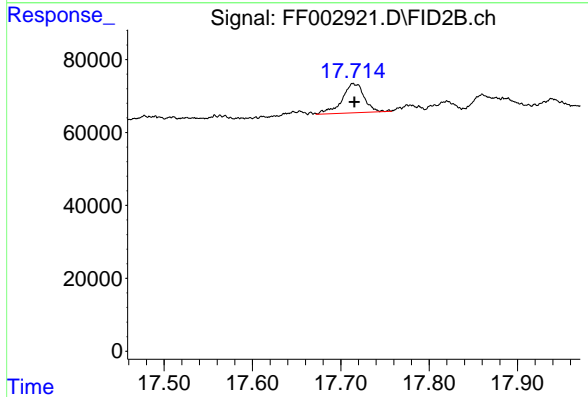

#13 N-TRIACONTANE
R.T.: 17.714 min
Delta R.T.: -0.002 min
Response: 140153
Conc: 1.09 ug/ml

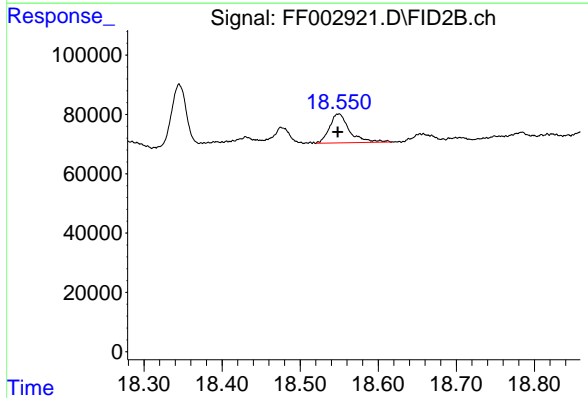

#14 N-DOTRIACONTANE
R.T.: 18.550 min
Delta R.T.: 0.001 min
Response: 174940
Conc: 1.46 ug/ml

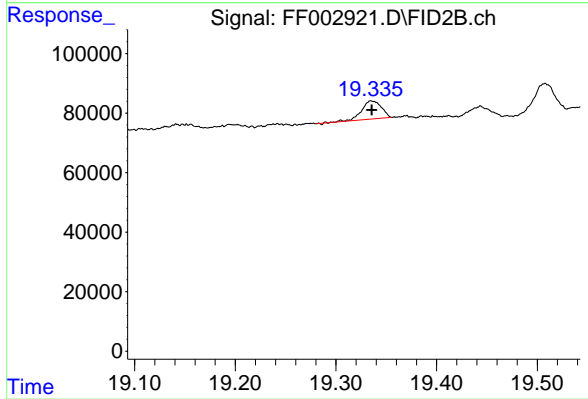

#15 N-TETRATRIACONTANE
R.T.: 19.335 min
Delta R.T.: 0.000 min
Response: 82225
Conc: 0.73 ug/ml