

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
 Data File : FF002923.D
 Signal(s) : FID2B.ch
 Acq On : 06 Dec 2018 01:26
 Operator : AJ\SJ
 Sample : J6210-07 5X
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 03:08:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	294007	2.265 ug/ml
Target Compounds			
1) N-OCTANE	2.242	49219	0.318 ug/ml
4) N-TETRADECANE	8.242f	95389	0.595 ug/ml
7) N-EICOSANE	12.593	129120	0.837 ug/ml
10) N-TETRACOSANE	14.820	208201	1.441 ug/ml
12) N-OCTACOSANE	16.874	126301	0.943 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120518\
Data File : FF002923.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2018 01:26
Operator : AJ\SJ
Sample : J6210-07 5X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 03:08:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

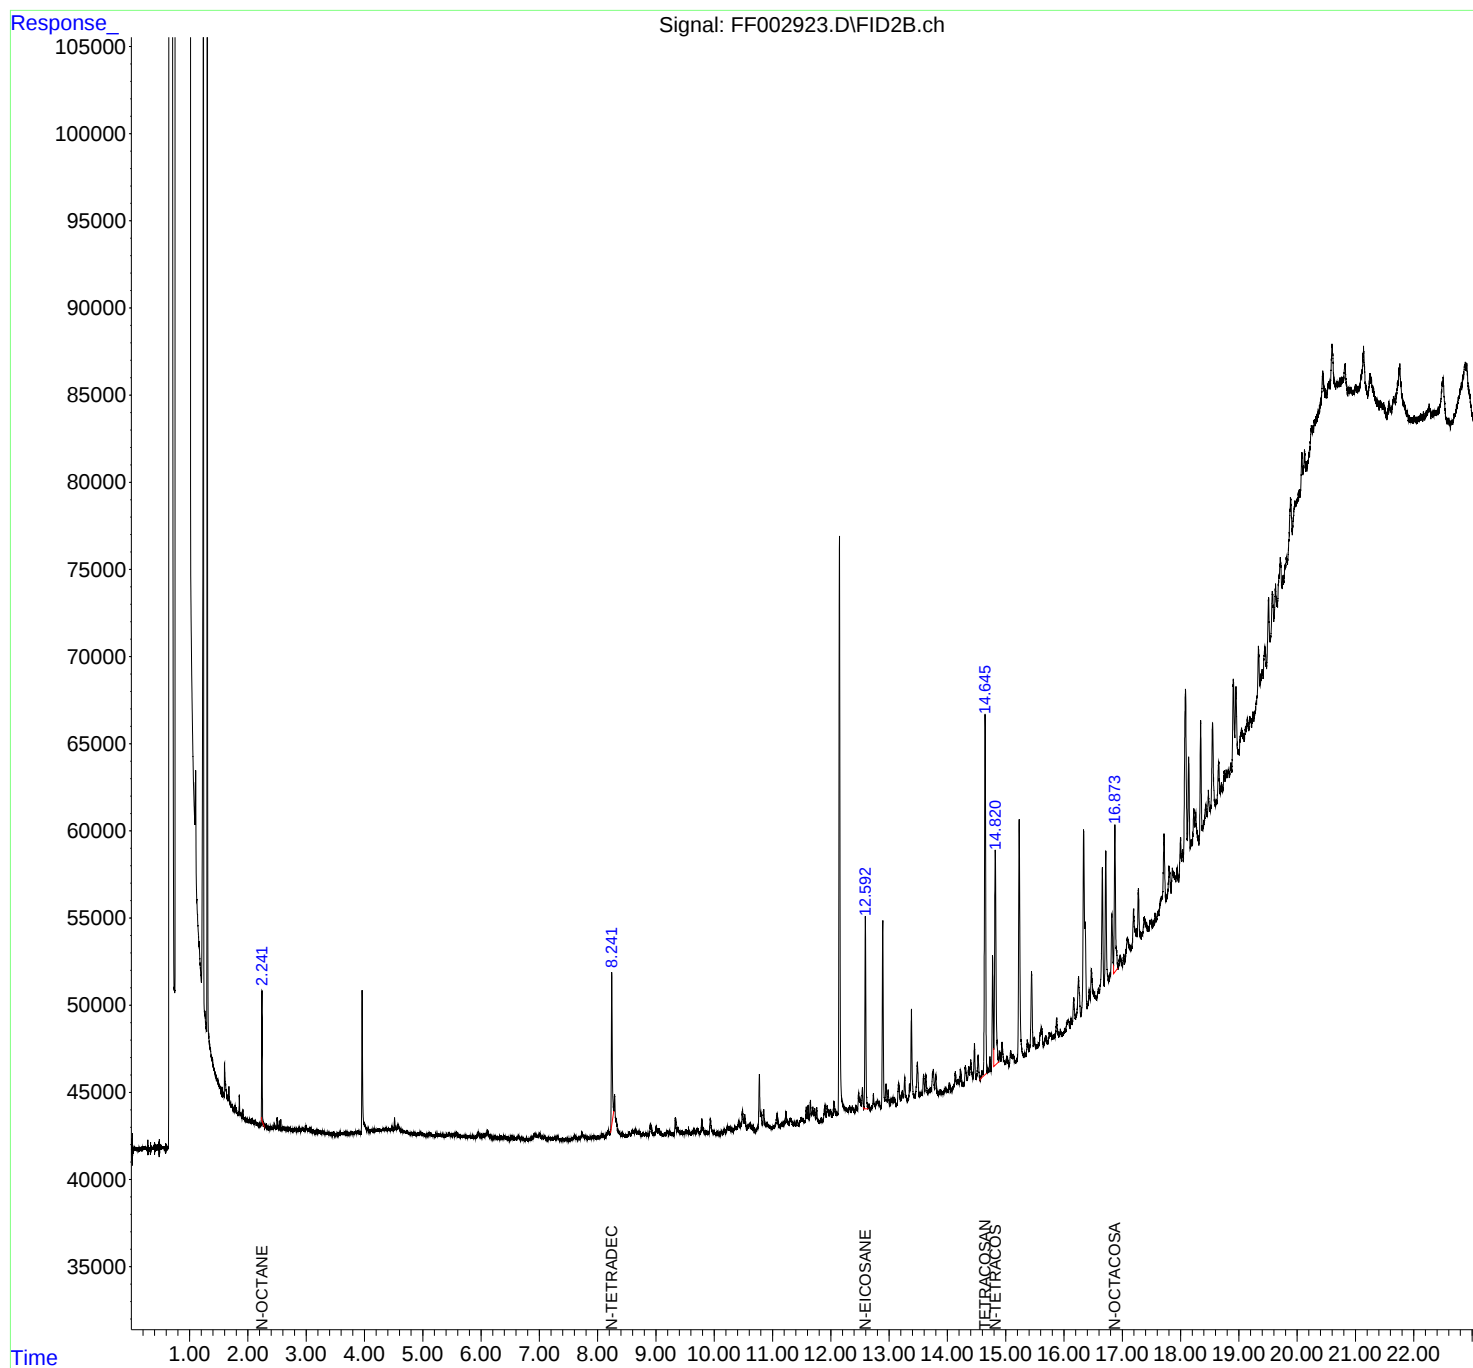


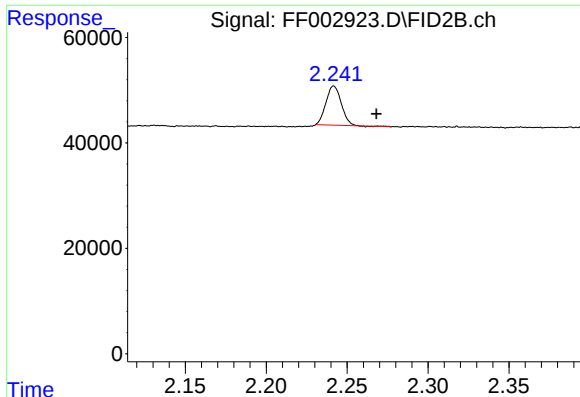

#1 N-OCTANE


R.T.: 2.242 min
Delta R.T.: -0.026 min
Response: 49219
Conc: 0.32 ug/ml

Instrument :
FID_F
ClientSampleId :

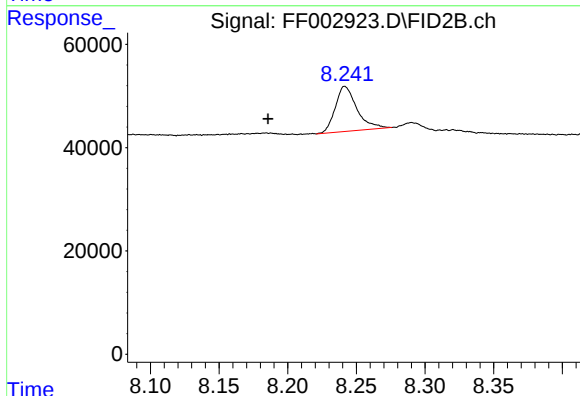


#4 N-TETRADECANE

R.T.: 8.242 min
Delta R.T.: 0.056 min
Response: 95389
Conc: 0.60 ug/ml

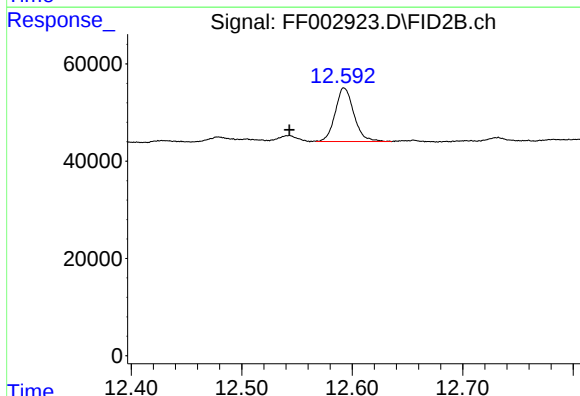


#7 N-EICOSANE

R.T.: 12.593 min
Delta R.T.: 0.050 min
Response: 129120
Conc: 0.84 ug/ml

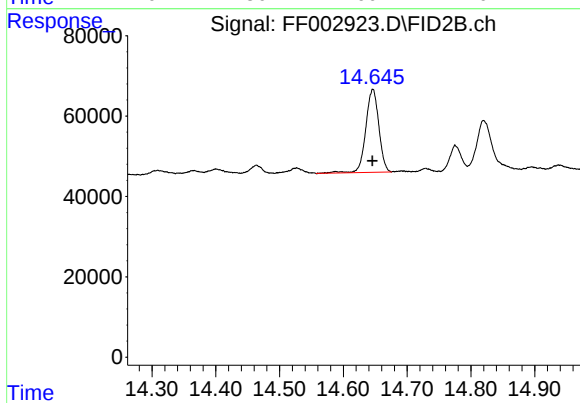

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.646 min
Delta R.T.: 0.001 min
Response: 294007
Conc: 2.26 ug/ml

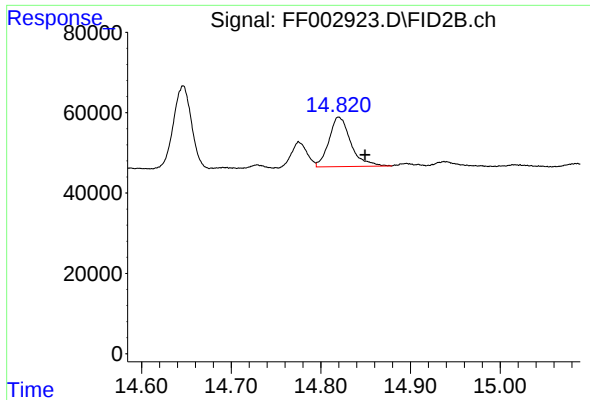

#10 N-TETRACOSANE

R.T.: 14.820 min
Delta R.T.: -0.030 min
Response: 208201
Conc: 1.44 ug/ml

Instrument :
FID_F
ClientSampleId :

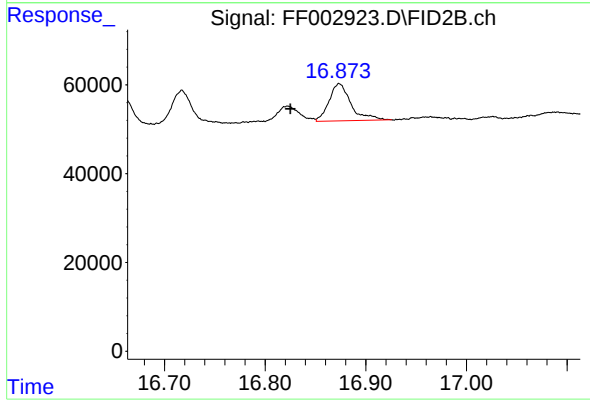

#12 N-OCTACOSANE

R.T.: 16.874 min
Delta R.T.: 0.049 min
Response: 126301
Conc: 0.94 ug/ml