

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120519\
Data File : FF006004.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2019 11:14
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 05 13:06:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.422	2890260	22.208 ug/ml
12)	N-OCTACOSANE	16.821	2678143	21.655 ug/ml
13)	N-TRIACONTANE	17.704	180133	1.484 ug/ml
14)	N-DOTRIACONTANE	18.536	175289	1.531 ug/ml
15)	N-TETRATRIACONTANE	19.319	85627	0.796 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120519\
Data File : FF006004.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2019 11:14
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 05 13:06:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

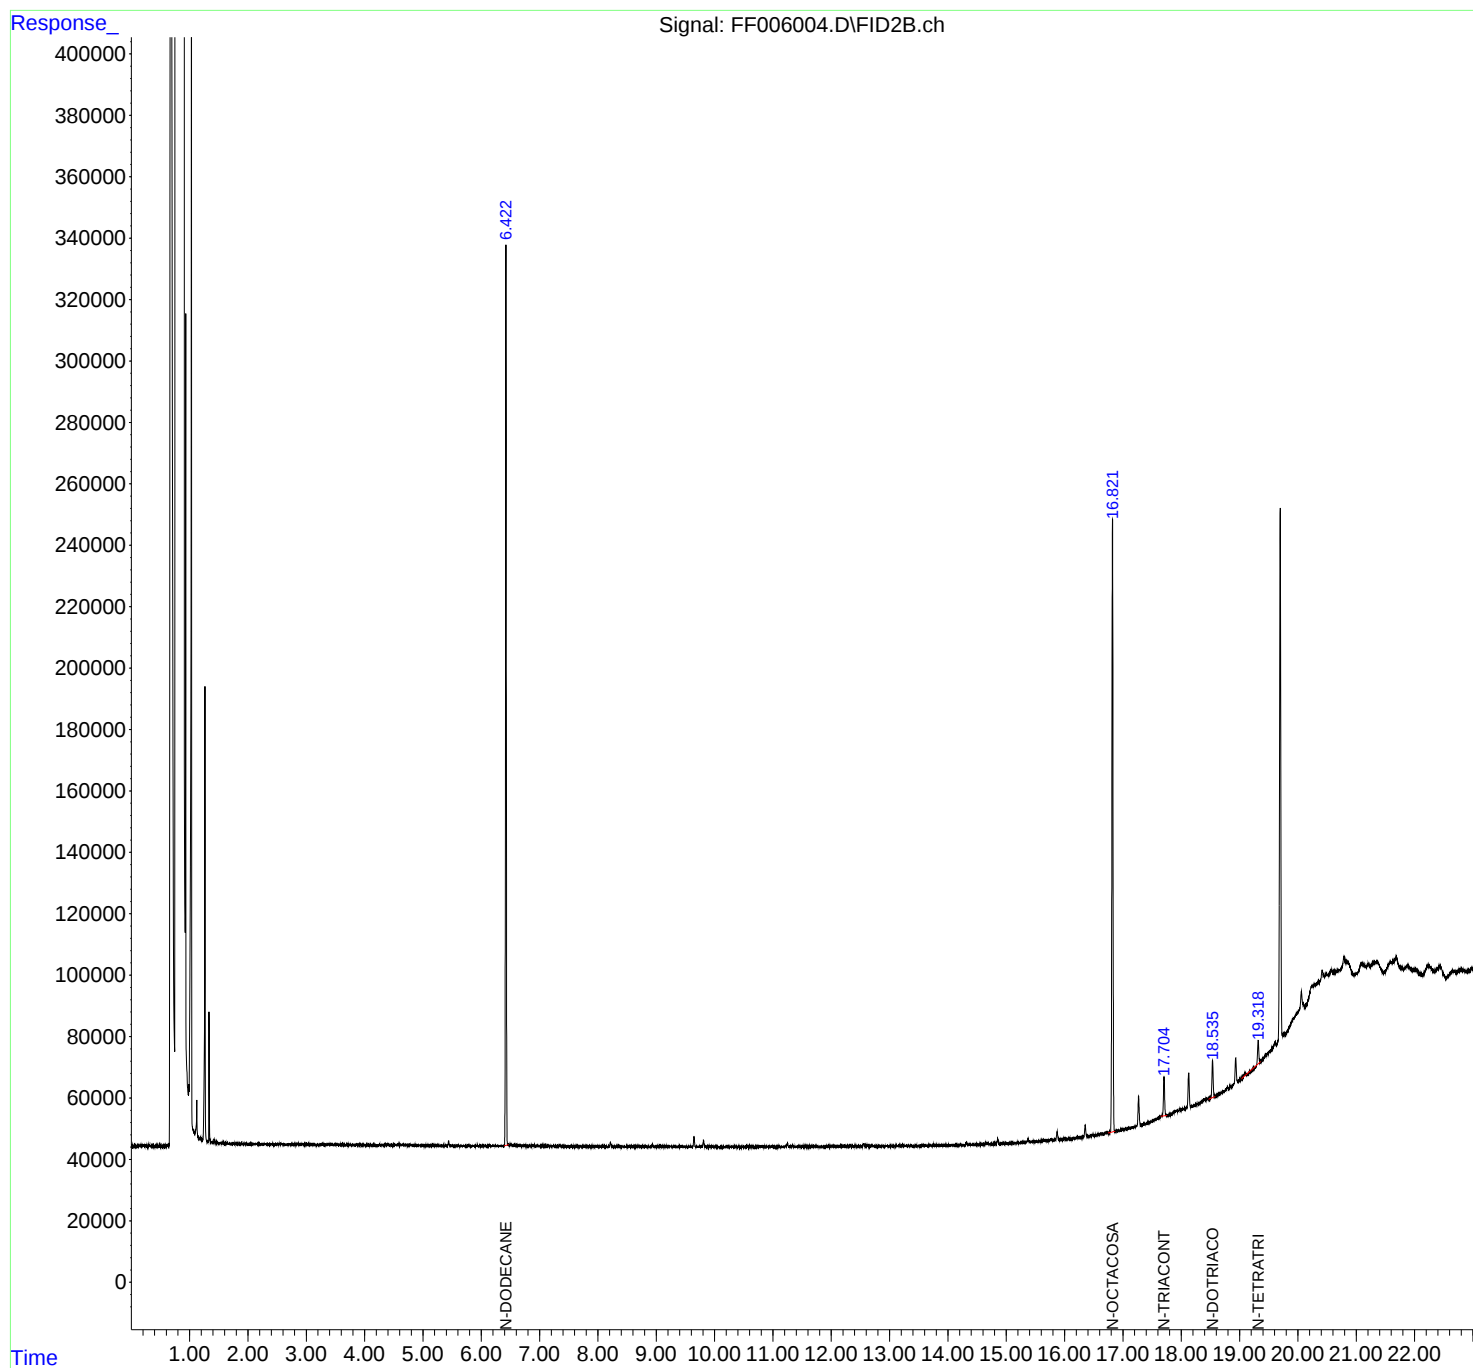


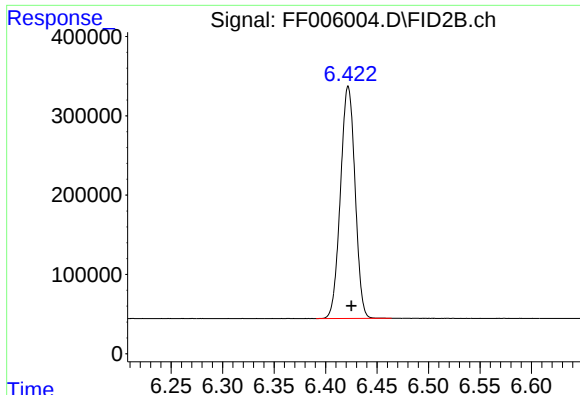

#3 N-DODECANE


R.T.: 6.422 min
Delta R.T.: -0.003 min
Response: 2890260
Conc: 22.21 ug/ml

Instrument :
FID_F
ClientSampleId :

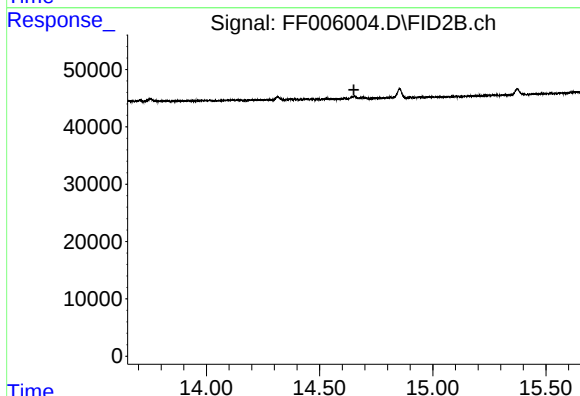


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.651 min
Response: 0
Conc: N.D.

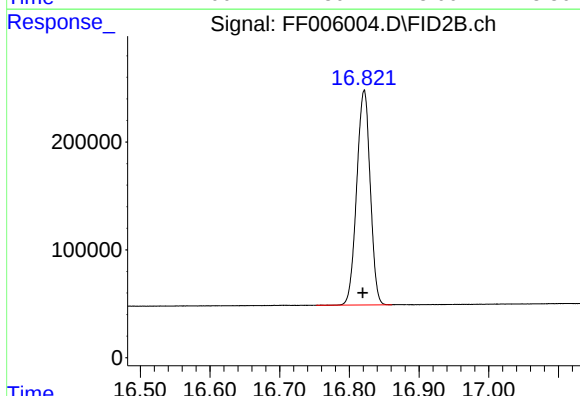


#12 N-OCTACOSANE

R.T.: 16.821 min
Delta R.T.: 0.002 min
Response: 2678143
Conc: 21.66 ug/ml

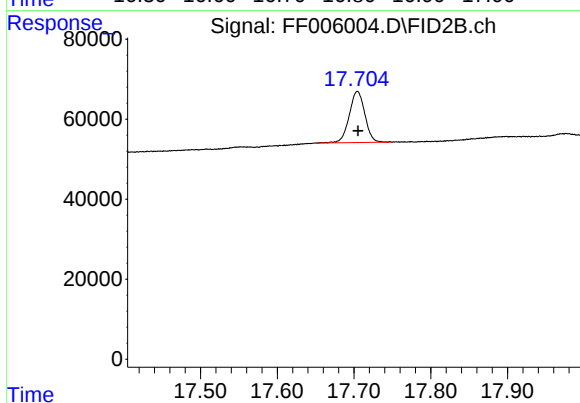

#13 N-TRIACONTANE


R.T.: 17.704 min
Delta R.T.: 0.000 min
Response: 180133
Conc: 1.48 ug/ml

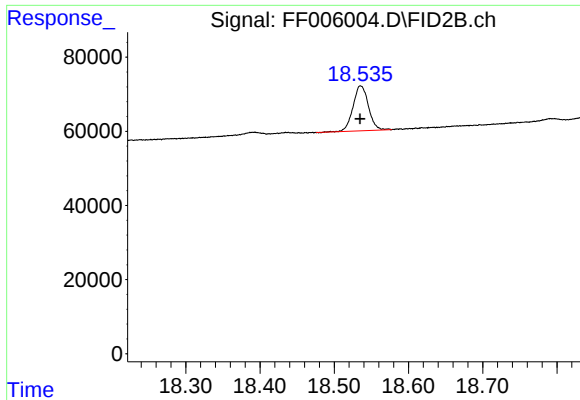

#14 N-DOTRIACONTANE

R.T.: 18.536 min
Delta R.T.: 0.000 min
Response: 175289
Conc: 1.53 ug/ml

Instrument :
FID_F
ClientSampleId :

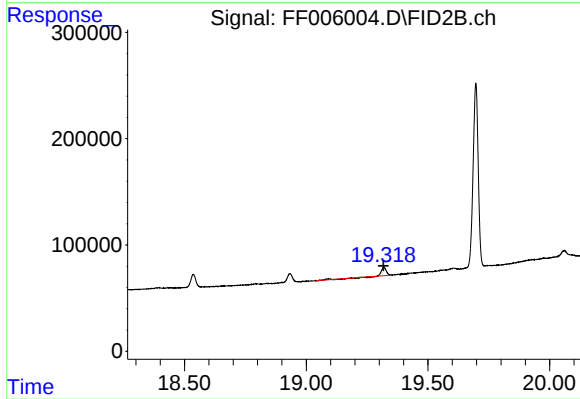

#15 N-TETRATRIACONTANE

R.T.: 19.319 min
Delta R.T.: 0.002 min
Response: 85627
Conc: 0.80 ug/ml