

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120519\
Data File : FF006005.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2019 11:44
Operator : DD\AJ
Sample : K6119-05 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-4-(0-2)

Integration File: autoint1.e
Quant Time: Dec 05 13:06:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.651	801099	7.128 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120519\
Data File : FF006005.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2019 11:44
Operator : DD\AJ
Sample : K6119-05 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-4-(0-2)

Integration File: autoint1.e
Quant Time: Dec 05 13:06:20 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

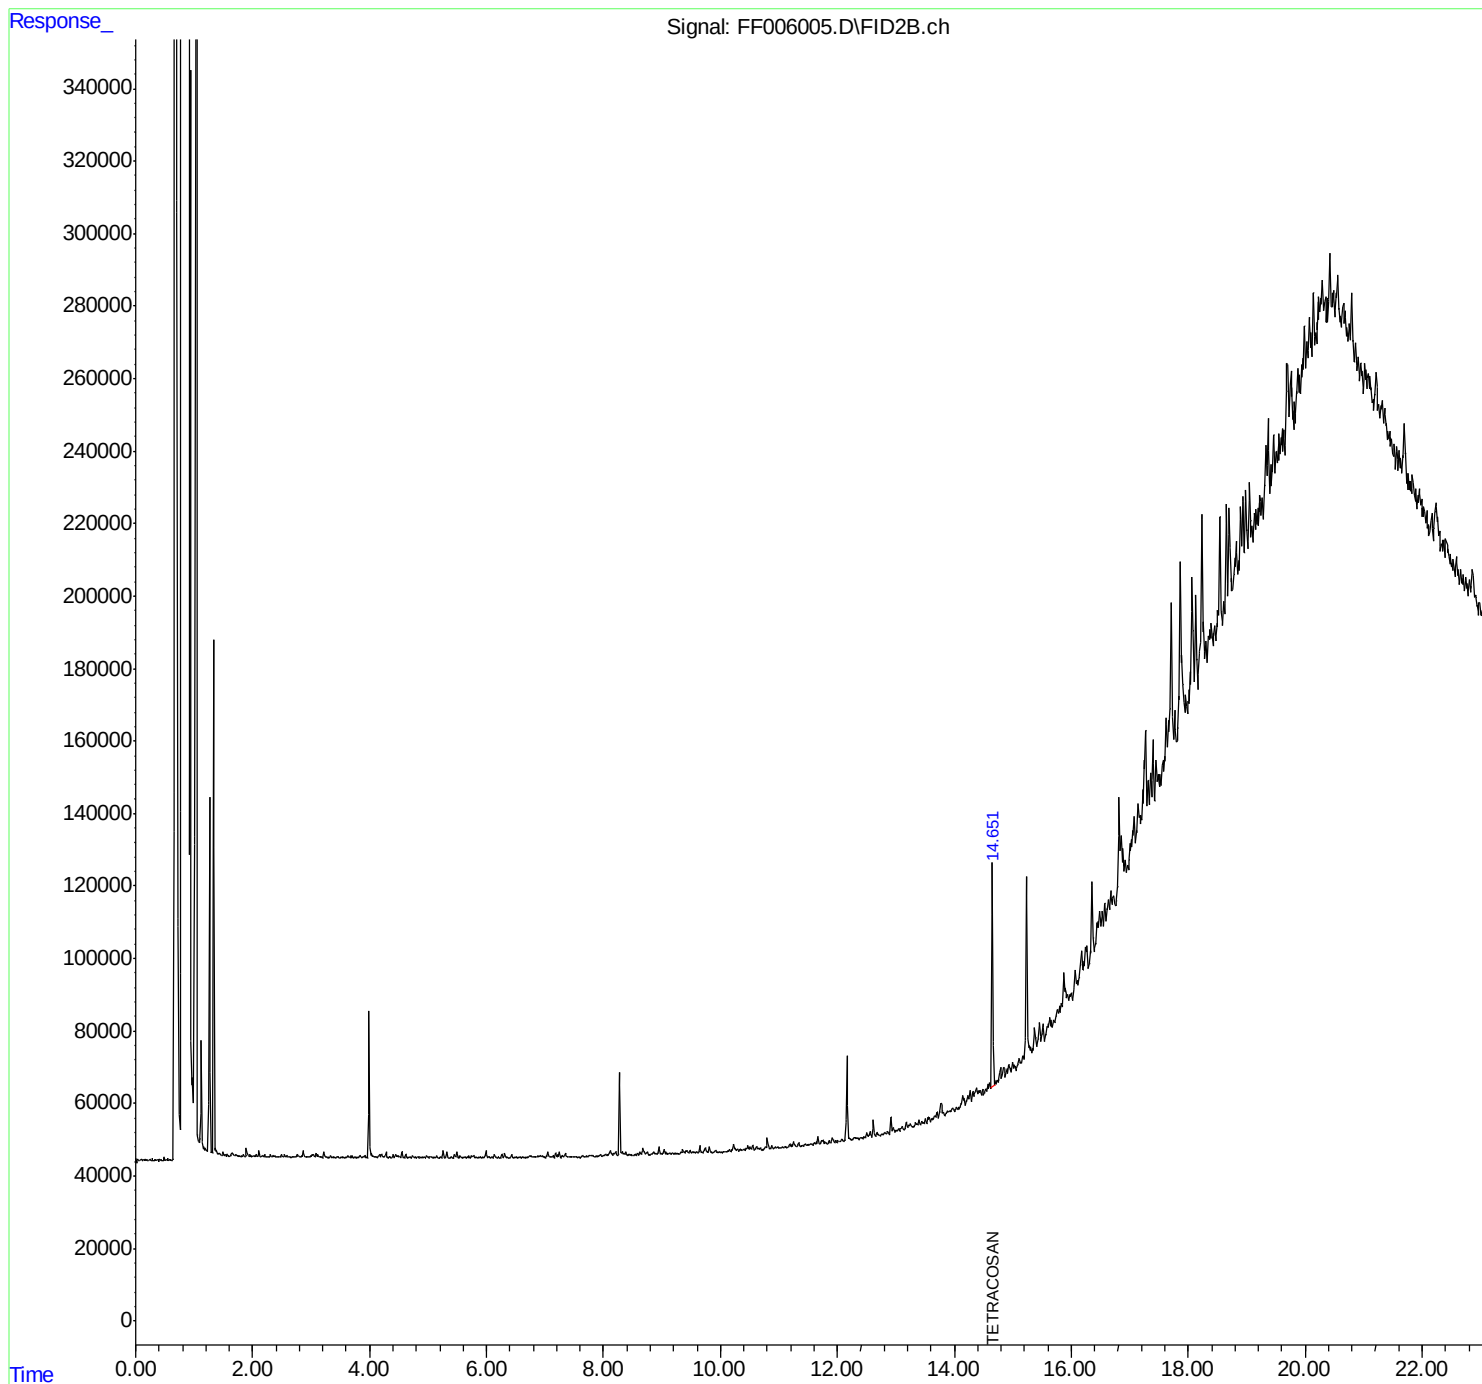

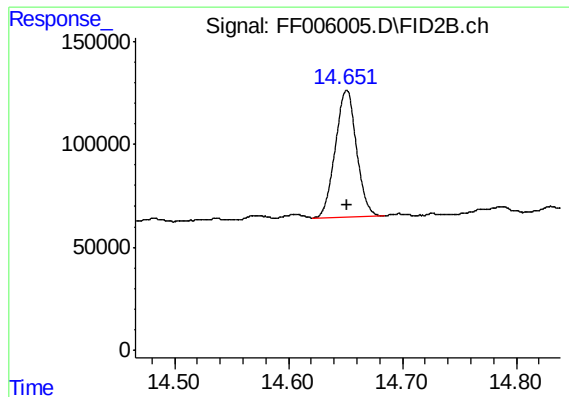

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.651 min
Delta R.T.: 0.000 min
Response: 801099
Conc: 7.13 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-4-(0-2)