

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120522\
Data File : FF011762.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2022 16:36
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 04:25:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.955	32832	0.273 ug/ml
15)	N-TETRATRIACONTANE	19.735	21883	0.185 ug/ml
16)	N-HEXATRIACONTANE	20.481	61511	0.529 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120522\
Data File : FF011762.D
Signal(s) : FID2B.ch
Acq On : 05 Dec 2022 16:36
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 04:25:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

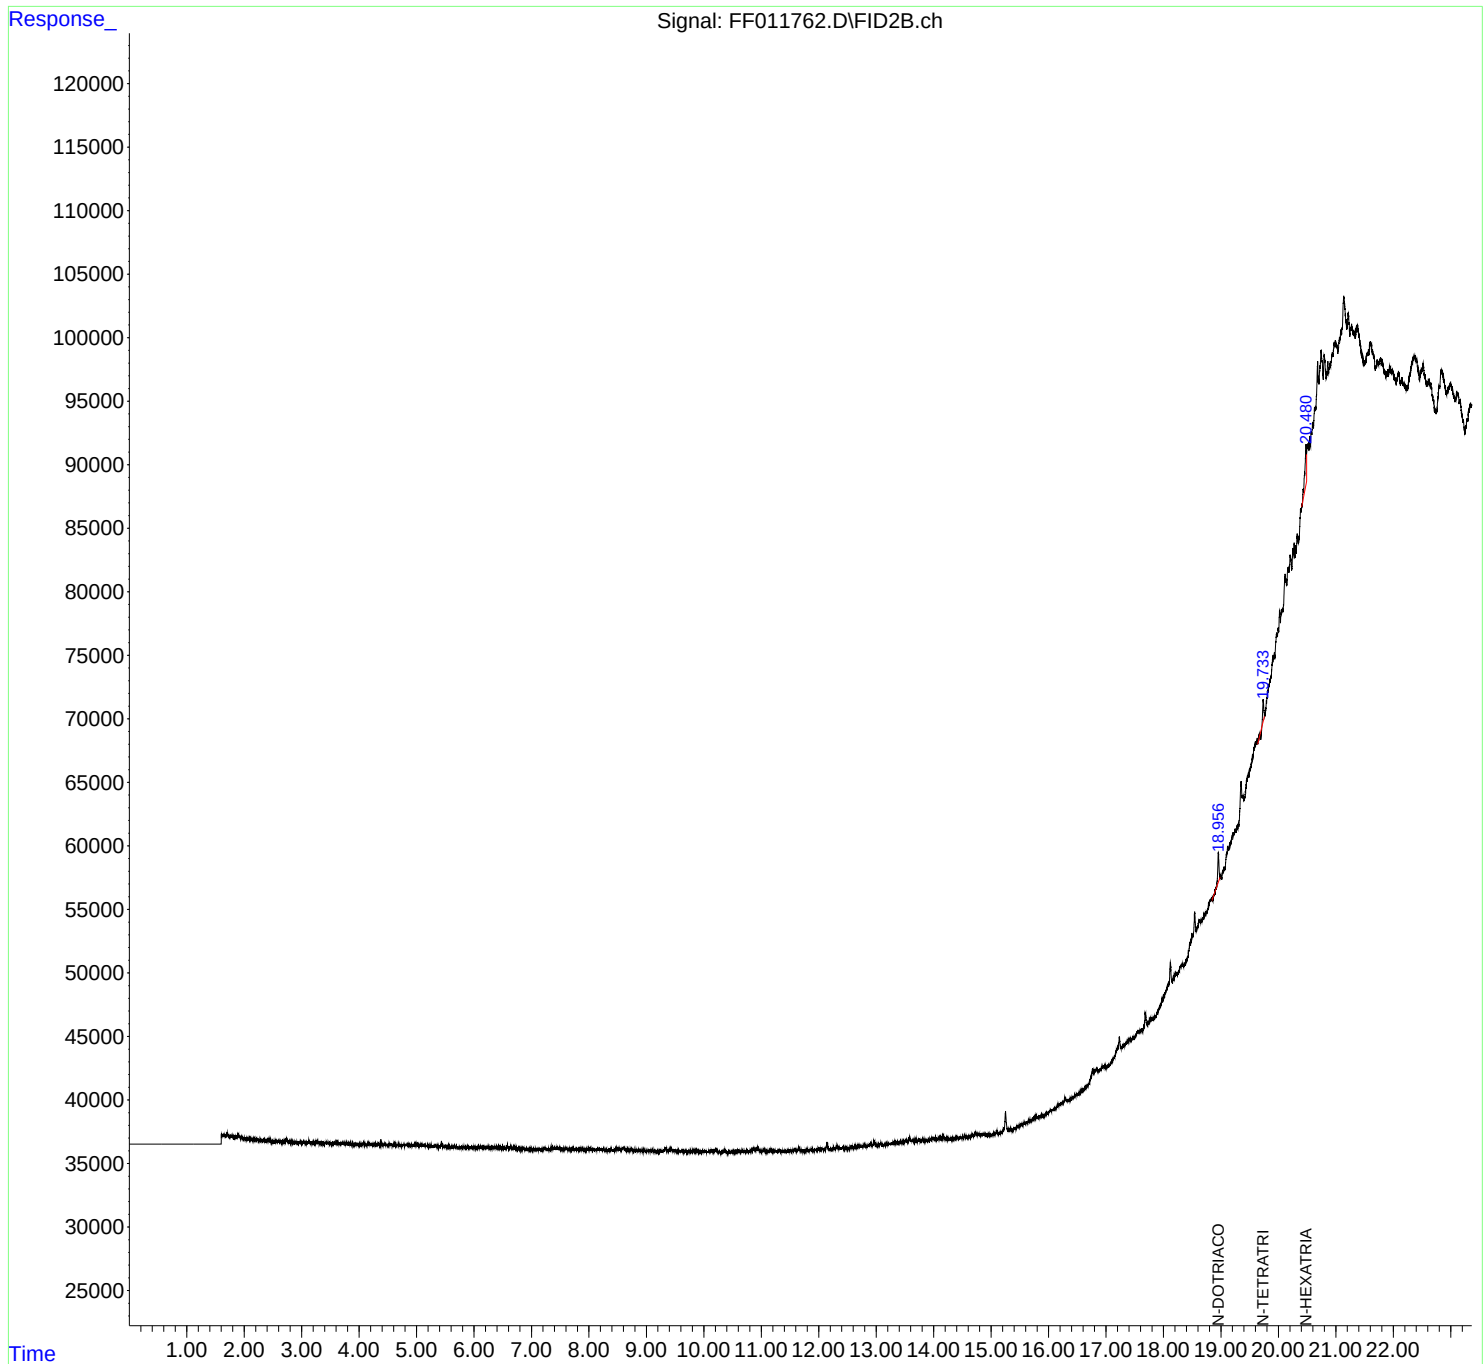


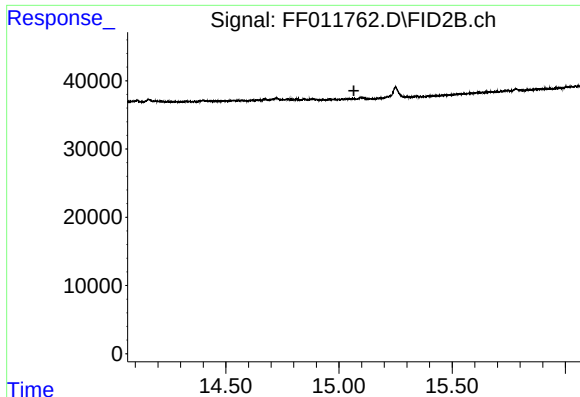

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.066 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

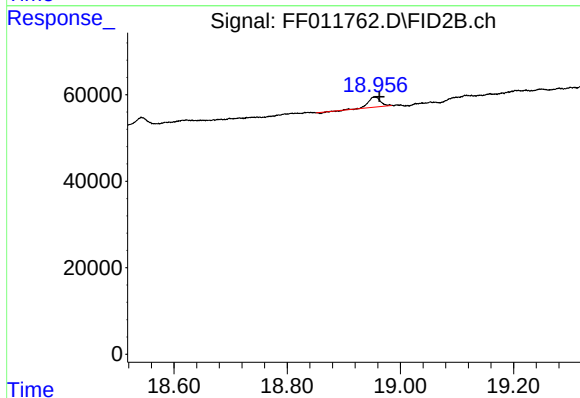


#14 N-DOTRIACONTANE

R.T.: 18.955 min
Delta R.T.: -0.008 min
Response: 32832
Conc: 0.27 ug/ml

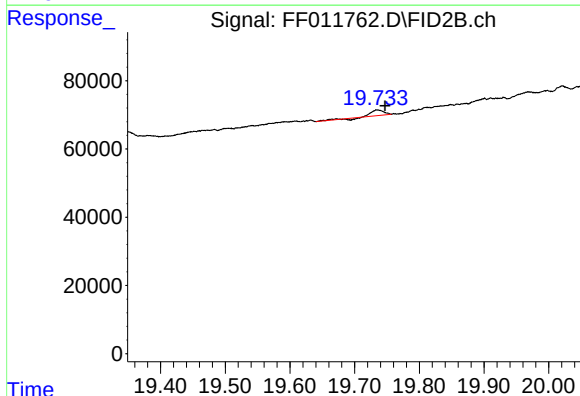

#15 N-TETRATRIACONTANE

R.T.: 19.735 min
Delta R.T.: -0.012 min
Response: 21883
Conc: 0.18 ug/ml

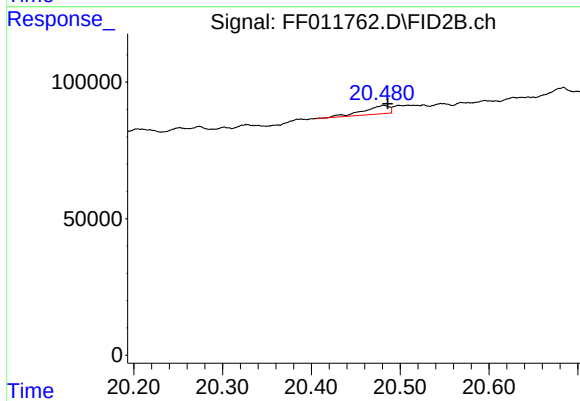

#16 N-HEXATRIACONTANE

R.T.: 20.481 min
Delta R.T.: -0.005 min
Response: 61511
Conc: 0.53 ug/ml