

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120624\
 Data File : FF015139.D
 Signal(s) : FID2B.ch
 Acq On : 06 Dec 2024 11:18
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 06 23:06:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
 Quant Title :
 QLast Update : Thu Nov 21 01:46:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.729	2816089	21.615 ug/ml
12) N-OCTACOSANE	17.184	2167808	18.599 ug/ml
13) N-TRIACONTANE	18.071	104380	0.900 ug/ml
14) N-DOTRIACONTANE	18.902	122247	1.087 ug/ml
15) N-TETRATRIACONTANE	19.687	102963	1.058 ug/ml
16) N-HEXATRIACONTANE	20.428	77186	0.988 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120624\
Data File : FF015139.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2024 11:18
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 06 23:06:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
Quant Title :
QLast Update : Thu Nov 21 01:46:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

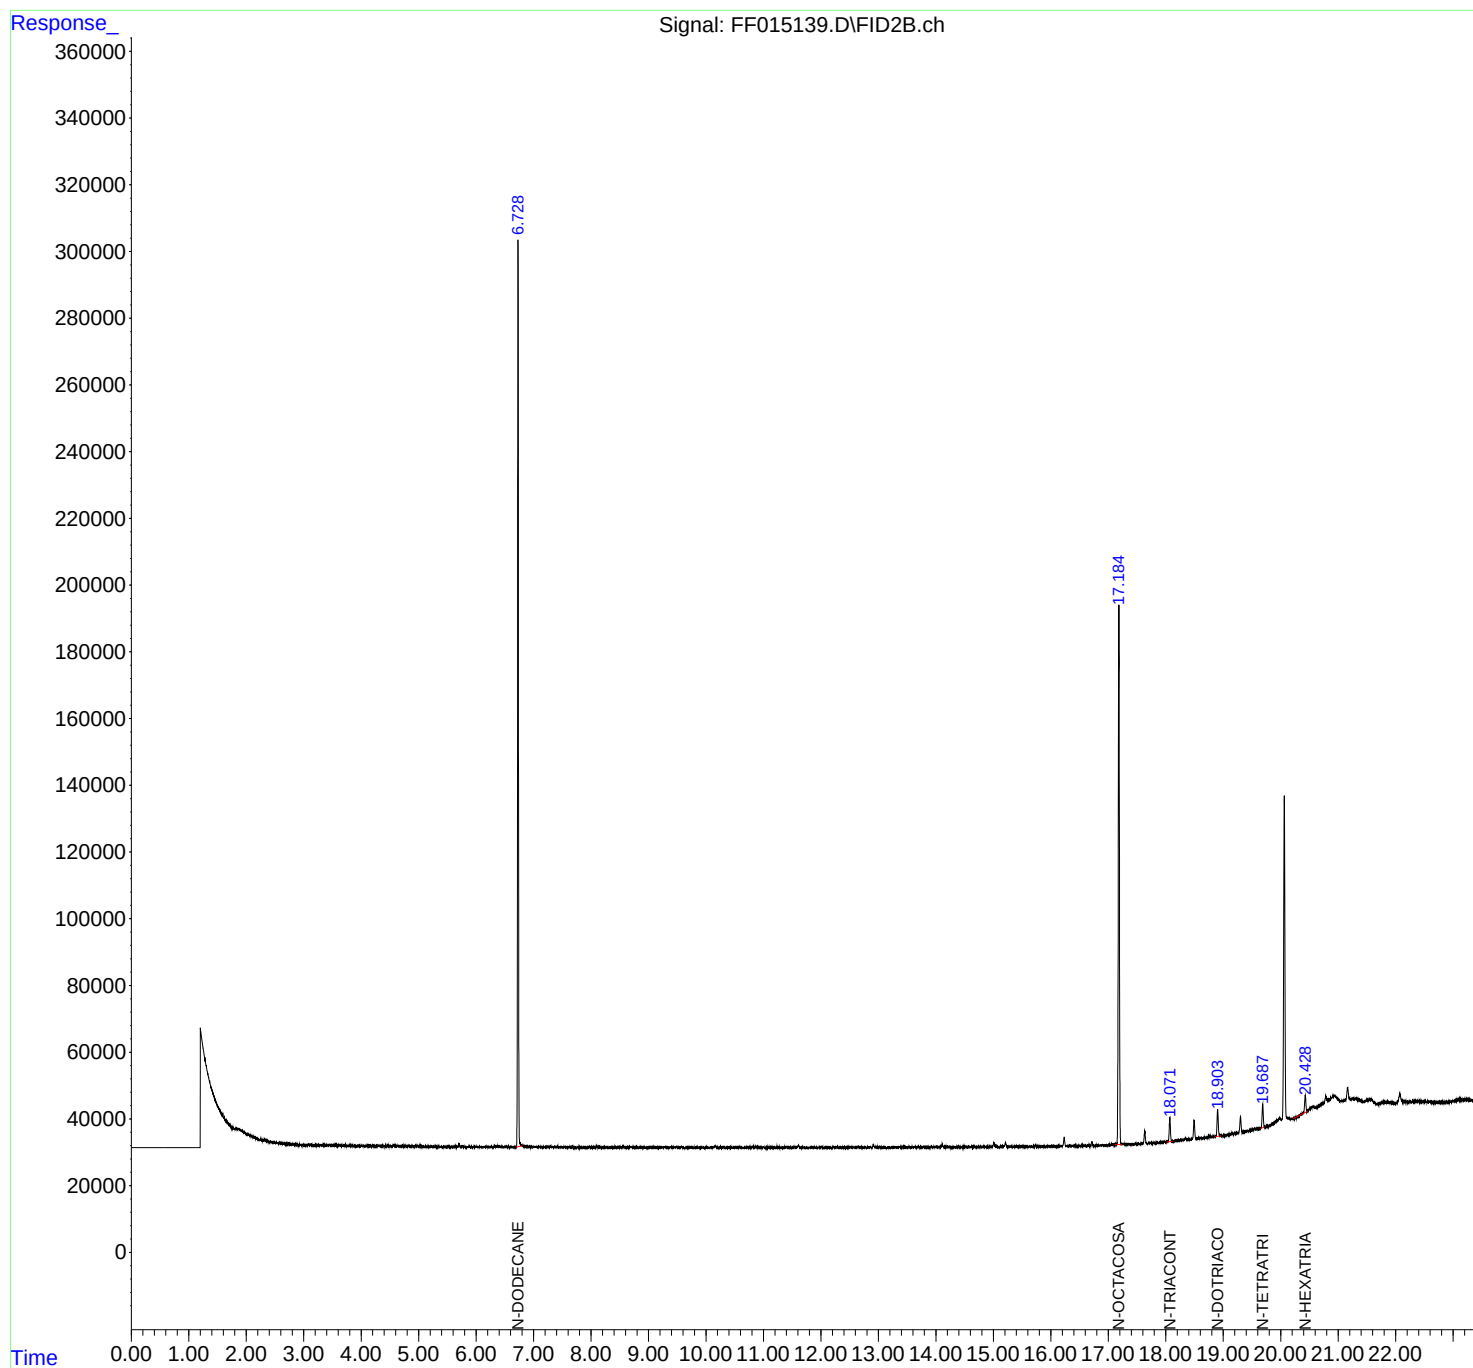


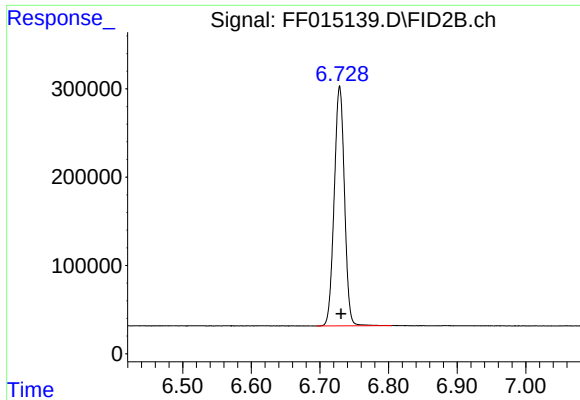

#3 N-DODECANE


R.T.: 6.729 min
Delta R.T.: -0.002 min
Response: 2816089
Conc: 21.62 ug/ml

Instrument :
FID_F
ClientSampleId :

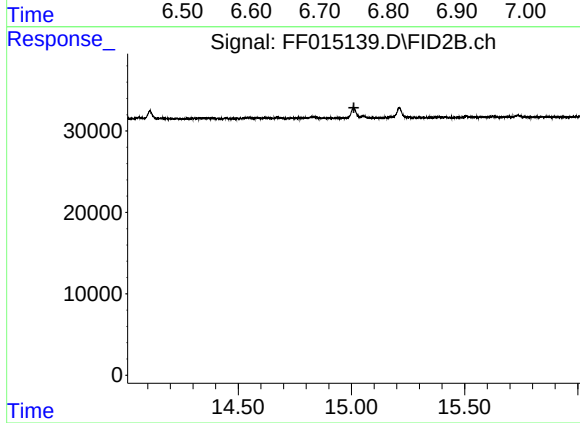


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.011 min
Response: 0
Conc: N.D.

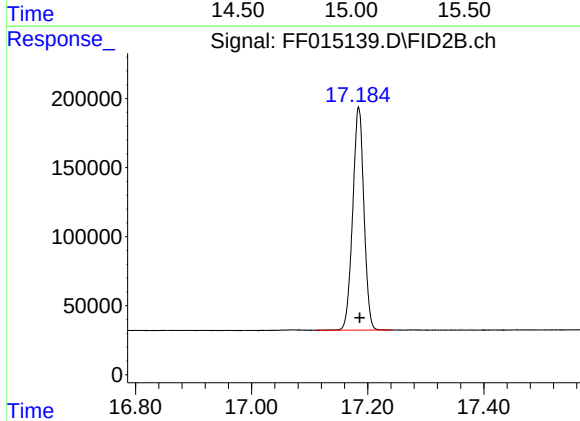


#12 N-OCTACOSANE

R.T.: 17.184 min
Delta R.T.: -0.001 min
Response: 2167808
Conc: 18.60 ug/ml

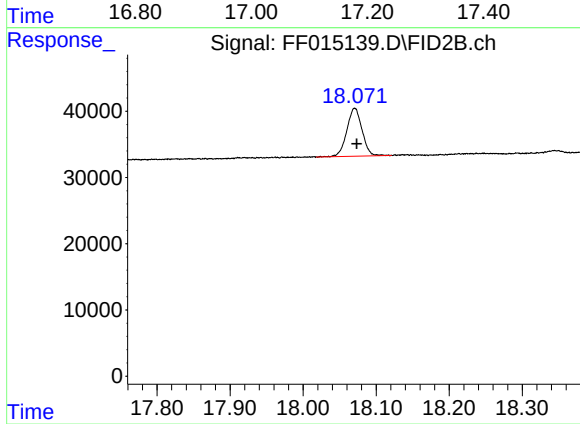

#13 N-TRIACONTANE


R.T.: 18.071 min
Delta R.T.: -0.003 min
Response: 104380
Conc: 0.90 ug/ml

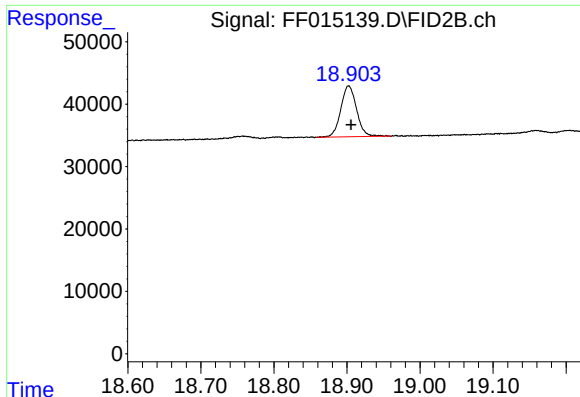

#14 N-DOTRIACONTANE


R.T.: 18.902 min
Delta R.T.: -0.003 min
Response: 122247
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :

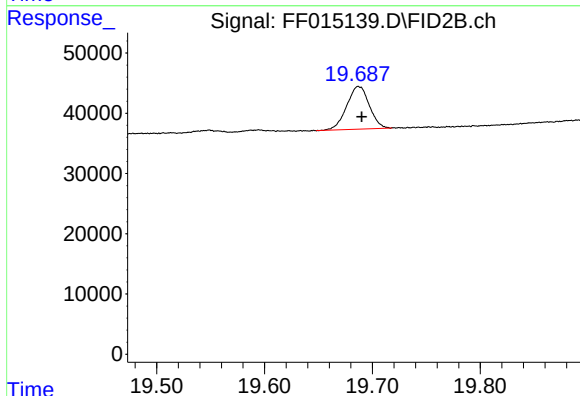

#15 N-TETRATRIACONTANE

R.T.: 19.687 min
Delta R.T.: -0.003 min
Response: 102963
Conc: 1.06 ug/ml

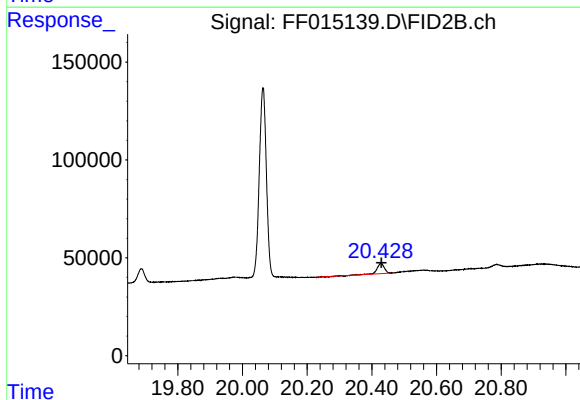

#16 N-HEXATRIACONTANE

R.T.: 20.428 min
Delta R.T.: -0.001 min
Response: 77186
Conc: 0.99 ug/ml