

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120624\  
Data File : FF015146.D  
Signal(s) : FID2B.ch  
Acq On : 06 Dec 2024 16:34  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 06 23:09:29 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF112124.M  
Quant Title :  
QLast Update : Thu Nov 21 01:46:50 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.010 | 2007656  | 18.165 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.905 | 123430   | 1.097 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.693 | 218953   | 2.250 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.433 | 145355   | 1.860 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120624\  
Data File : FF015146.D  
Signal(s) : FID2B.ch  
Acq On : 06 Dec 2024 16:34  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 06 23:09:29 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF112124.M  
Quant Title :  
QLast Update : Thu Nov 21 01:46:50 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

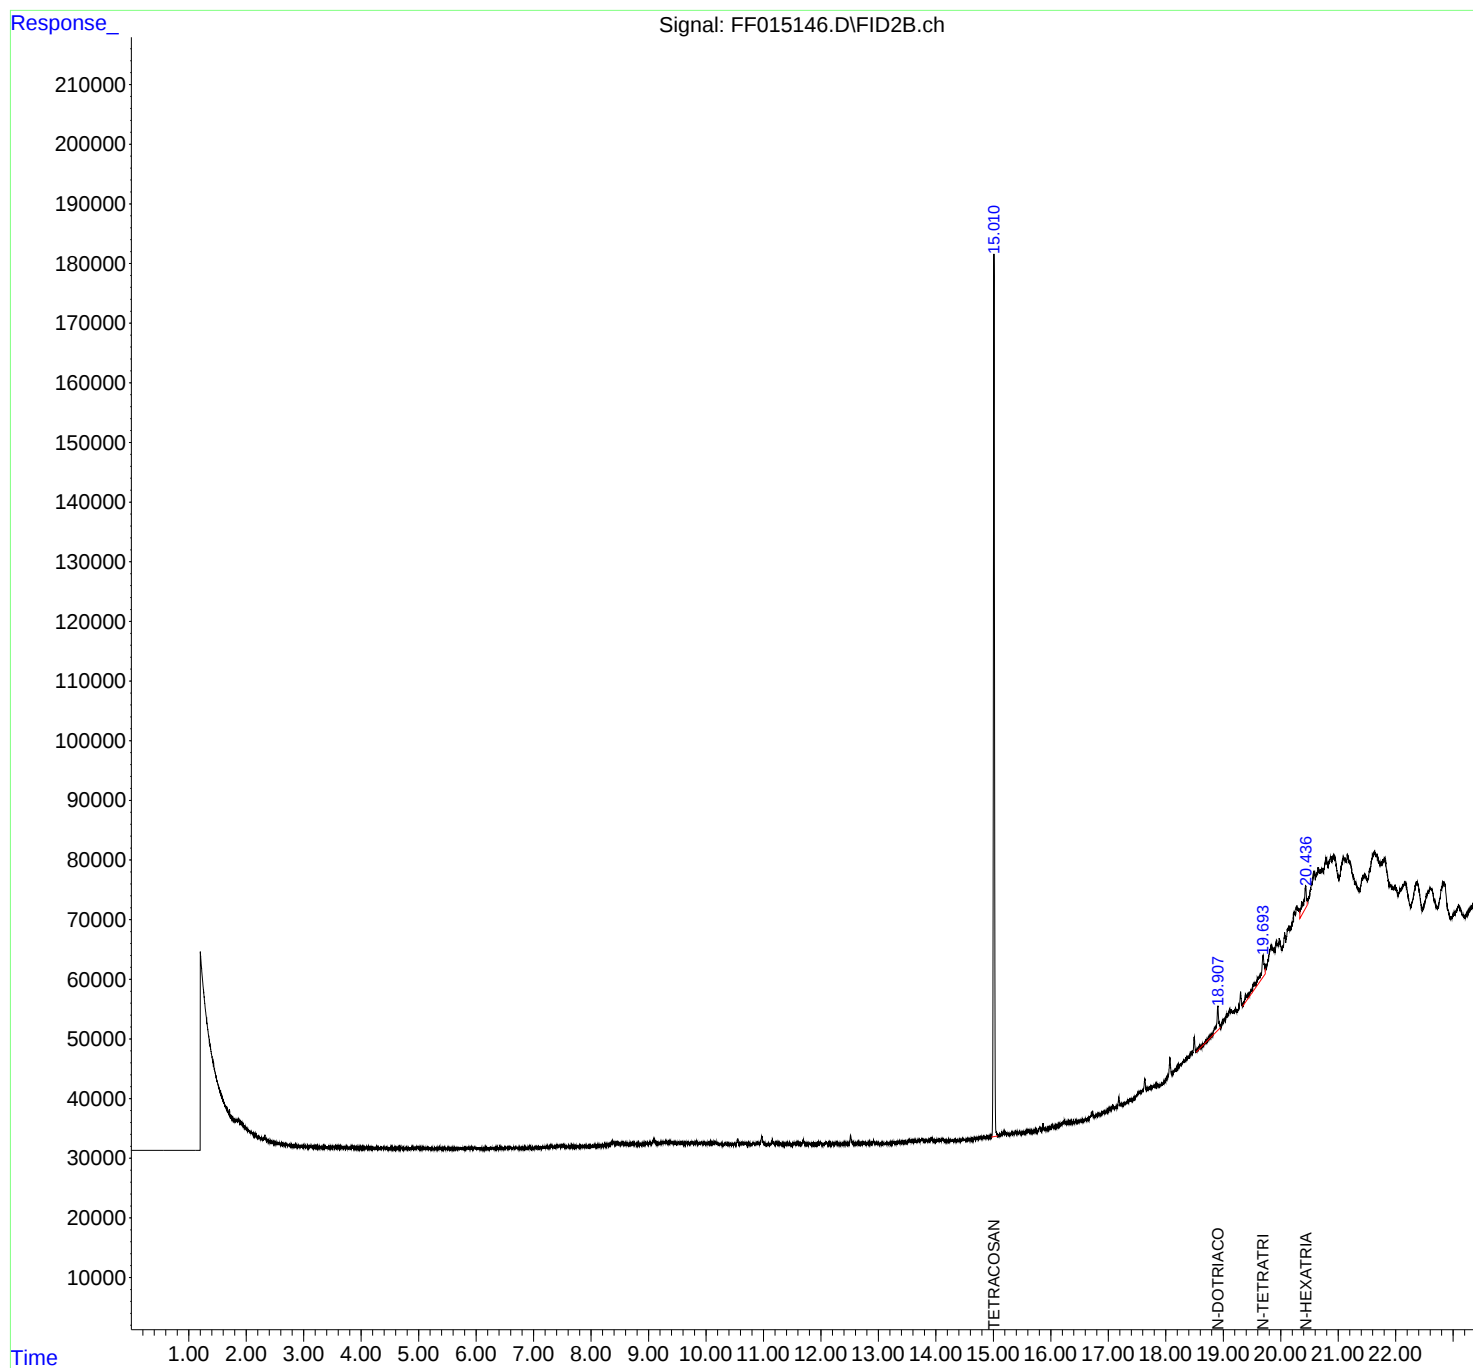


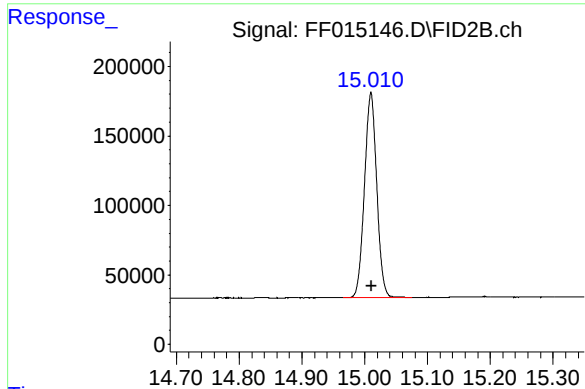

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.010 min  
Delta R.T.: 0.000 min  
Response: 2007656  
Conc: 18.16 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

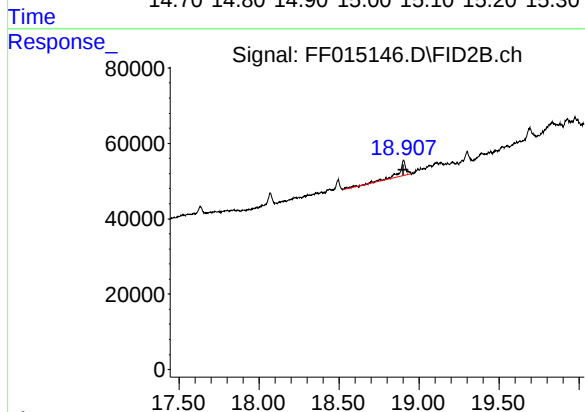


#14 N-DOTRIACONTANE

R.T.: 18.905 min  
Delta R.T.: 0.000 min  
Response: 123430  
Conc: 1.10 ug/ml

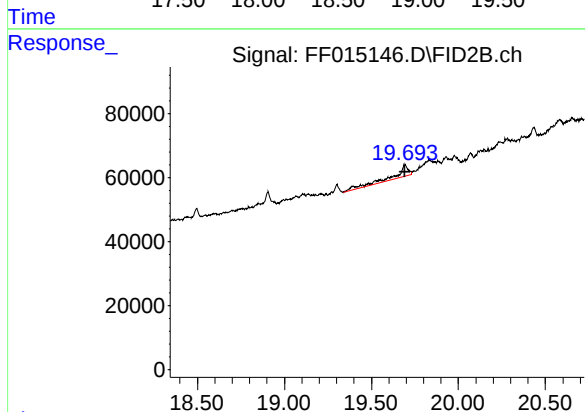

#15 N-TETRATRIACONTANE

R.T.: 19.693 min  
Delta R.T.: 0.003 min  
Response: 218953  
Conc: 2.25 ug/ml

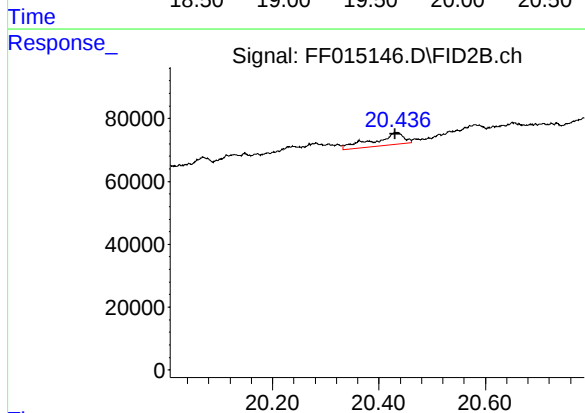

#16 N-HEXATRIACONTANE

R.T.: 20.433 min  
Delta R.T.: 0.004 min  
Response: 145355  
Conc: 1.86 ug/ml