

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120624\
Data File : FF015140.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2024 13:44
Operator : YP\AJ
Sample : PB165425BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB165425BL

Integration File: autoint1.e
Quant Time: Dec 06 23:06:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
Quant Title :
QLast Update : Thu Nov 21 01:46:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.008	1683520	15.232 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120624\
Data File : FF015140.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2024 13:44
Operator : YP\AJ
Sample : PB165425BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB165425BL

Integration File: autoint1.e
Quant Time: Dec 06 23:06:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
Quant Title :
QLast Update : Thu Nov 21 01:46:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

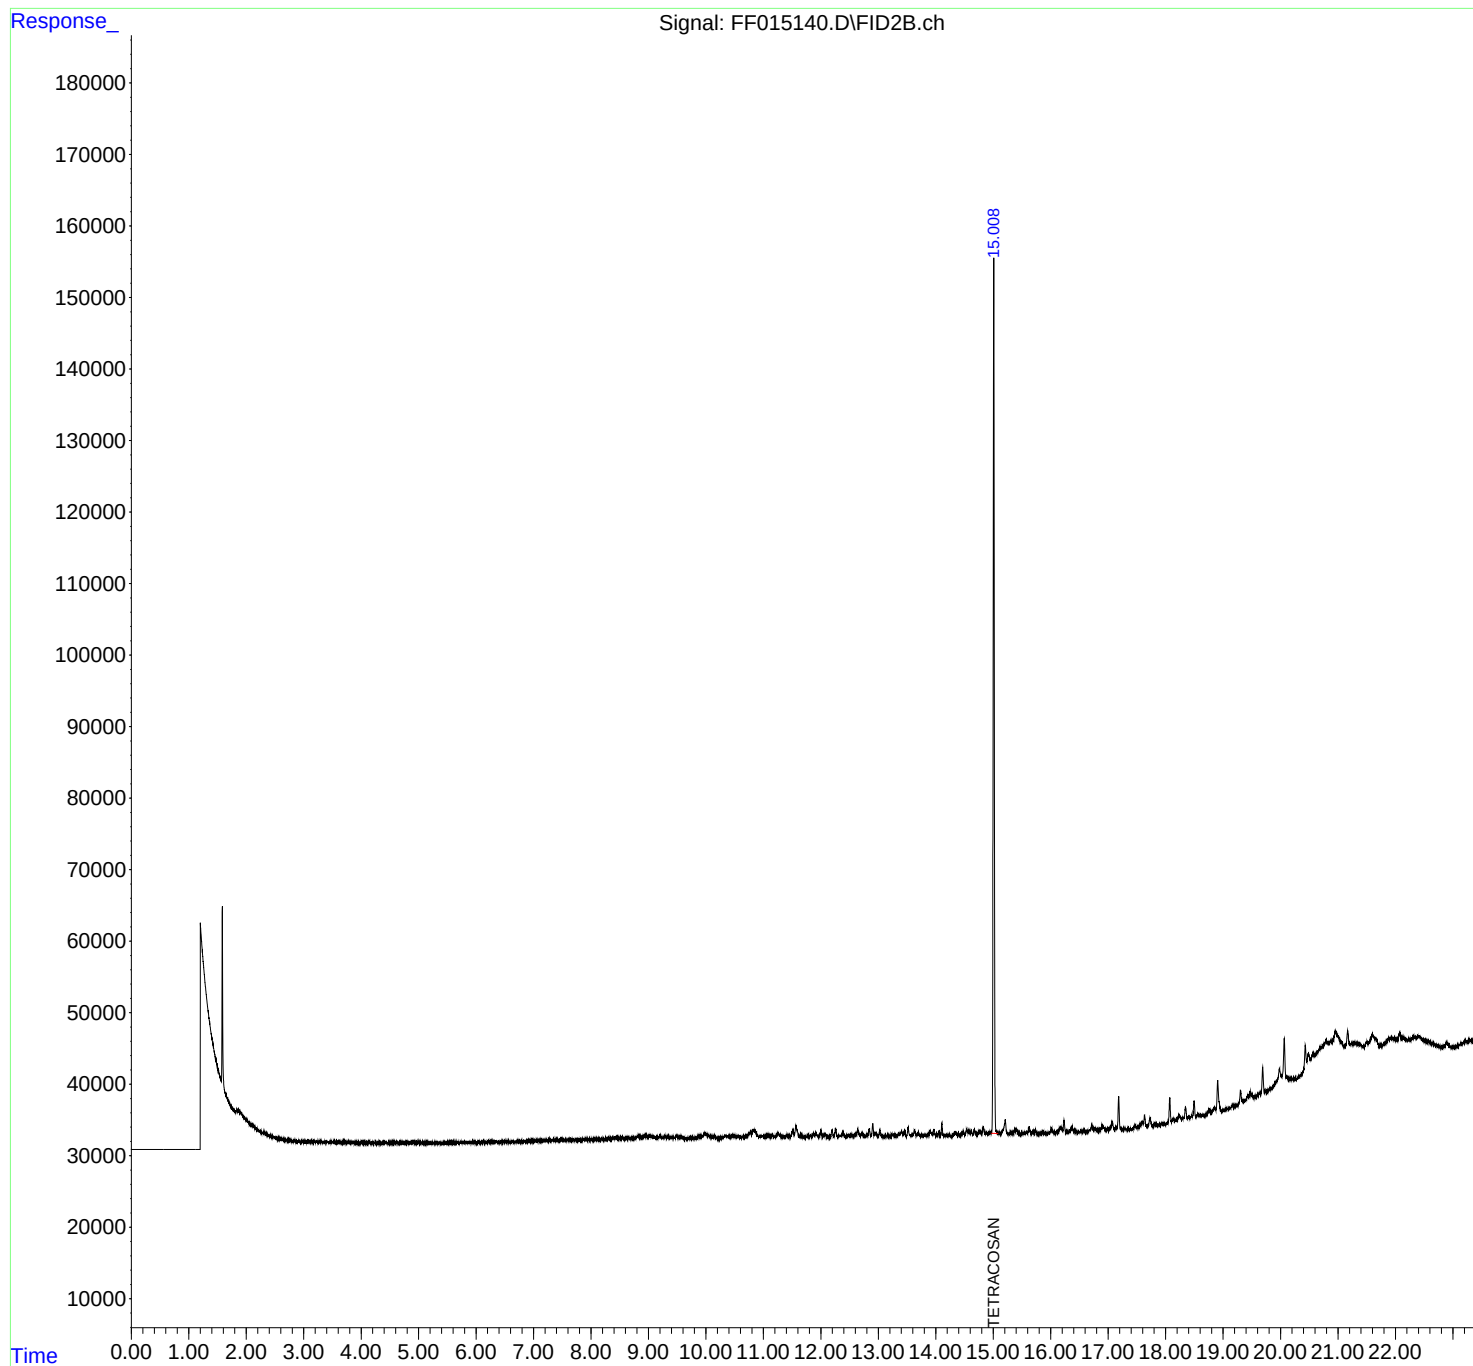

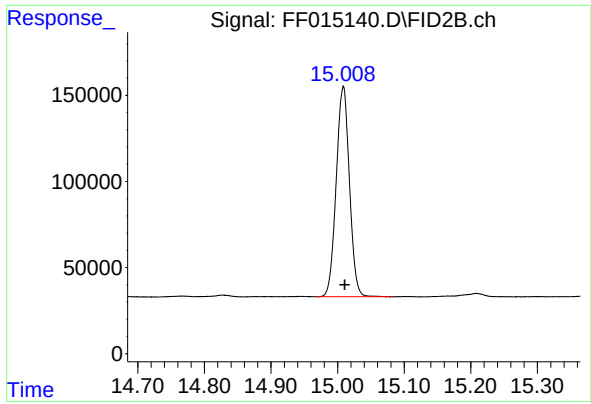

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.008 min
Delta R.T.: -0.002 min
Response: 1683520
Conc: 15.23 ug/ml

Instrument :
FID_F
ClientSampleId :
PB165425BL