

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120718\  
Data File : FF002946.D  
Signal(s) : FID2B.ch  
Acq On : 07 Dec 2018 18:14  
Operator : AJ\SJ  
Sample : J6291-04  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Dec 08 01:51:27 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120418.M  
Quant Title :  
QLast Update : Tue Dec 04 16:40:56 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                          | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.640 | 1696308  | 13.066 ug/ml |
| Target Compounds            |                          |        |          |              |
| 4)                          | N-TETRADECANE            | 8.237f | 195146   | 1.217 ug/ml  |
| 7)                          | N-EICOSANE               | 12.589 | 291206   | 1.888 ug/ml  |
| 10)                         | N-TETRACOSANE            | 14.818 | 149587   | 1.035 ug/ml  |
| 12)                         | N-OCTACOSANE             | 16.866 | 157825   | 1.178 ug/ml  |
| 14)                         | N-DOTRIACONTANE          | 18.544 | 132362   | 1.108 ug/ml  |
| -----                       |                          |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120718\  
Data File : FF002946.D  
Signal(s) : FID2B.ch  
Acq On : 07 Dec 2018 18:14  
Operator : AJ\SJ  
Sample : J6291-04  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Dec 08 01:51:27 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120418.M  
Quant Title :  
QLast Update : Tue Dec 04 16:40:56 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

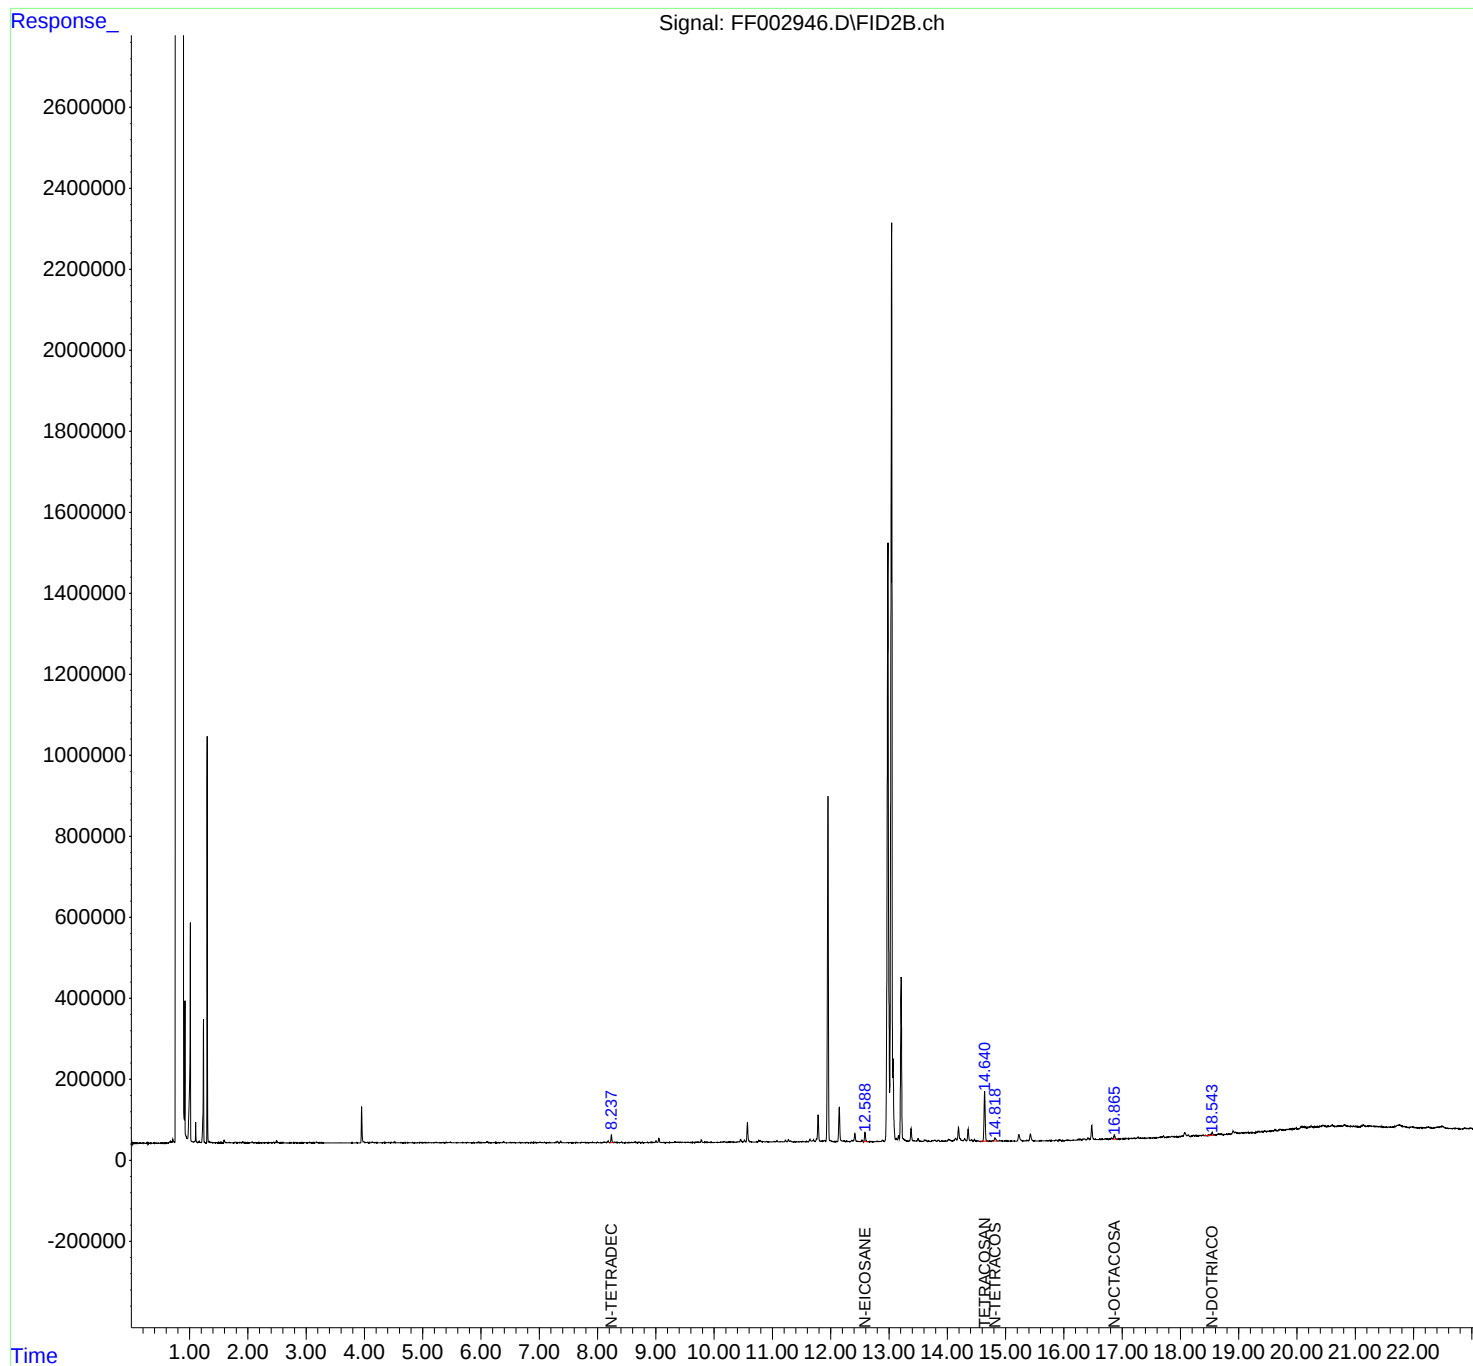

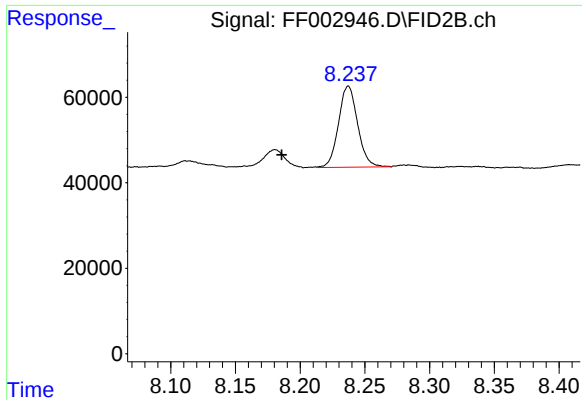


#4 N-TETRADECANE

R.T.: 8.237 min  
Delta R.T.: 0.051 min  
Response: 195146  
Conc: 1.22 ug/ml

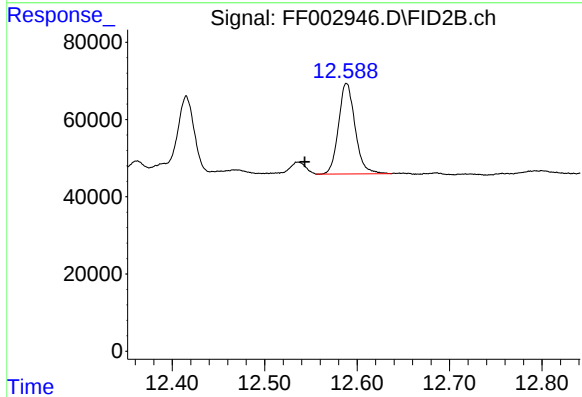


#7 N-EICOSANE

R.T.: 12.589 min  
Delta R.T.: 0.045 min  
Response: 291206  
Conc: 1.89 ug/ml

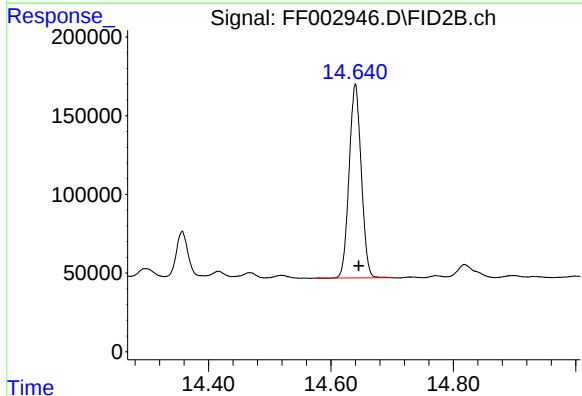


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.640 min  
Delta R.T.: -0.005 min  
Response: 1696308  
Conc: 13.07 ug/ml

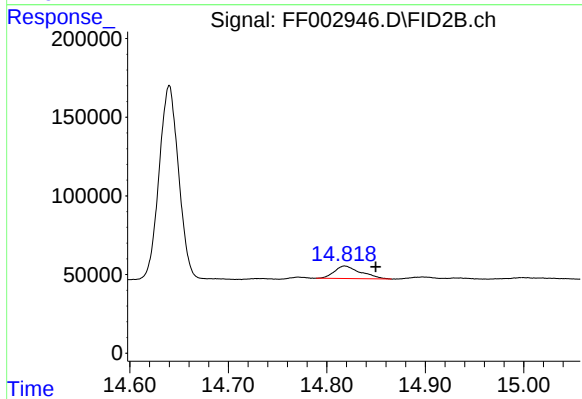


#10 N-TETRACOSANE

R.T.: 14.818 min  
Delta R.T.: -0.031 min  
Response: 149587  
Conc: 1.04 ug/ml

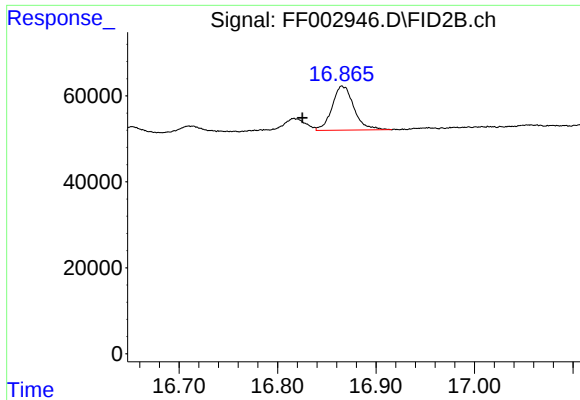

#12 N-OCTACOSANE

R.T.: 16.866 min  
Delta R.T.: 0.041 min  
Response: 157825  
Conc: 1.18 ug/ml

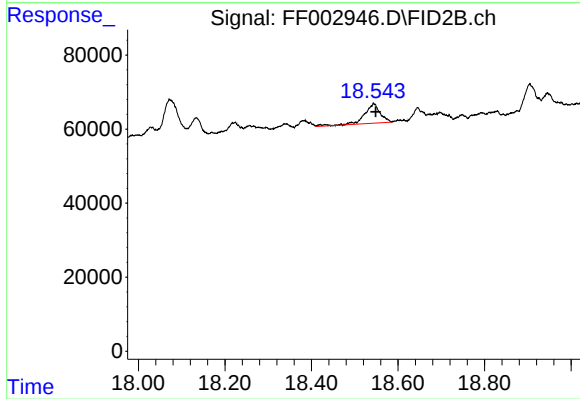

#14 N-DOTRIACONTANE

R.T.: 18.544 min  
Delta R.T.: -0.004 min  
Response: 132362  
Conc: 1.11 ug/ml