

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120718\
 Data File : FF002948.D
 Signal(s) : FID2B.ch
 Acq On : 07 Dec 2018 19:15
 Operator : AJ\SJ
 Sample : J6261-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 08 01:51:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	332393076	2560.309 ug/ml
Target Compounds			
2) N-DECANE	4.365	1184996	7.564 ug/ml
3) N-DODECANE	6.396	10069950	63.414 ug/ml
4) N-TETRADECANE	8.166	24989123	155.902 ug/ml
5) N-HEXADECANE	9.799	222941001	1392.115 ug/ml
6) N-OCTADECANE	11.215	406254812	2564.461 ug/ml
7) N-EICOSANE	12.552	871022726	5647.561 ug/ml
8) N-DOCOSANE	13.743	780092103	5216.956 ug/ml
10) N-TETRACOSANE	14.873	106908811	739.775 ug/ml
11) N-HEXACOSANE	15.864	48960163	350.774 ug/ml
12) N-OCTACOSANE	16.825	13336070	99.533 ug/ml
13) N-TRIACONTANE	17.720	1794676	14.006 ug/ml
14) N-DOTRIACONTANE	18.545	254913	2.135 ug/ml
15) N-TETRATRIACONTANE	19.340	191152	1.687 ug/ml
17) N-OCTATRIACONTANE	20.772	224552	2.212 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120718\
 Data File : FF002948.D
 Signal(s) : FID2B.ch
 Acq On : 07 Dec 2018 19:15
 Operator : AJ\SJ
 Sample : J6261-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1


Integration File: autoint1.e
 Quant Time: Dec 08 01:51:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

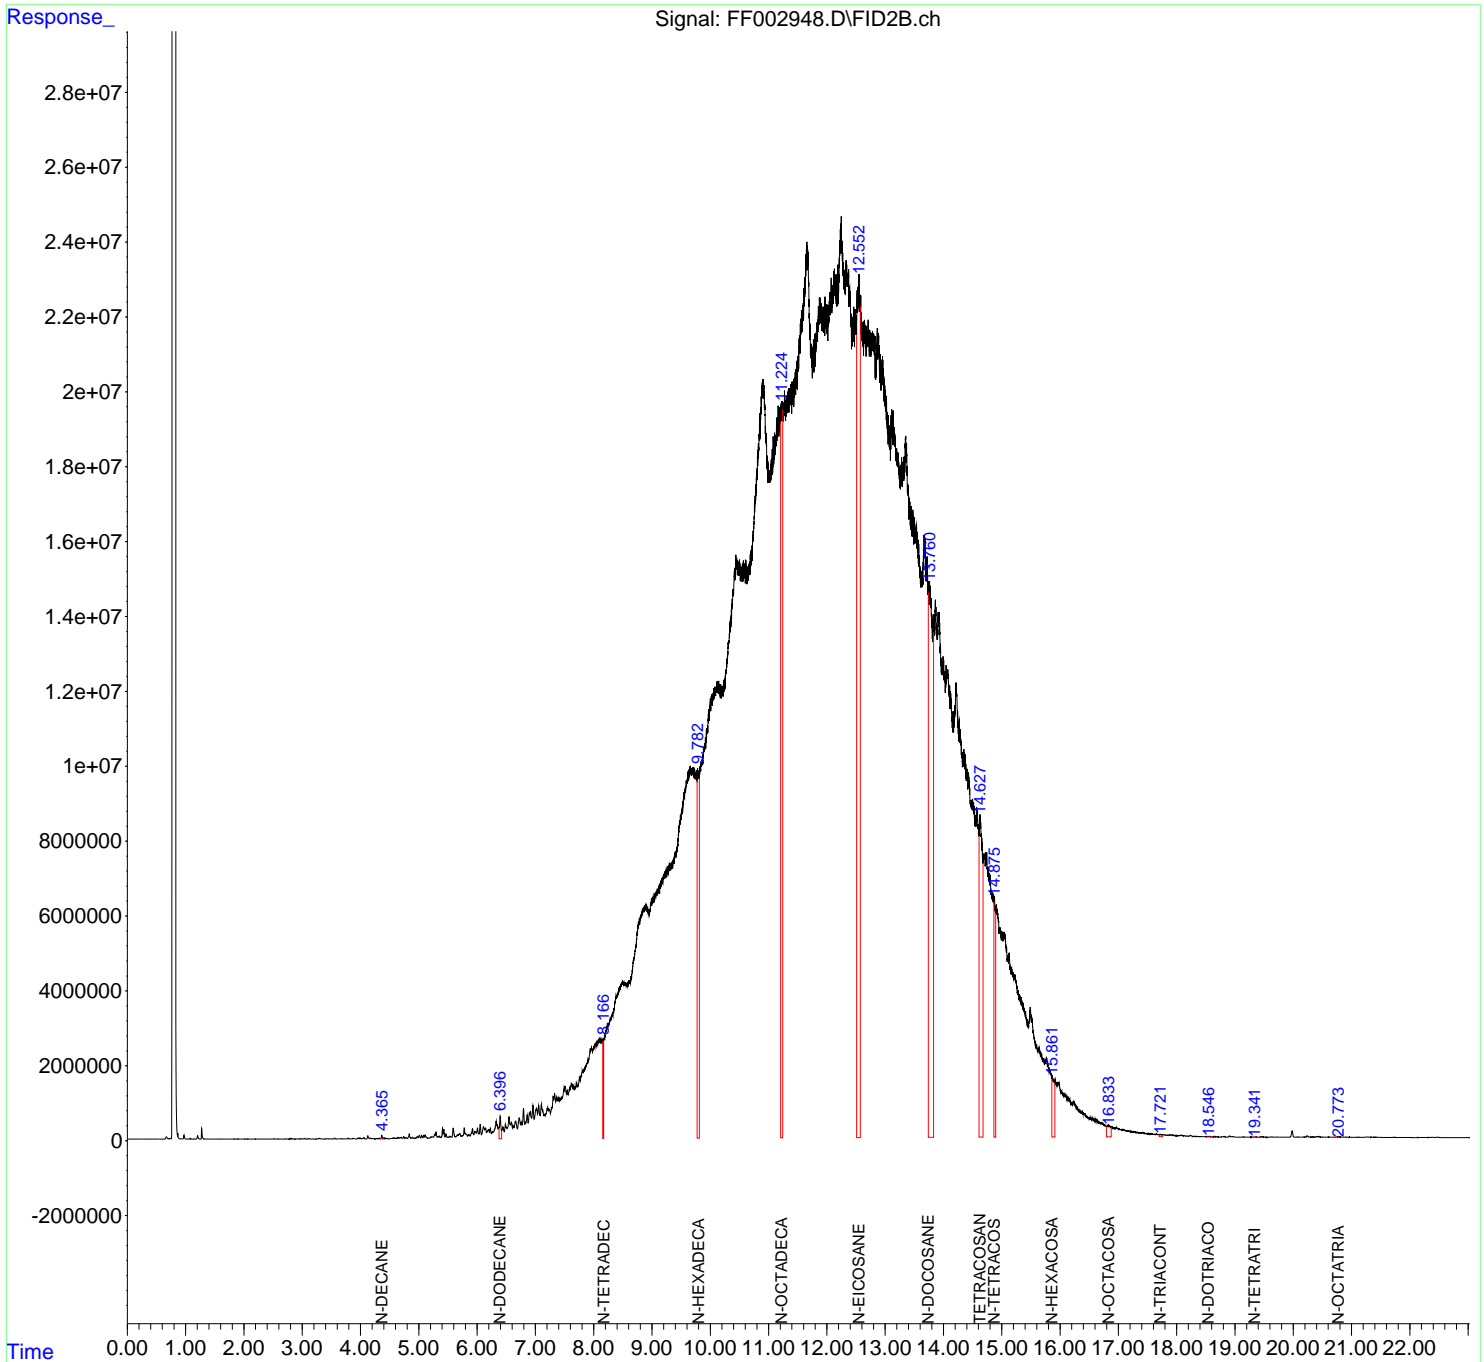


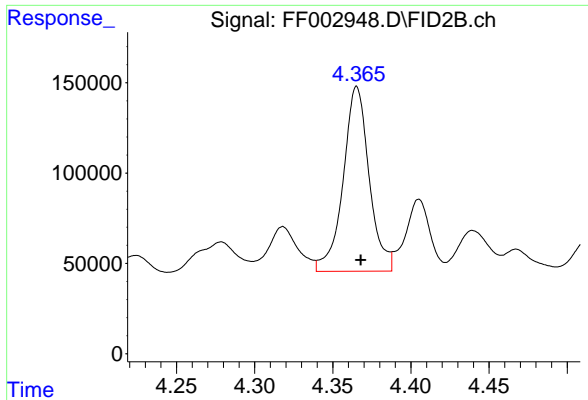


#2 N-DECANE
R.T.: 4.365 min
Delta R.T.: -0.002 min
Response: 1184996
Conc: 7.56 ug/ml

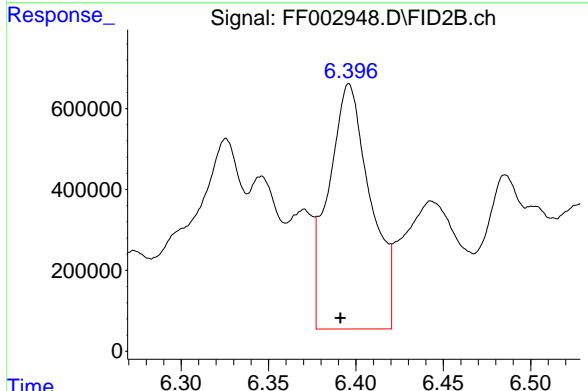


#3 N-DODECANE
R.T.: 6.396 min
Delta R.T.: 0.005 min
Response: 10069950
Conc: 63.41 ug/ml

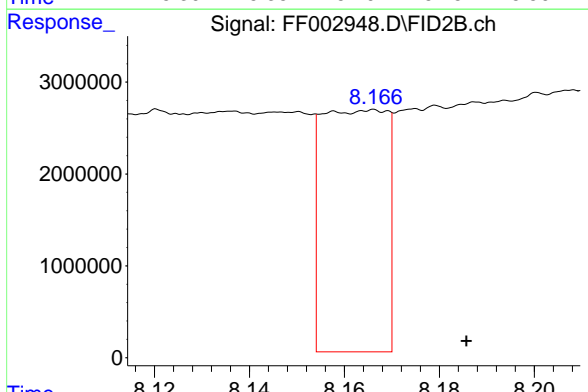


#4 N-TETRADECANE
R.T.: 8.166 min
Delta R.T.: -0.020 min
Response: 24989123
Conc: 155.90 ug/ml

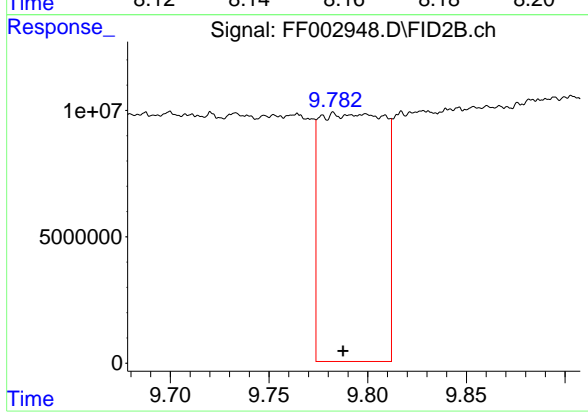


#5 N-HEXADECANE
R.T.: 9.799 min
Delta R.T.: 0.011 min
Response: 222941001
Conc: 1392.11 ug/ml

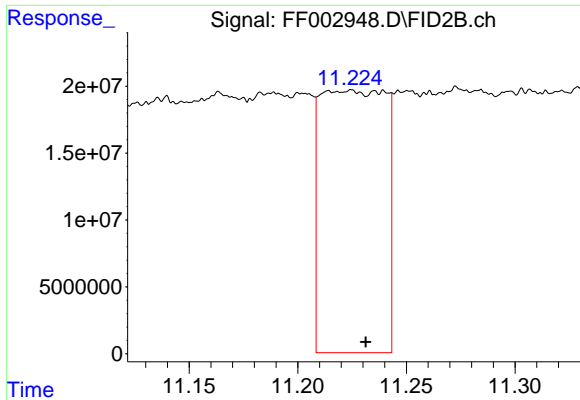


#6 N-OCTADECANE
 R.T.: 11.215 min
 Delta R.T.: -0.017 min
 Response: 406254812
 Conc: 2564.46 ug/ml

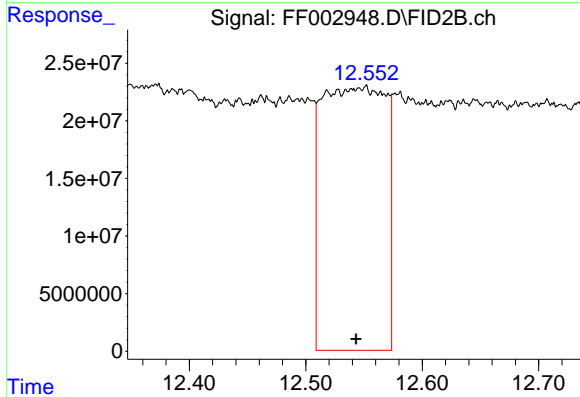


#7 N-EICOSANE
 R.T.: 12.552 min
 Delta R.T.: 0.008 min
 Response: 871022726
 Conc: 5647.56 ug/ml

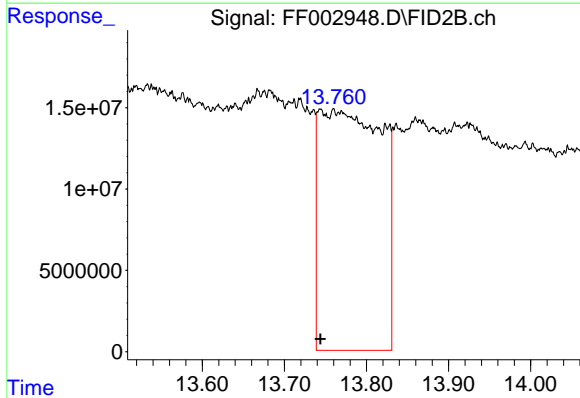


#8 N-DOCOSANE
 R.T.: 13.743 min
 Delta R.T.: 0.000 min
 Response: 780092103
 Conc: 5216.96 ug/ml

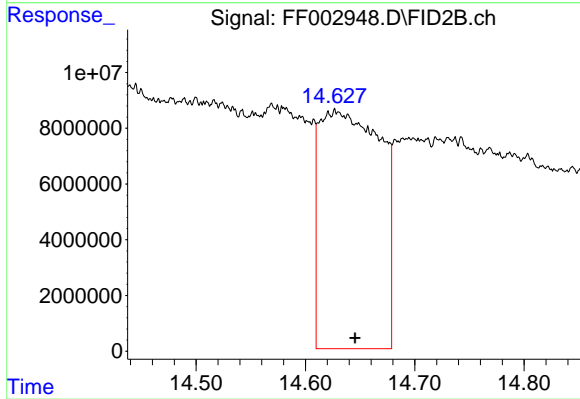


#9 TETRACOSANE-d50 (SURROGATE)
 R.T.: 14.628 min
 Delta R.T.: -0.018 min
 Response: 332393076
 Conc: 2560.31 ug/ml

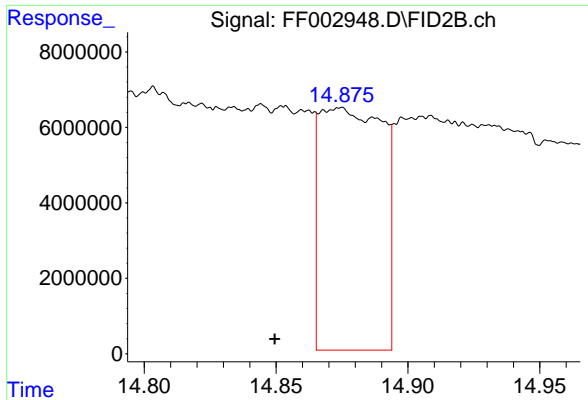


#10 N-TETRACOSANE
R.T.: 14.873 min
Delta R.T.: 0.024 min
Response: 106908811
Conc: 739.77 ug/ml

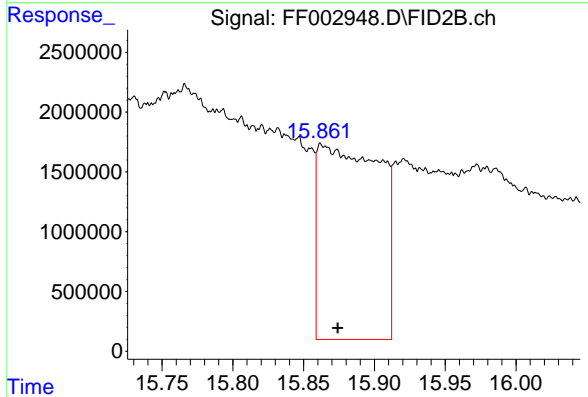


#11 N-HEXACOSANE
R.T.: 15.864 min
Delta R.T.: -0.011 min
Response: 48960163
Conc: 350.77 ug/ml

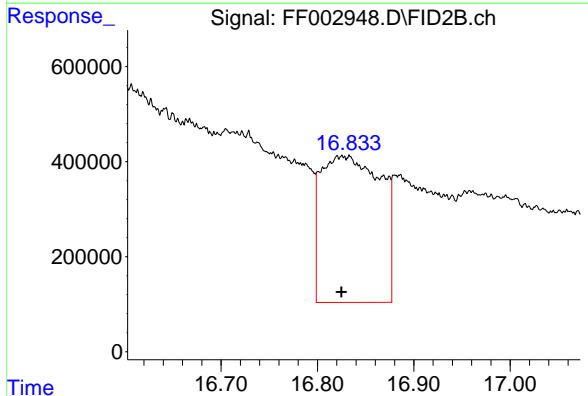

#12 N-OCTACOSANE
R.T.: 16.825 min
Delta R.T.: 0.000 min
Response: 13336070
Conc: 99.53 ug/ml

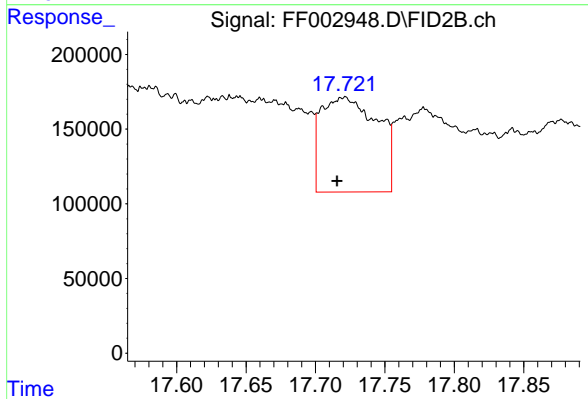


#13 N-TRIACONTANE
R.T.: 17.720 min
Delta R.T.: 0.005 min
Response: 1794676
Conc: 14.01 ug/ml

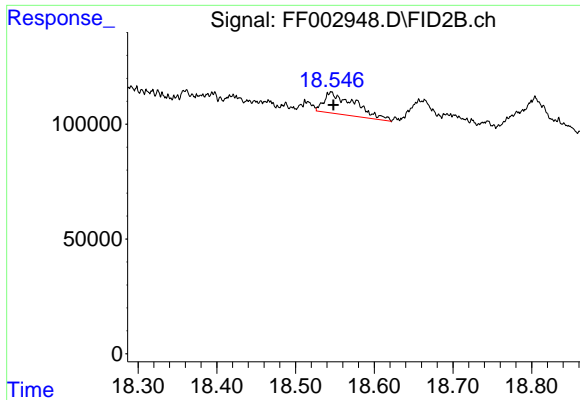


#14 N-DOTRIACONTANE

R.T.: 18.545 min
Delta R.T.: -0.004 min
Response: 254913
Conc: 2.13 ug/ml

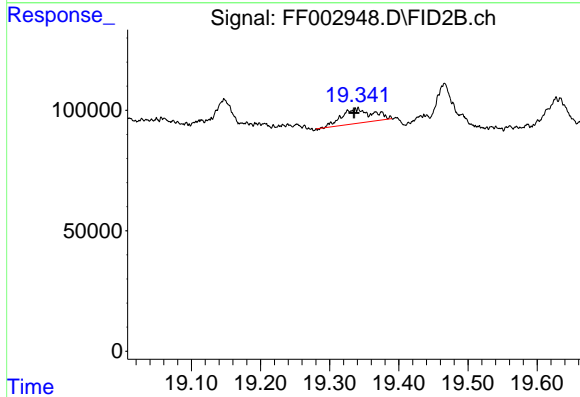

#15 N-TETRATRIACONTANE

R.T.: 19.340 min
Delta R.T.: 0.005 min
Response: 191152
Conc: 1.69 ug/ml

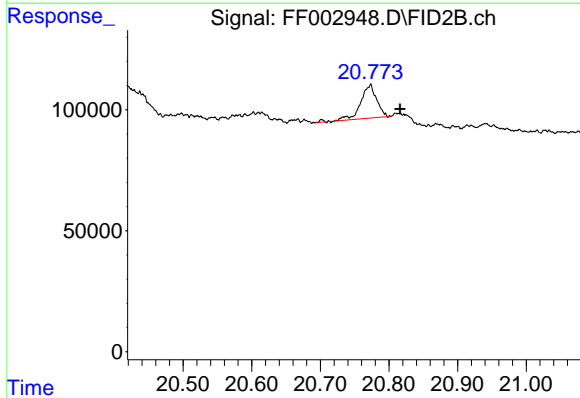

#17 N-OCTATRIACONTANE

R.T.: 20.772 min
Delta R.T.: -0.044 min
Response: 224552
Conc: 2.21 ug/ml