

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120719\
Data File : FF006016.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2019 10:00
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Dec 06 13:20:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.696	122719	0.846 ug/ml
14) N-DOTRIACONTANE	18.527	194405	1.400 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120719\
Data File : FF006016.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2019 10:00
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
MECL2

Integration File: autoint1.e
Quant Time: Dec 06 13:20:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

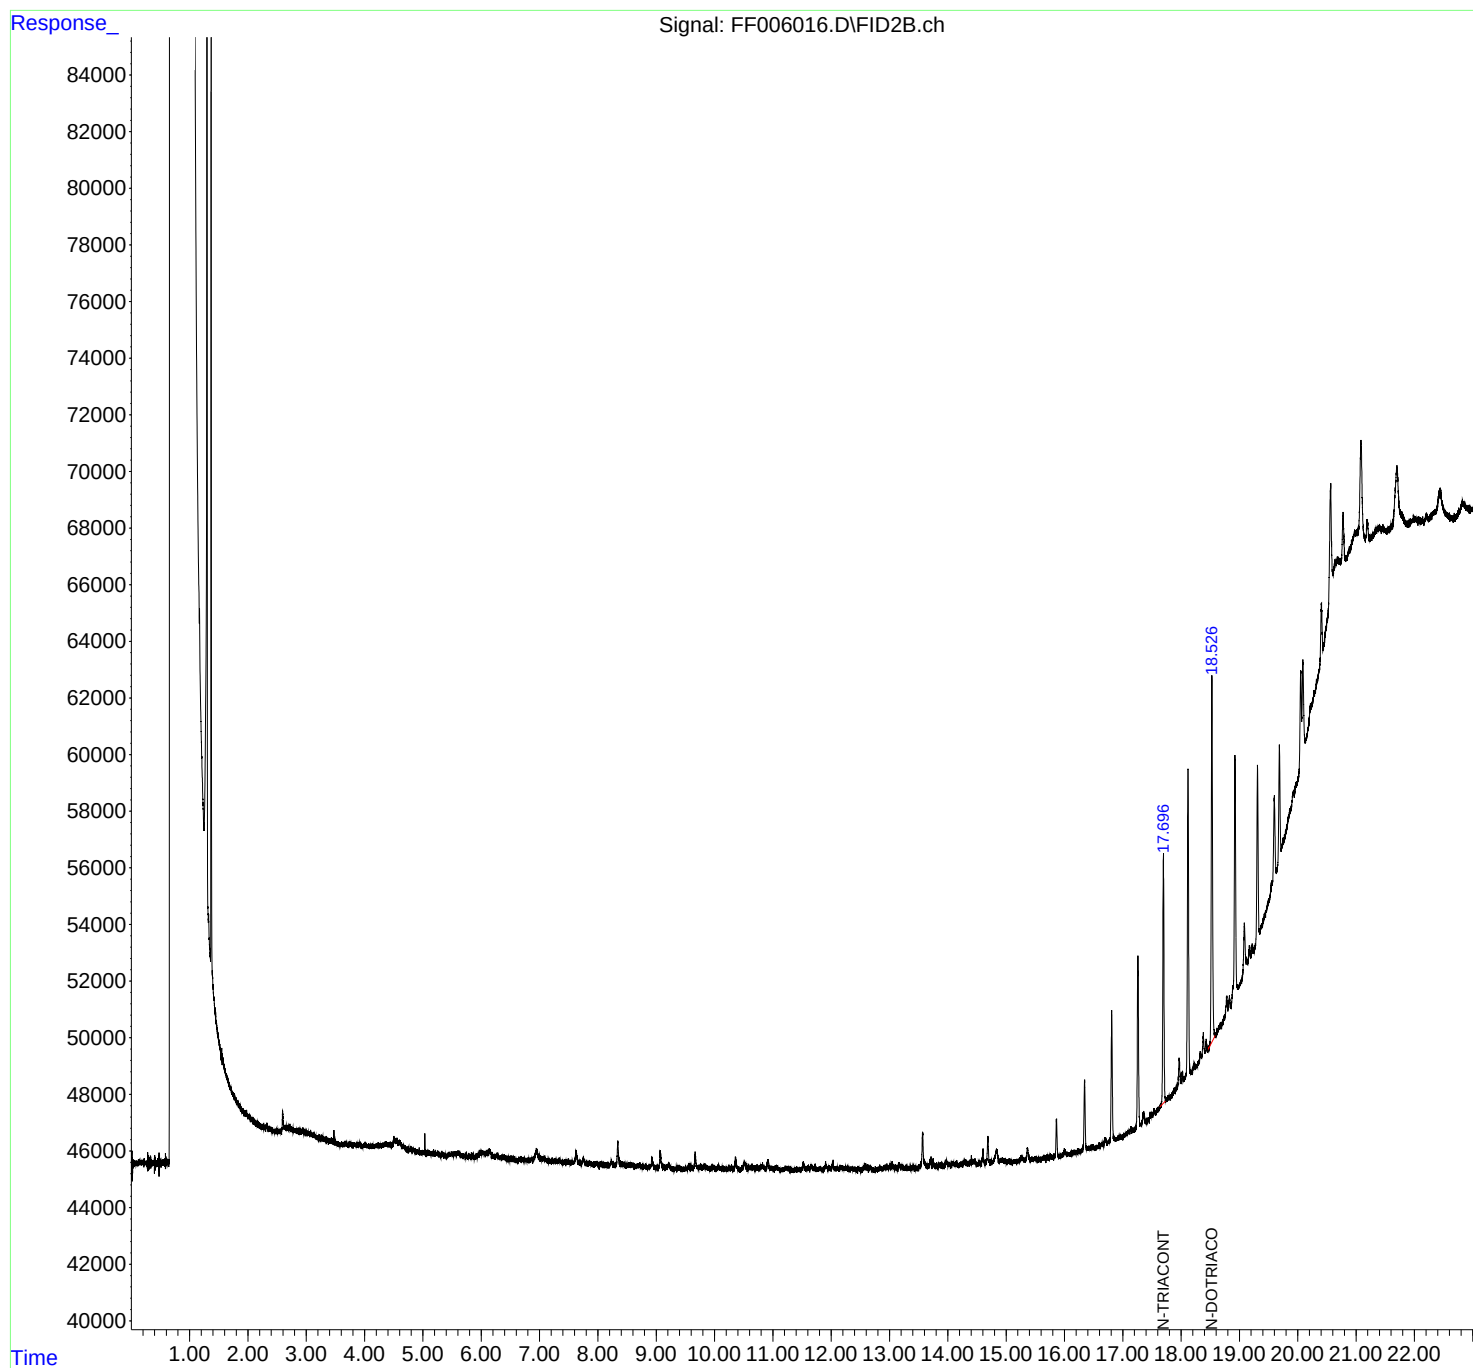


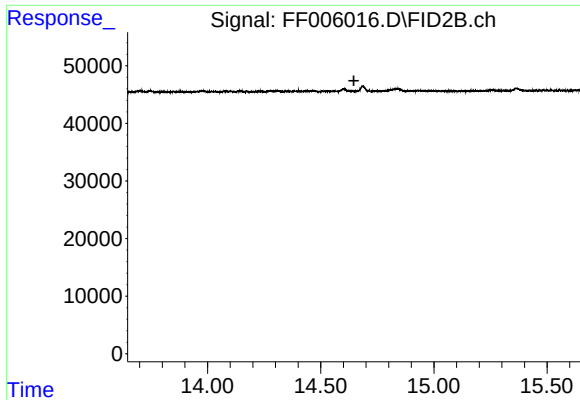

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.646 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

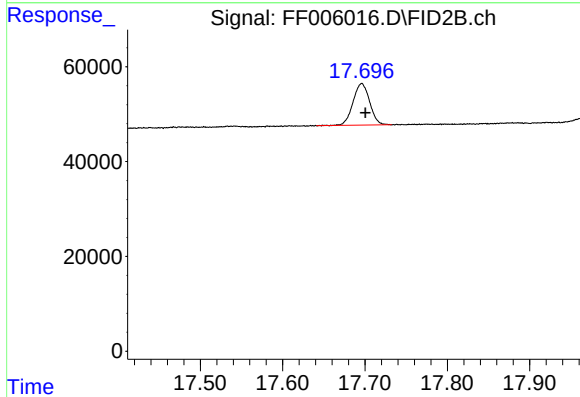

#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: -0.005 min
Response: 122719
Conc: 0.85 ug/ml

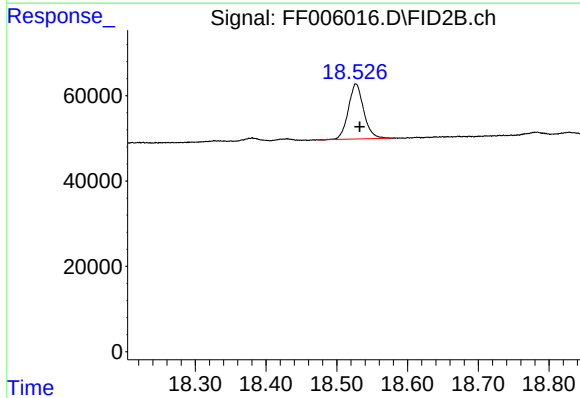

#14 N-DOTRIACONTANE

R.T.: 18.527 min
Delta R.T.: -0.005 min
Response: 194405
Conc: 1.40 ug/ml