

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120722\
Data File : FF011773.D
Signal(s) : FID2B.ch
Acq On : 07 Dec 2022 13:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 08 01:30:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.770	2196688	15.907 ug/ml
12)	N-OCTACOSANE	17.230	2036566	16.522 ug/ml
13)	N-TRIACONTANE	18.115	136902	1.130 ug/ml
14)	N-DOTRIACONTANE	18.948	178744	1.485 ug/ml
15)	N-TETRATRIACONTANE	19.732	146332	1.235 ug/ml
16)	N-HEXATRIACONTANE	20.471	89082	0.766 ug/ml
17)	N-OCTATRIACONTANE	21.214	54715	0.453 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120722\
Data File : FF011773.D
Signal(s) : FID2B.ch
Acq On : 07 Dec 2022 13:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 08 01:30:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

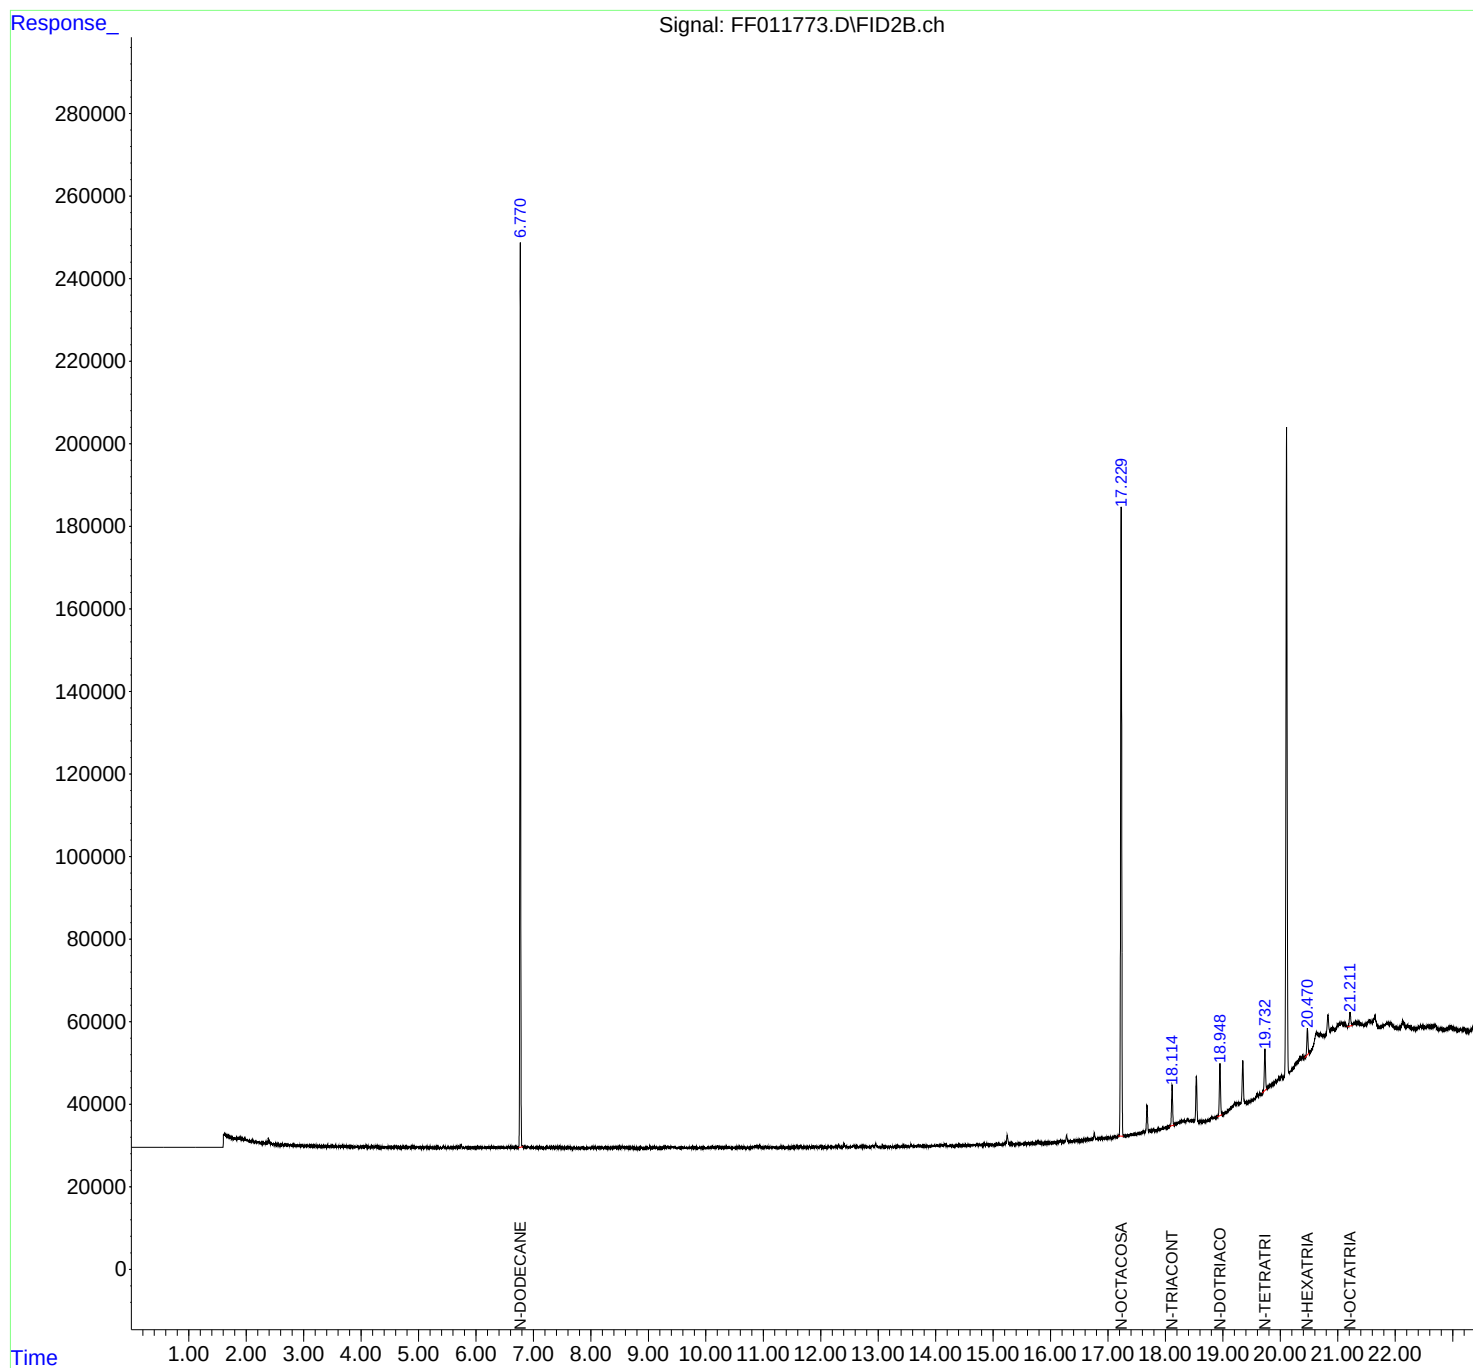


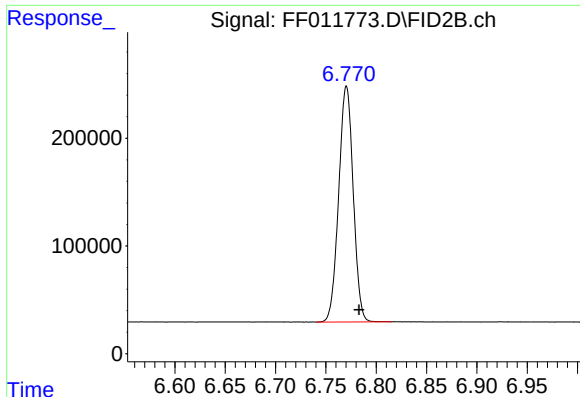

#3 N-DODECANE


R.T.: 6.770 min
Delta R.T.: -0.012 min
Response: 2196688
Conc: 15.91 ug/ml

Instrument :
FID_F
ClientSampleId :

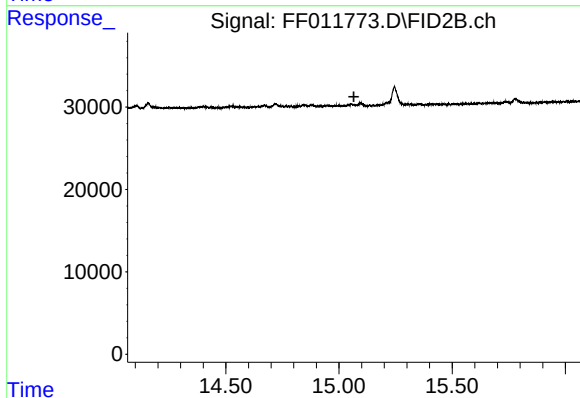


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

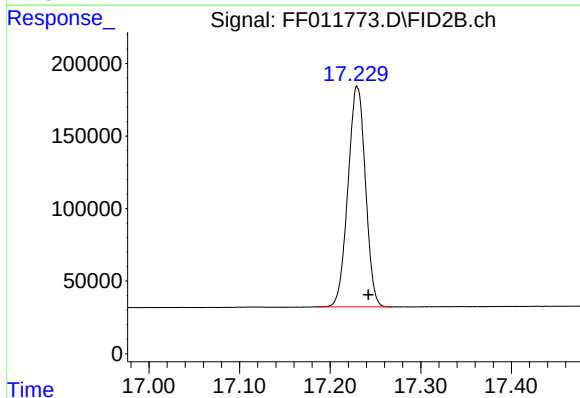


#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: -0.012 min
Response: 2036566
Conc: 16.52 ug/ml

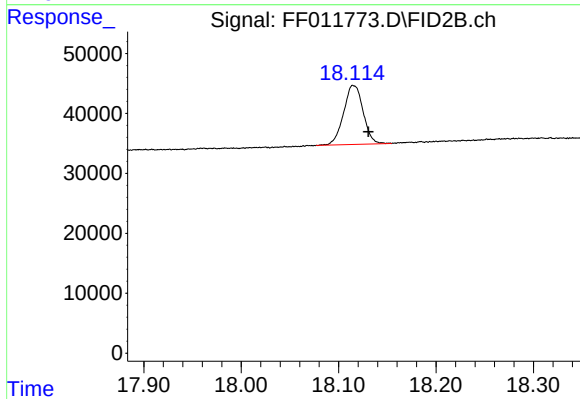

#13 N-TRIACONTANE


R.T.: 18.115 min
Delta R.T.: -0.015 min
Response: 136902
Conc: 1.13 ug/ml

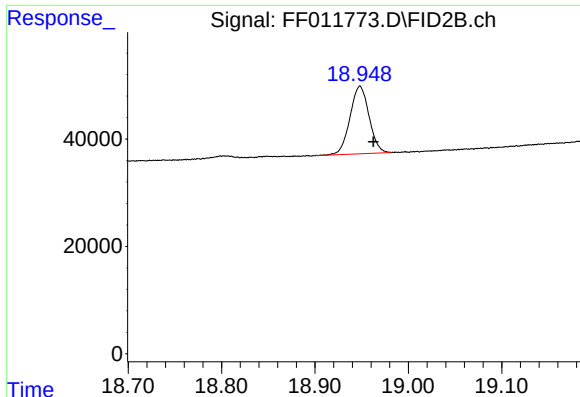

#14 N-DOTRIACONTANE


R.T.: 18.948 min
Delta R.T.: -0.015 min
Response: 178744
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

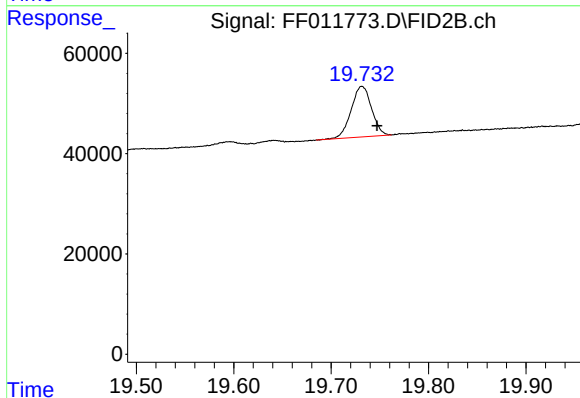


#15 N-TETRATRIACONTANE

R.T.: 19.732 min
Delta R.T.: -0.015 min
Response: 146332
Conc: 1.23 ug/ml

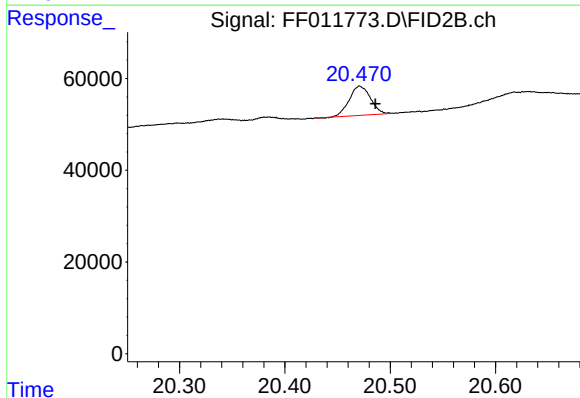

#16 N-HEXATRIACONTANE

R.T.: 20.471 min
Delta R.T.: -0.015 min
Response: 89082
Conc: 0.77 ug/ml

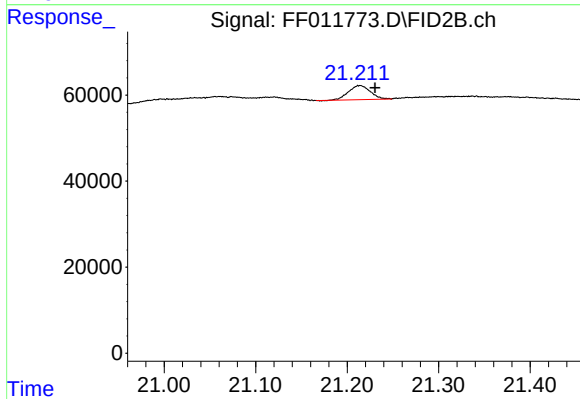

#17 N-OCTATRIACONTANE

R.T.: 21.214 min
Delta R.T.: -0.016 min
Response: 54715
Conc: 0.45 ug/ml