

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120722\
 Data File : FF011775.D
 Signal(s) : FID2B.ch
 Acq On : 07 Dec 2022 16:22
 Operator : YP\AJ
 Sample : N5897-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 08 01:31:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
 Quant Title :
 QLast Update : Tue Dec 06 04:24:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.056	2499748	21.892 ug/ml
Target Compounds			
4) N-TETRADECANE	8.597	108918	0.792 ug/ml
5) N-HEXADECANE	10.216	243882	1.759 ug/ml
6) N-OCTADECANE	11.668	139607	1.003 ug/ml
7) N-EICOSANE	12.954	130494	0.964 ug/ml
8) N-DOCOSANE	14.154	100197	0.756 ug/ml
10) N-TETRACOSANE	15.301	109828	0.835 ug/ml
11) N-HEXACOSANE	16.279	139792	1.103 ug/ml
12) N-OCTACOSANE	17.239	310289	2.517 ug/ml
13) N-TRIACONTANE	18.119	204995	1.692 ug/ml
14) N-DOTRIACONTANE	18.936	339657	2.822 ug/ml
15) N-TETRATRIACONTANE	19.754	349114	2.946 ug/ml
16) N-HEXATRIACONTANE	20.553f	38851	0.334 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF120722\
Data File : FF011775.D
Signal(s) : FID2B.ch
Acq On : 07 Dec 2022 16:22
Operator : YP\AJ
Sample : N5897-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 08 01:31:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

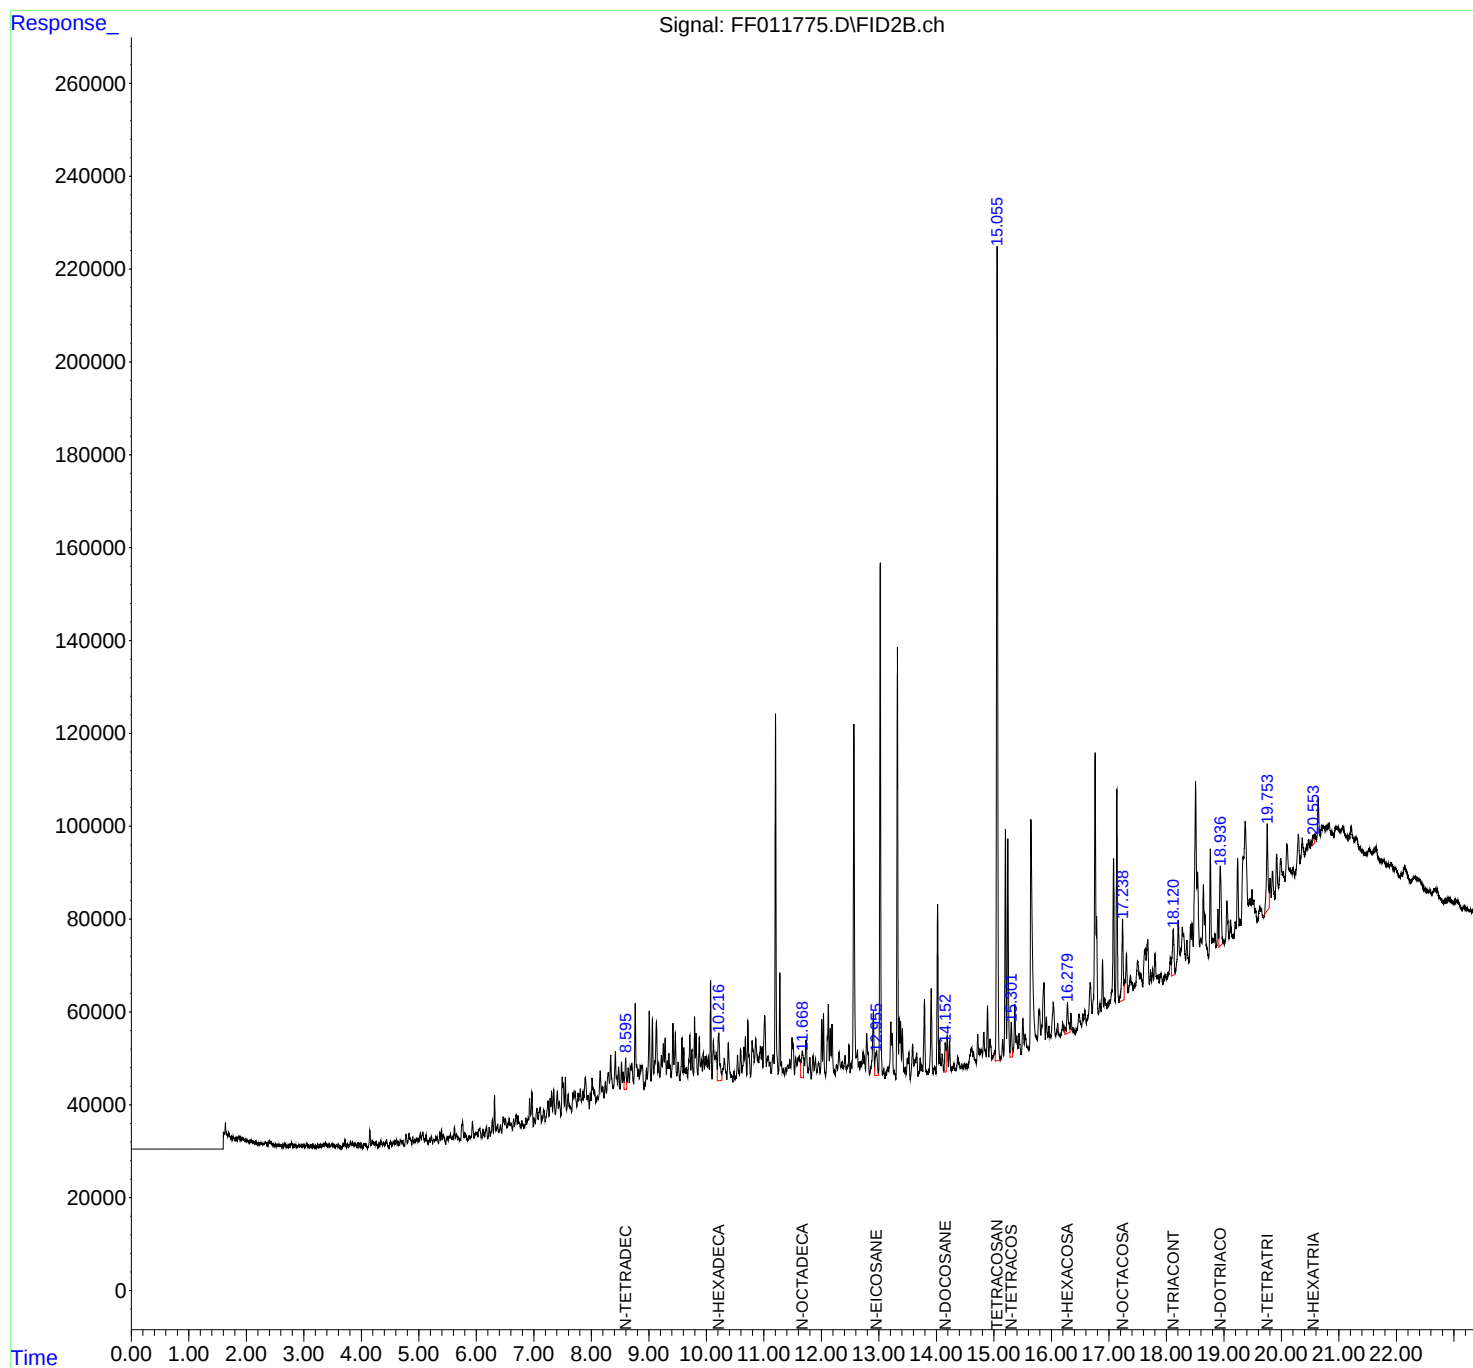


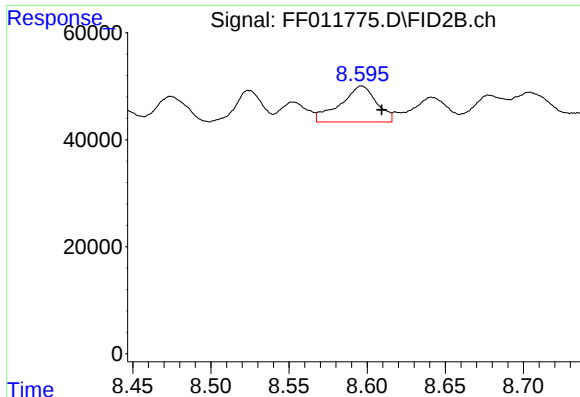

#4 N-TETRADECANE


R.T.: 8.597 min
Delta R.T.: -0.013 min
Response: 108918
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :

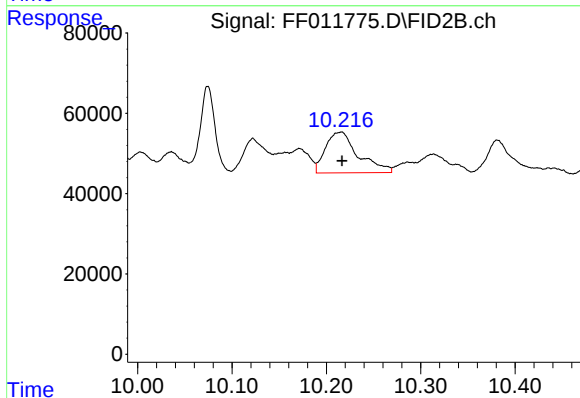


#5 N-HEXADECANE

R.T.: 10.216 min
Delta R.T.: 0.000 min
Response: 243882
Conc: 1.76 ug/ml

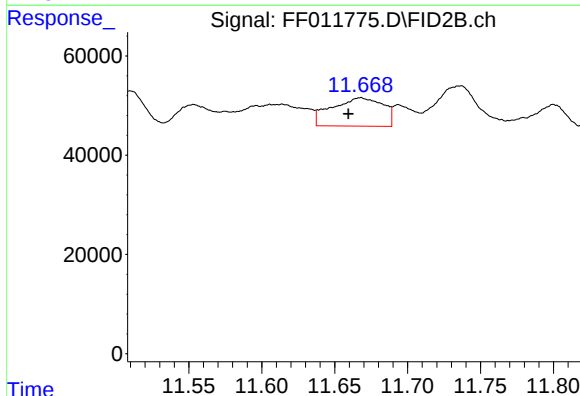


#6 N-OCTADECANE

R.T.: 11.668 min
Delta R.T.: 0.008 min
Response: 139607
Conc: 1.00 ug/ml

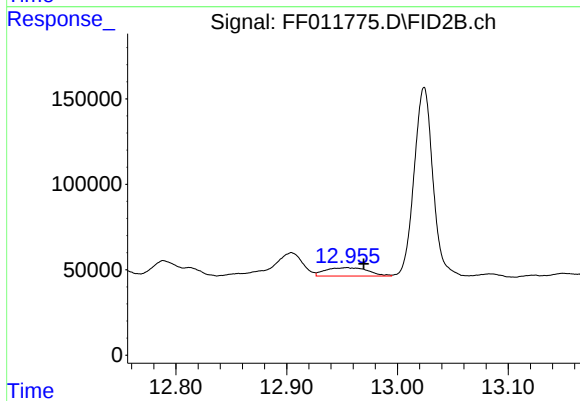

#7 N-EICOSANE


R.T.: 12.954 min
Delta R.T.: -0.015 min
Response: 130494
Conc: 0.96 ug/ml

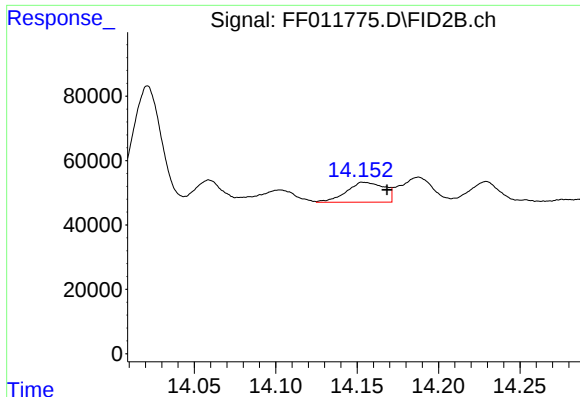

#8 N-DOCOSANE


R.T.: 14.154 min
Delta R.T.: -0.014 min
Response: 100197
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

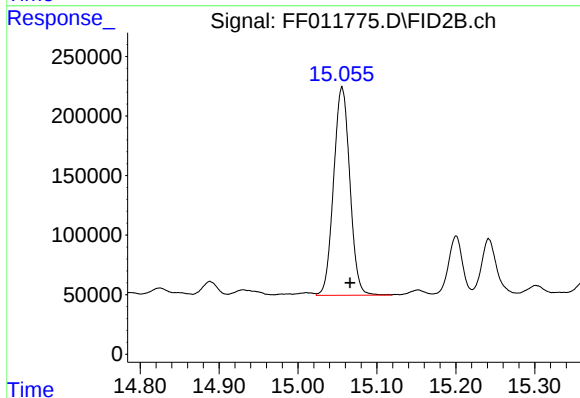


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.056 min
Delta R.T.: -0.010 min
Response: 2499748
Conc: 21.89 ug/ml

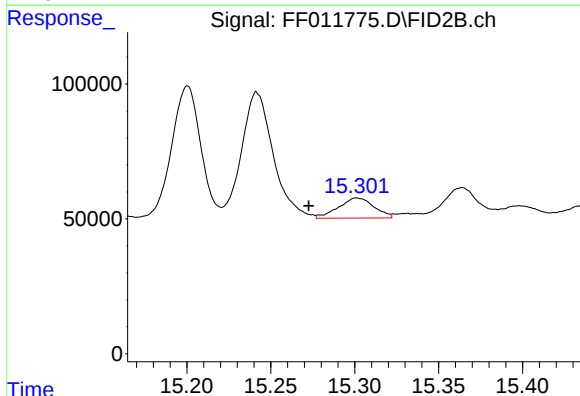


#10 N-TETRACOSANE

R.T.: 15.301 min
Delta R.T.: 0.029 min
Response: 109828
Conc: 0.84 ug/ml

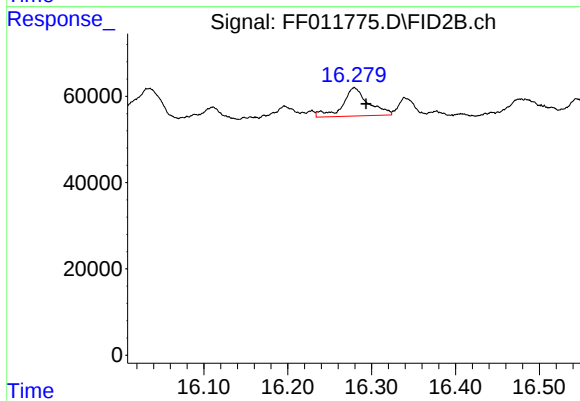

#11 N-HEXACOSANE


R.T.: 16.279 min
Delta R.T.: -0.014 min
Response: 139792
Conc: 1.10 ug/ml

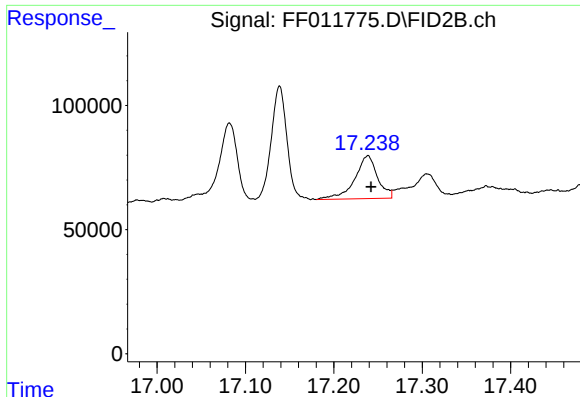

#12 N-OCTACOSANE


R.T.: 17.239 min
Delta R.T.: -0.004 min
Response: 310289
Conc: 2.52 ug/ml

Instrument :
FID_F
ClientSampleId :

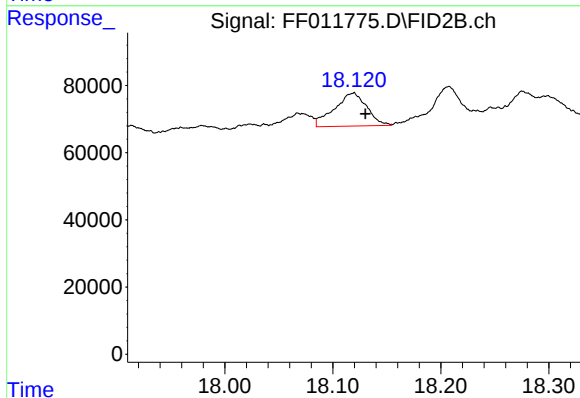


#13 N-TRIACONTANE

R.T.: 18.119 min
Delta R.T.: -0.011 min
Response: 204995
Conc: 1.69 ug/ml

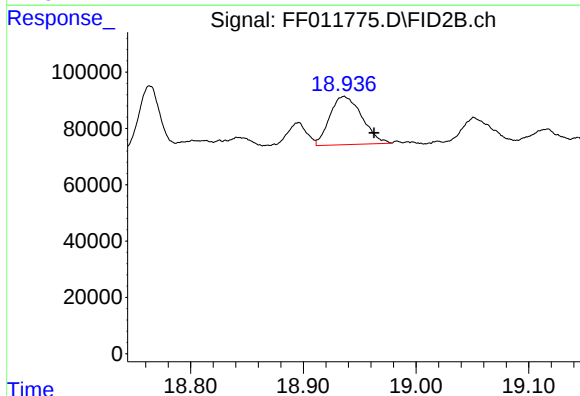


#14 N-DOTRIACONTANE

R.T.: 18.936 min
Delta R.T.: -0.027 min
Response: 339657
Conc: 2.82 ug/ml

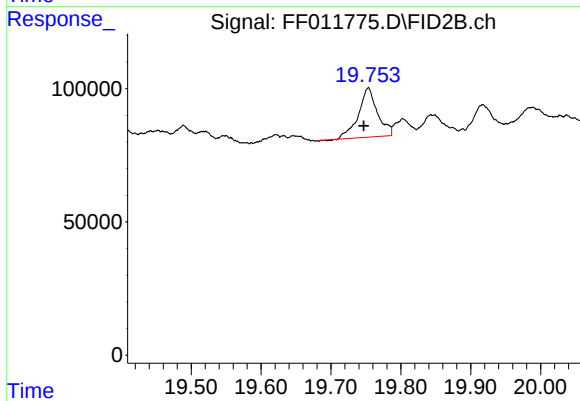

#15 N-TETRATRIACONTANE

R.T.: 19.754 min
Delta R.T.: 0.006 min
Response: 349114
Conc: 2.95 ug/ml

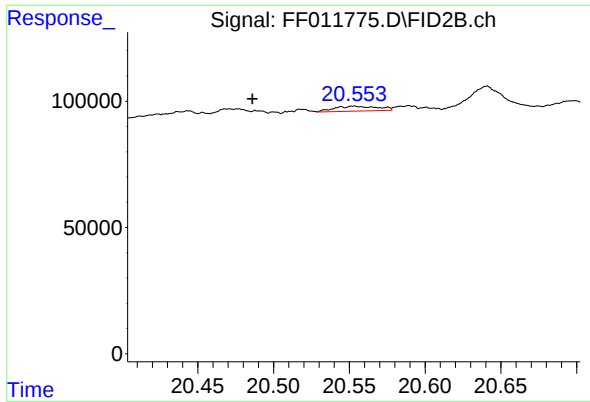

#16 N-HEXATRIACONTANE

R.T.: 20.553 min
Delta R.T.: 0.067 min
Response: 38851
Conc: 0.33 ug/ml

Instrument :
FID_F
ClientSampleId :