

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120722\  
Data File : FF011773.D  
Signal(s) : FID2B.ch  
Acq On : 07 Dec 2022 13:03  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: Sample.e  
Quant Time: Dec 08 01:30:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120522.M  
Quant Title :  
QLast Update : Tue Dec 06 04:24:35 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.770  | 2196688  | 15.907 ug/ml |
| 12)                         | N-OCTACOSANE | 17.230 | 2036566  | 16.522 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF120722\  
Data File : FF011773.D  
Signal(s) : FID2B.ch  
Acq On : 07 Dec 2022 13:03  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: Sample.e  
Quant Time: Dec 08 01:30:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120522.M  
Quant Title :  
QLast Update : Tue Dec 06 04:24:35 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

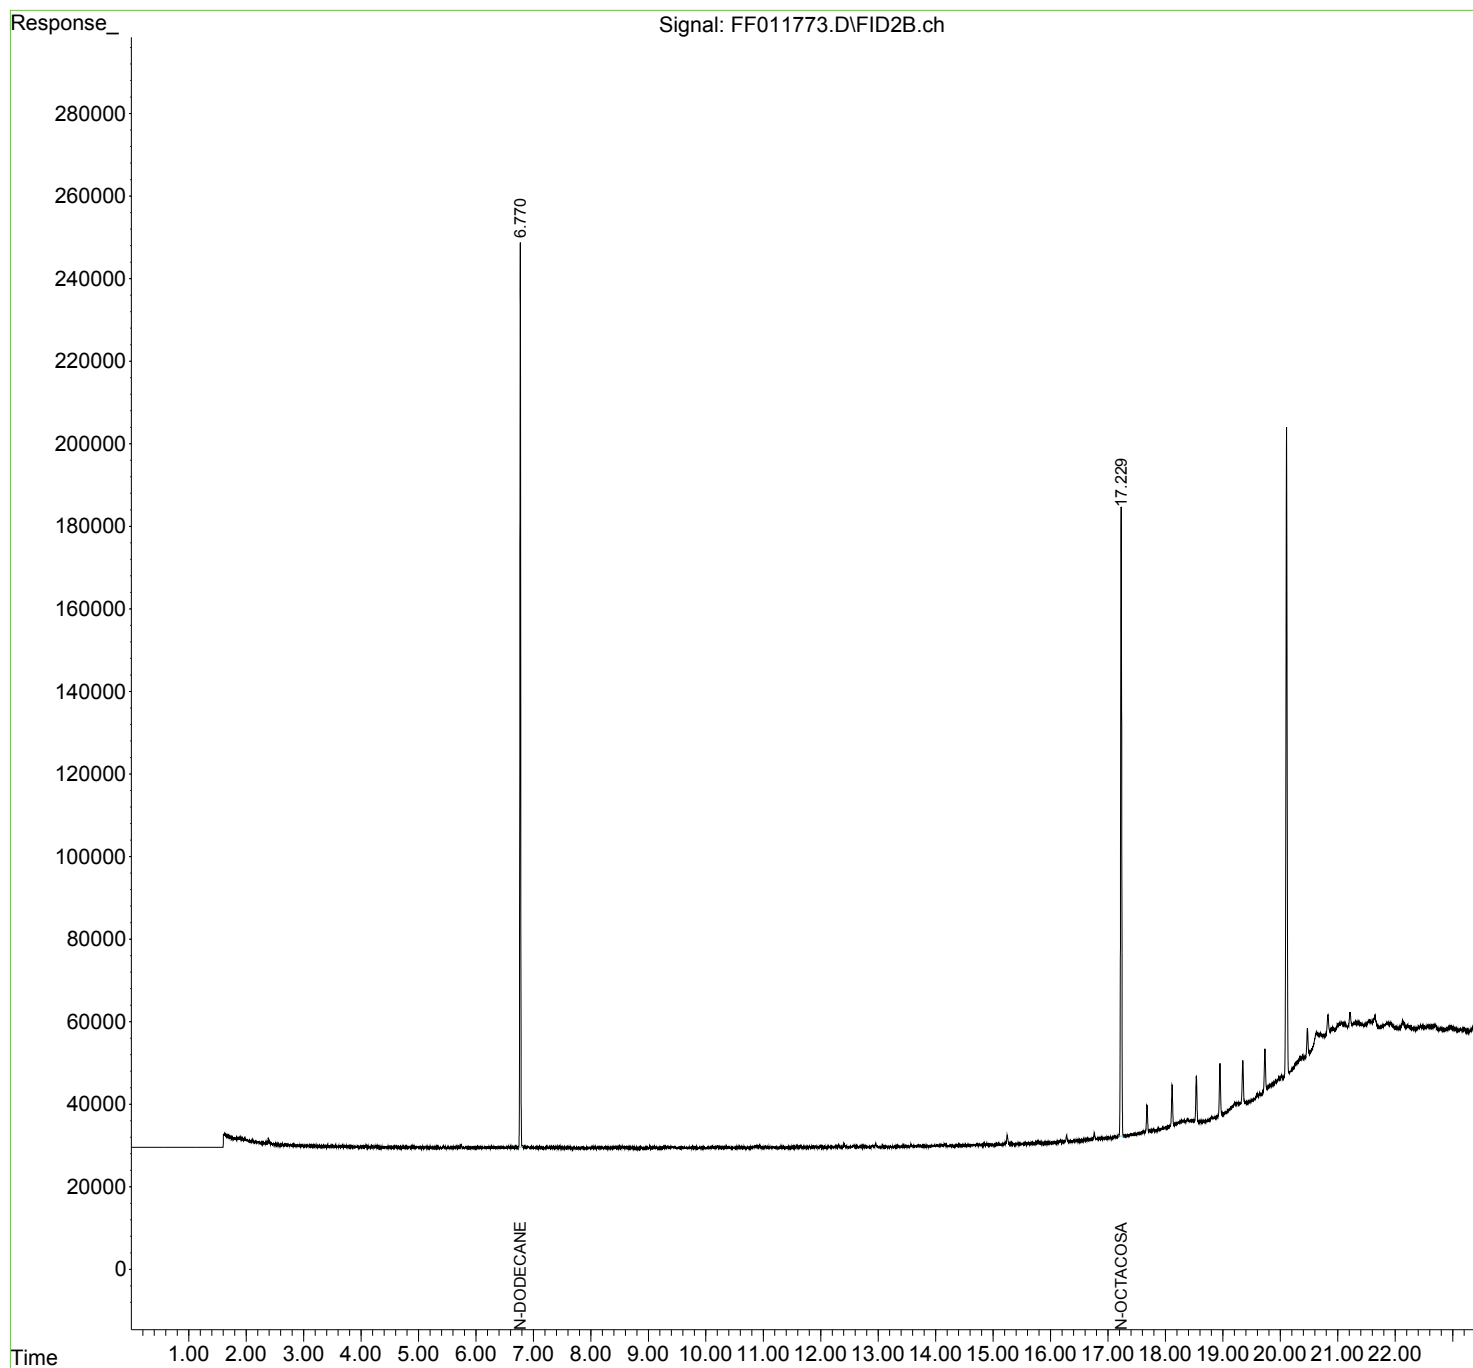


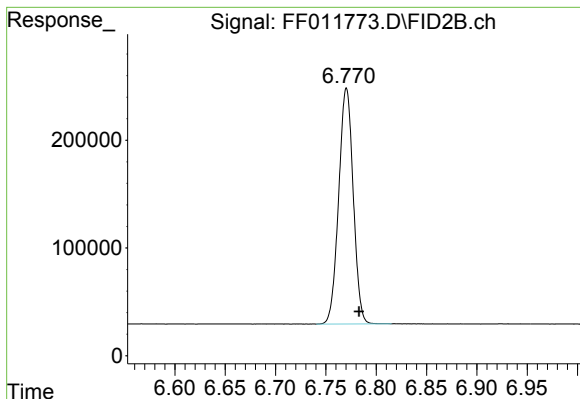

#3 N-DODECANE


R.T.: 6.770 min  
Delta R.T.: -0.012 min  
Response: 2196688  
Conc: 15.91 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

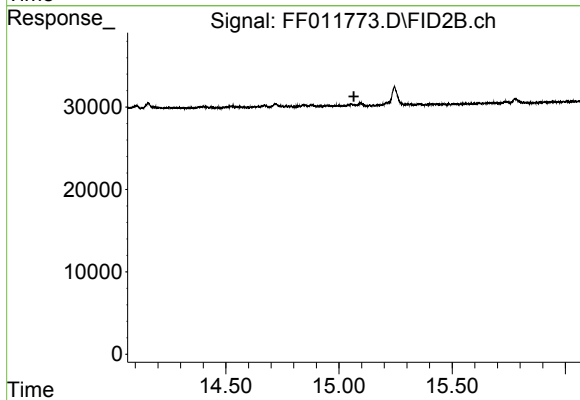

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 15.066 min  
Response: 0  
Conc: N.D.

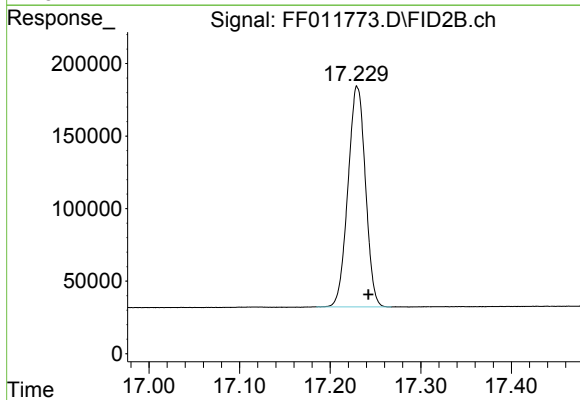

#12 N-OCTACOSANE

R.T.: 17.230 min  
Delta R.T.: -0.012 min  
Response: 2036566  
Conc: 16.52 ug/ml